

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091623\
 Data File : PD078005.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2023 09:51
 Operator : AR\AJ
 Sample : 04330-02
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZYG3

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/19/2023
 Supervised By : Ankita Jodhani 09/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 02:30:39 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.541	2.759	21706580	15628932	8.554	10.575m
2) SA Decachlor...	9.077	7.898	49264826	20989800	15.770m	12.961
Target Compounds						
8) B Heptachlo...	5.685	4.709	40765605	5381632	10.548	2.562 #
10) B trans-Chl...	5.949	4.939	55073325	25278621	14.792m	12.659m
13) MA Dieldrin	6.351	5.347	19071588	26446974	5.095	12.799m#
17) MA 4,4'-DDT	7.005	6.015	74048427	35776511	27.028m	25.313

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091623\
Data File : PD078005.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2023 09:51
Operator : AR\AJ
Sample : 04330-02
Misc :
ALS Vial : 7 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 02:30:39 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

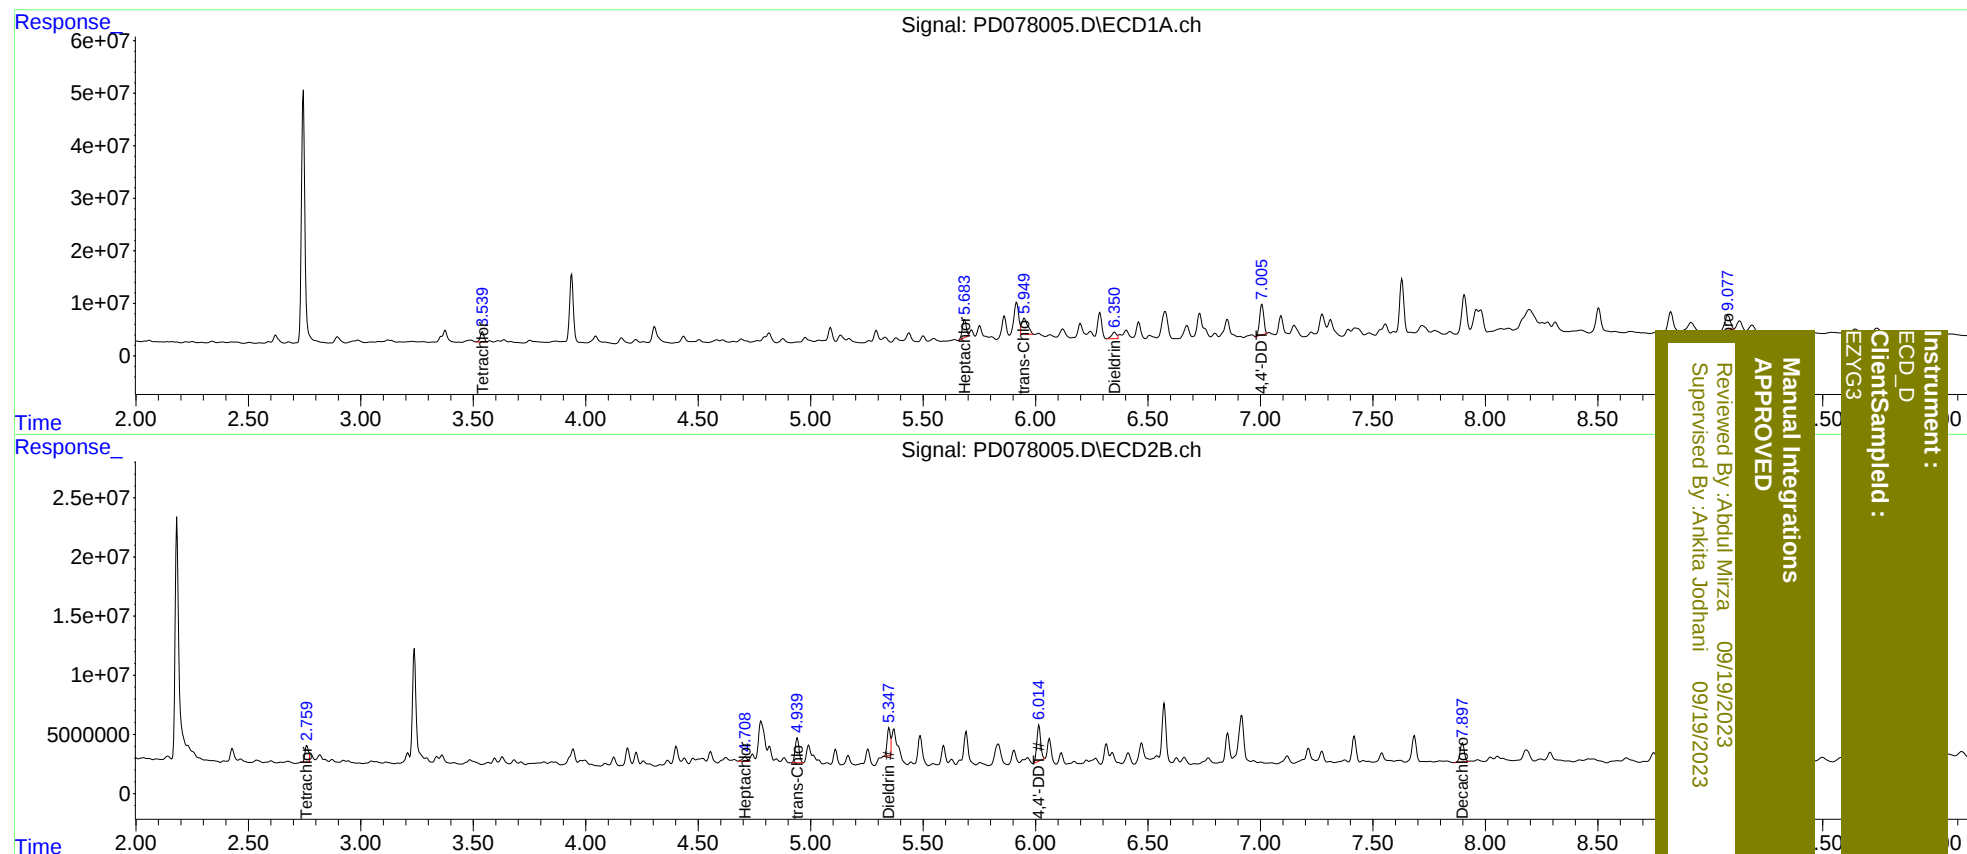

Instrument :
ECD_D
Client Sampled :
EZY63
Manual Integrations
APPROVED
Reviewed By : Abdul Mirza 09/19/2023
Supervised By : Ankita Jodhani 09/19/2023