

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091623\
 Data File : PD078017.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 15 Sep 2023 12:31
 Operator : AR\AJ
 Sample : 04330-18MSD
 Misc :
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 EZYX6MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/18/2023
 Supervised By :Ankita Jodhani 09/19/2023

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 16 02:33:27 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 06 16:40:06 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.541	2.760	41590339	25330368	16.389	17.140
27)	SA Decachlor...	9.084	7.899	56235318	26976909	18.002	16.657
Target Compounds							
2)	A alpha-BHC	3.997	3.261	87763097	53038148	20.497m	23.399
3)	MA gamma-BHC...	4.330	3.590	79868283	49022874	19.754m	22.705
4)	MA Heptachlor	4.921	3.929	81337725	57588771	19.464m	25.903 #
5)	MB Aldrin	5.264	4.209	88732929	53948800	21.255	24.069
6)	B beta-BHC	4.529	3.888	31399785	20536700	17.091	20.784
7)	B delta-BHC	4.777	4.117	75202912	49438640	18.729	22.179
8)	B Heptachlo...	5.692	4.711	75131119	42778643	19.440	20.366
9)	A Endosulfan I	6.080	5.081	62709284	36825284	18.682	20.516
10)	B trans-Chl...	5.948	4.960	74740003	39422317	20.074m	19.741m
11)	B cis-Chlor...	6.029	5.025	66317933	38419152	17.207	18.787
12)	B 4,4'-DDE	6.201	5.214	133.0E6	75518361	37.515	39.754
13)	MA Dieldrin	6.356	5.346	139.9E6	85209152	37.387	41.235
14)	MA Endrin	6.587	5.622	123.6E6	68312949	40.067	37.364
15)	B Endosulfa...	6.806	5.917	124.1E6	78496642	37.495	43.376
16)	A 4,4'-DDD	6.720	5.769	126.3E6	58634500	47.489	43.564
17)	MA 4,4'-DDT	7.036	6.020	126.6E6	64211199	46.203	45.432
18)	B Endrin al...	6.937	6.094	94946299	48365032	36.539	34.383m
19)	B Endosulfa...	7.172	6.318	113.7E6	68901690	37.533	41.702
20)	A Methoxychlor	7.513	6.596	324.6E6	175.9E6	208.096	225.414
21)	B Endrin ke...	7.660	6.825	133.0E6	70181405	38.641	36.629

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091623\
Data File : PD078017.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 15 Sep 2023 12:31
Operator : AR\AJ
Sample : 04330-18MSD
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 16 02:33:27 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090623CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 06 16:40:06 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

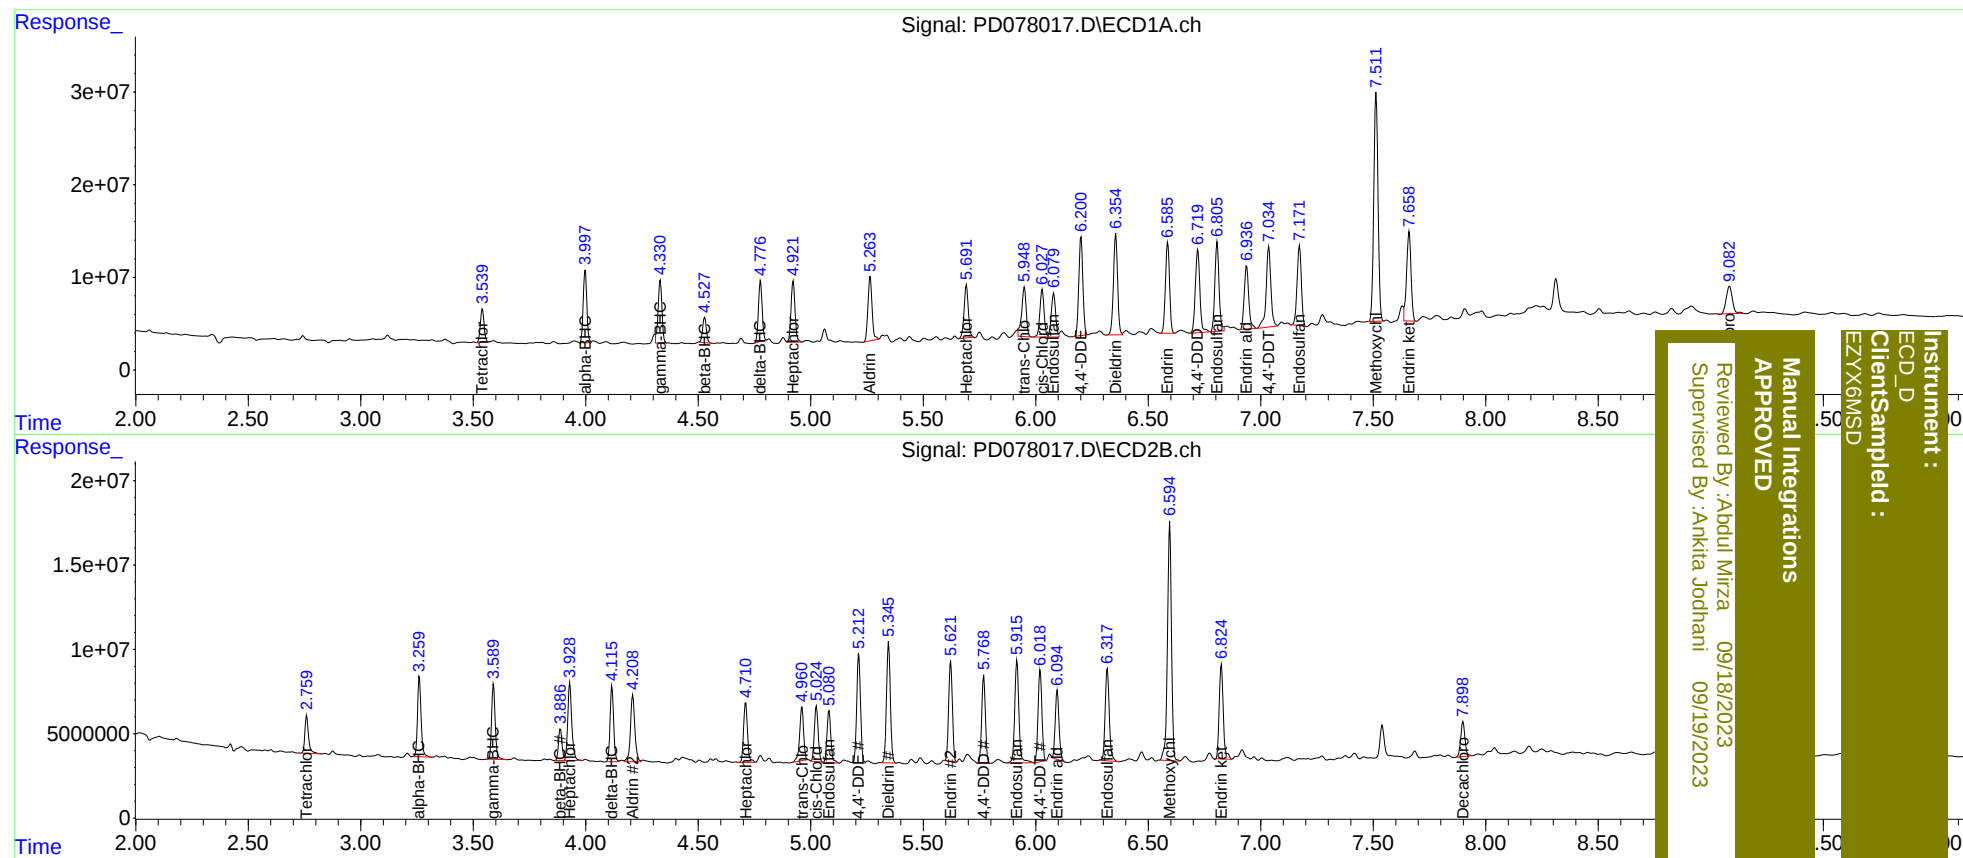

Instrument :
ECD_D
ClientSampled :
EZYX6MSD

Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/18/2023
Supervised By :Ankita Jodhani 09/19/2023