

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091624\
 Data File : PD085227.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2024 17:14
 Operator : AR\AJ
 Sample : P3878-16RE
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDC05RE

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/17/2024
 Supervised By : Ankita Jodhani 09/17/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 02:51:38 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.528	2.914	23830167	1933.8E6	23.561m	546.461m#
2) SA Decachlor...	9.029	8.097	19396459	46863811	14.851m	13.477m
Target Compounds						
2) A alpha-BHC	3.981	3.412	173.2E6	316.2E6	101.847	62.358 #
7) B delta-BHC	4.740	4.277	236.4E6	412.3E6	144.162m	83.050m#
9) A Endosulfan I	6.053	5.278	40339544	89920903	29.321m	23.458
11) B cis-Chlor...	6.010	5.225	52438975	91426247	35.466m	21.791 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091624\
Data File : PD085227.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2024 17:14
Operator : AR\AJ
Sample : P3878-16RE
Misc :
ALS Vial : 29 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 02:51:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

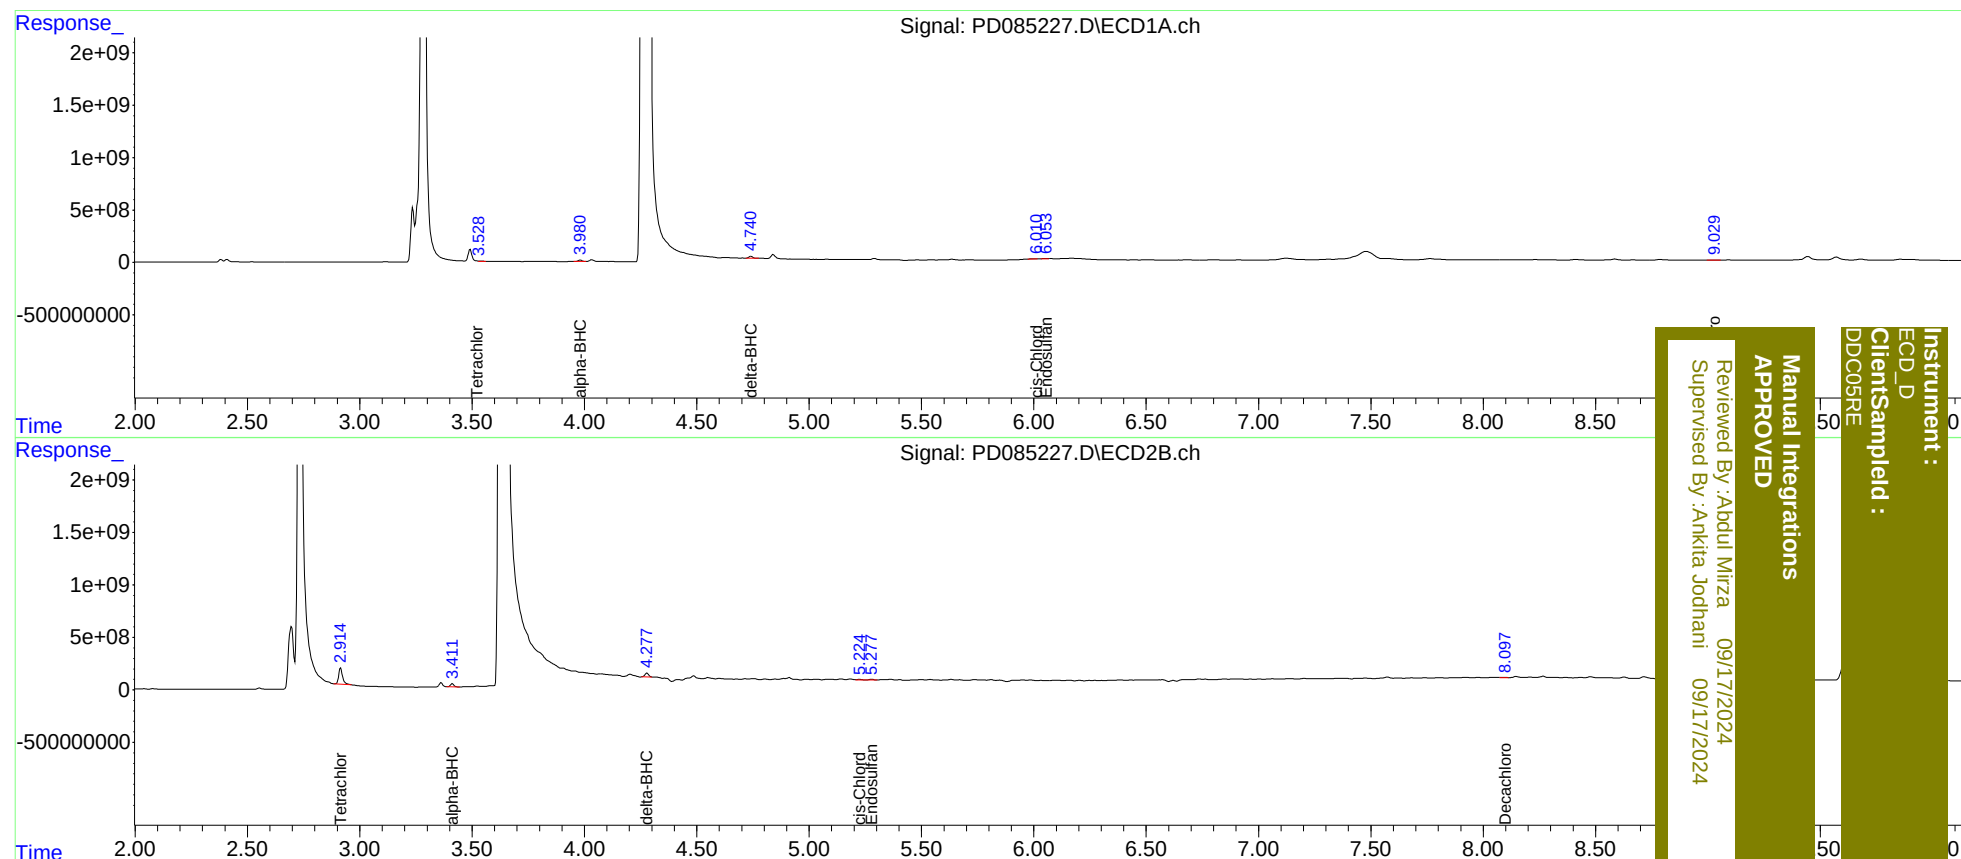

Reviewed By: Abdul Mirza 09/17/2024
Supervised By: Ankita Jodhani 09/17/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
DDC05RE