

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091624\
 Data File : PD085201.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2024 10:19
 Operator : AR\AJ
 Sample : PB163328BS
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS328

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/17/2024
 Supervised By :Ankita Jodhani 09/17/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 02:43:35 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.536	2.902	17538074	65608959	17.340	18.540
2)	SA Decachlor...	9.030	8.100	24720943	72329578	18.928	20.801
Target Compounds							
2)	A alpha-BHC	3.981	3.412	7009006	24790985	4.123	4.890
3)	MA gamma-BHC...	4.309	3.747	7414649	25389302	4.583m	5.239
4)	MA Heptachlor	4.908	4.101	7051699	21999617	4.583	5.168
5)	MB Aldrin	5.248	4.388	7376751	23315770	4.612	5.250
6)	B beta-BHC	4.493	4.040	3140394	11290024	4.323	5.208
7)	B delta-BHC	4.741	4.278	7502117	23791302	4.574	4.793
8)	B Heptachlo...	5.667	4.891	7156832	22162522	4.799	5.233
9)	A Endosulfan I	6.048	5.267	6413839	20584448	4.662m	5.370
10)	B trans-Chl...	5.922	5.145	6705653	22346893	4.755	5.433
11)	B cis-Chlor...	6.001	5.209	6969532	22557861	4.714m	5.377
12)	B 4,4'-DDE	6.171	5.395	10966811	39859547	8.791	10.161
13)	MA Dieldrin	6.322	5.534	12892311	44405543	8.740	10.336
14)	MA Endrin	6.548	5.812	10520898	40208453	9.324	10.860
15)	B Endosulfa...	6.759	6.102	12006756	41335134	9.096	11.148m
16)	A 4,4'-DDD	6.679	5.952	8399729	35127552	8.507	10.351
17)	MA 4,4'-DDT	6.995	6.207	6968956	31710917	7.785	9.913 #
18)	B Endrin al...	6.888	6.282	9499717	32533300	10.519	11.394
19)	B Endosulfa...	7.122	6.505	10852175	38776120	9.420	10.857m
20)	A Methoxychlor	7.466	6.779	22630770	89312274	43.444	53.989
21)	B Endrin ke...	7.602	7.018	11653965	48389431	9.532	10.990

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091624\
Data File : PD085201.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2024 10:19
Operator : AR\AJ
Sample : PB163328BS
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 02:43:35 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

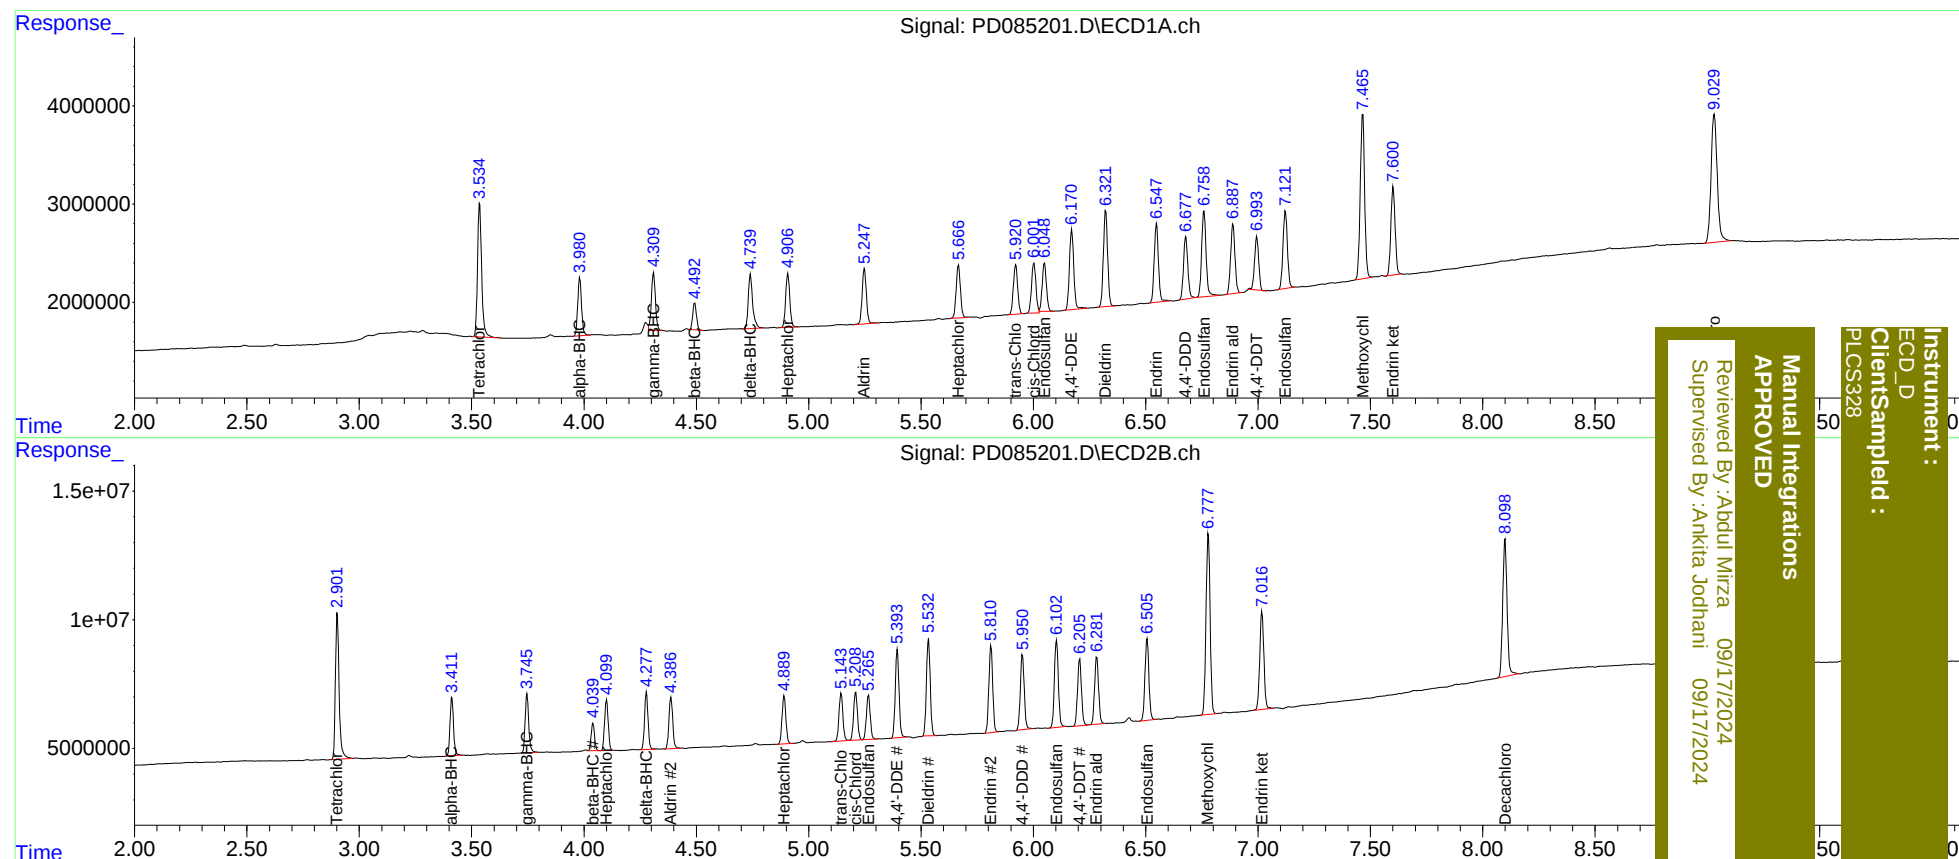

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 09/17/2024
Supervised By: Ankita Jodhani 09/17/2024

Instrument :
ECD_D
Client Sampled :
PLCS328