

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091624\
 Data File : PD085222.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2024 16:08
 Operator : AR\AJ
 Sample : P3898-18RE
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDC91RE

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/17/2024
 Supervised By : Ankita Jodhani 09/17/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 02:49:59 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.533	2.913	14463024	207.0E6	14.300m	58.495m#
2) SA Decachlor...	9.030	8.099	18824896	46724271	14.414m	13.437m
Target Compounds						
2) A alpha-BHC	3.981	3.413	13853659	28208825	8.148	5.564 #
7) B delta-BHC	4.740	4.279	12654105	39924050	7.716m	8.043

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091624\
Data File : PD085222.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2024 16:08
Operator : AR\AJ
Sample : P3898-18RE
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 02:49:59 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

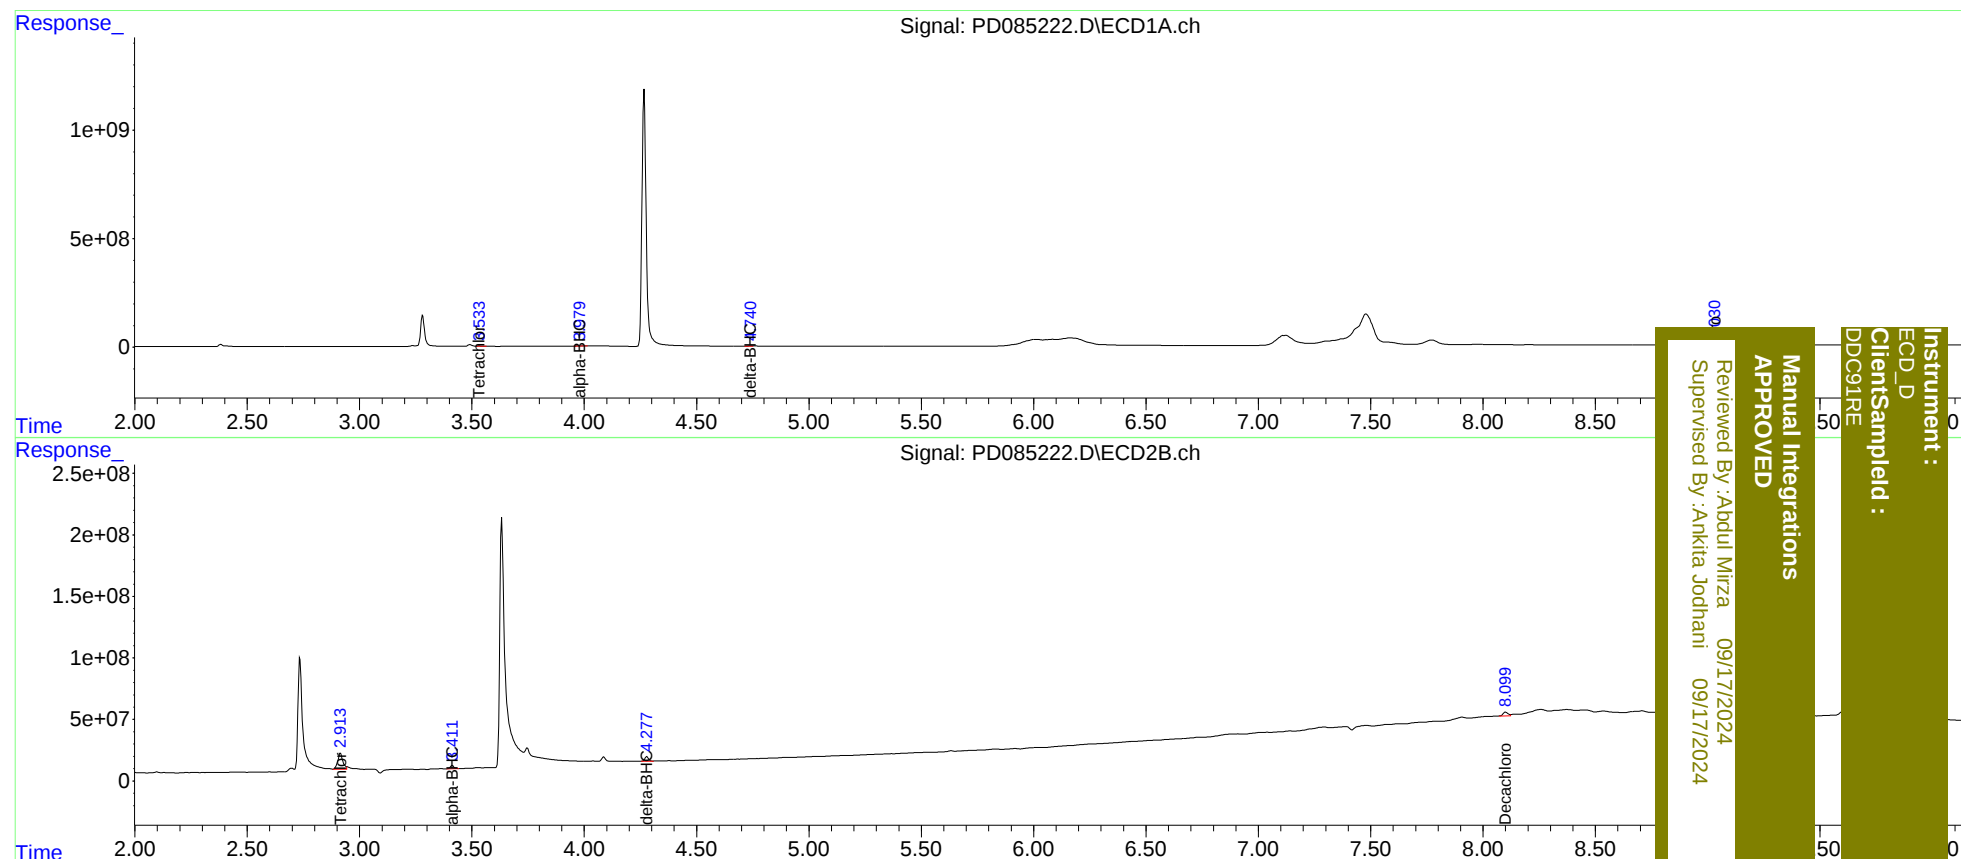

Reviewed By: Abdul Mirza 09/17/2024
Supervised By: Ankita Jodhani 09/17/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
DDC91RE