

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091719\
 Data File : PD054657.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 17 Sep 2019 15:50
 Operator : SG\AJ
 Sample : PIBLK15
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK15

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 03:50:30 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091619CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Sep 17 05:19:07 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.295	3.966	16758986	18541968	18.441	19.138
27) SA Decachlor...	7.977	9.004	35623812	37282395	32.648	33.287
Target Compounds						
8) B Heptachlo...	0.000	5.824	0	9040745	N.D.	6.657


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091719\
Data File : PD054657.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 17 Sep 2019 15:50
Operator : SG\AJ
Sample : PIBLK15
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK15

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 03:50:30 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091619CLP.M
Quant Title : GC Extractables
QLast Update : Tue Sep 17 05:19:07 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

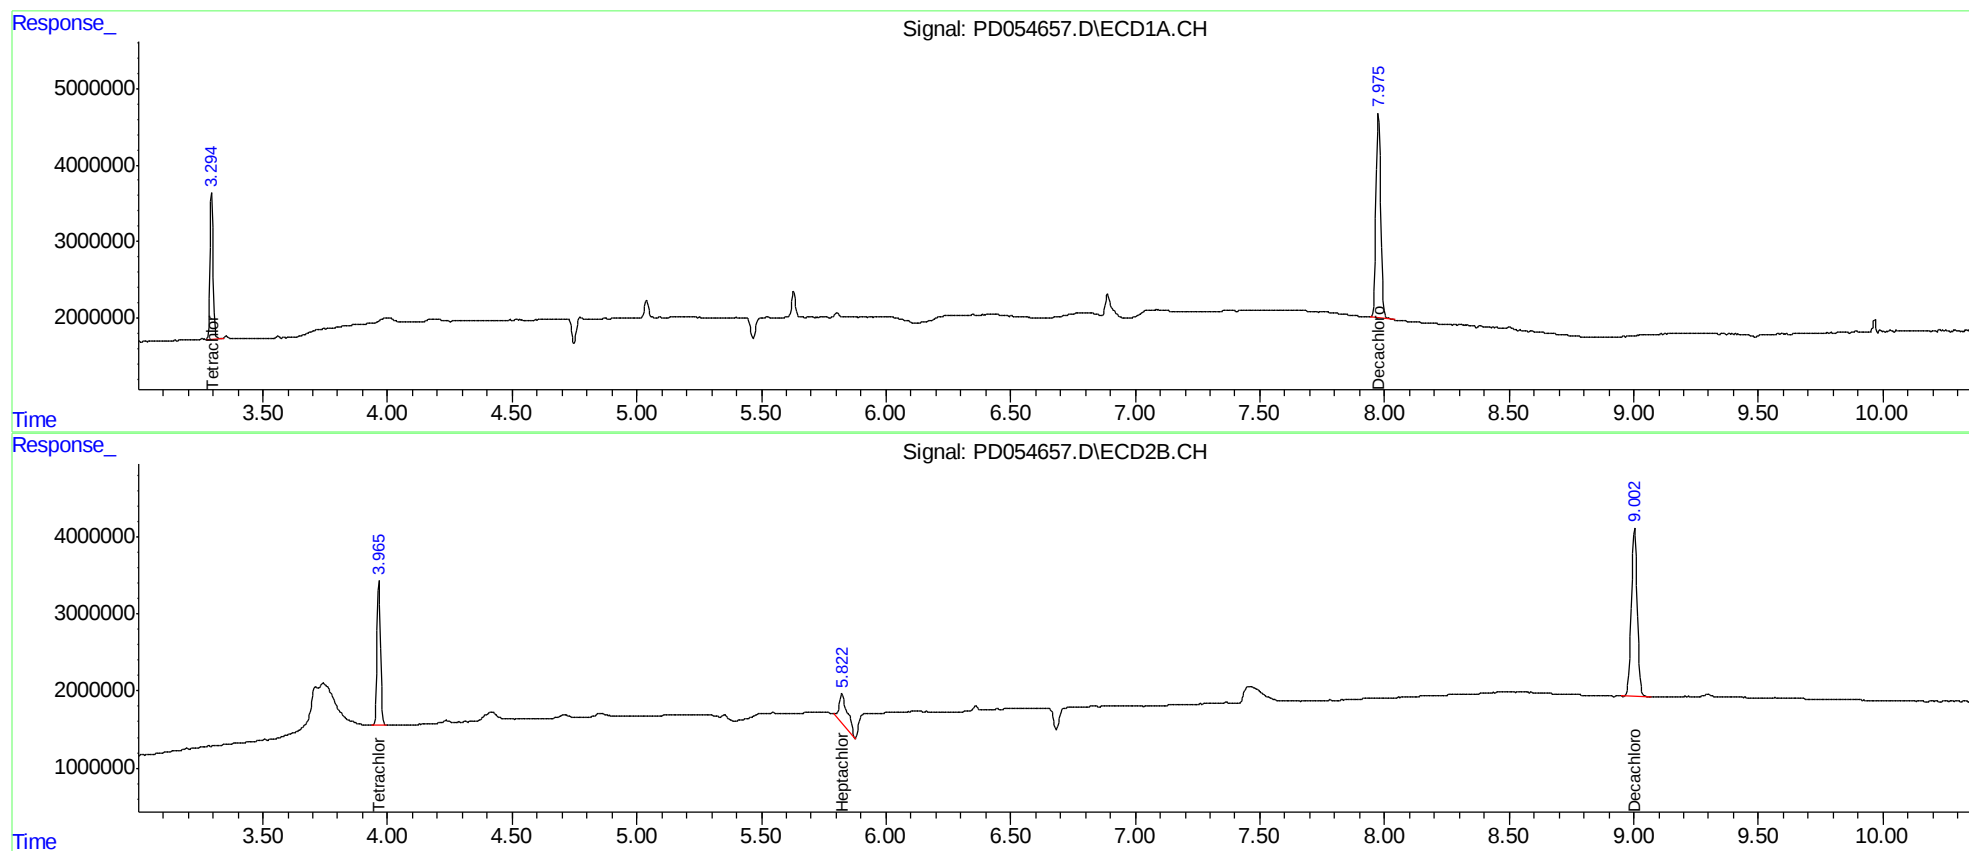


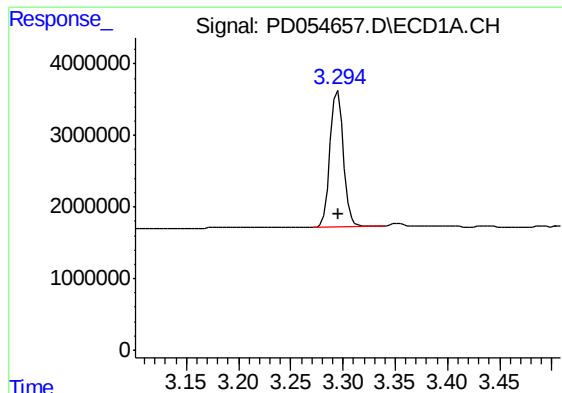

#1 Tetrachloro-m-xylene


R.T.: 3.295 min
Delta R.T.: 0.000 min
Response: 16758986
Conc: 18.44 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK15

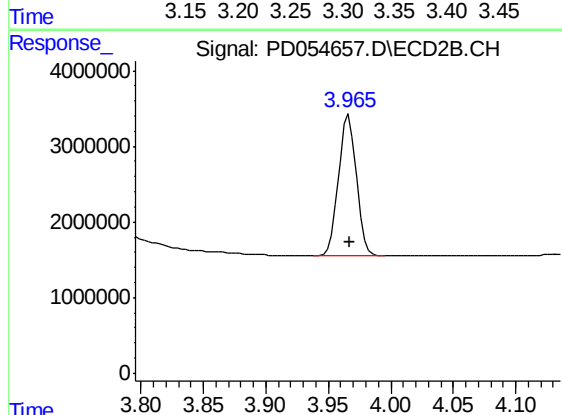


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: 0.000 min
Response: 18541968
Conc: 19.14 ng/ml

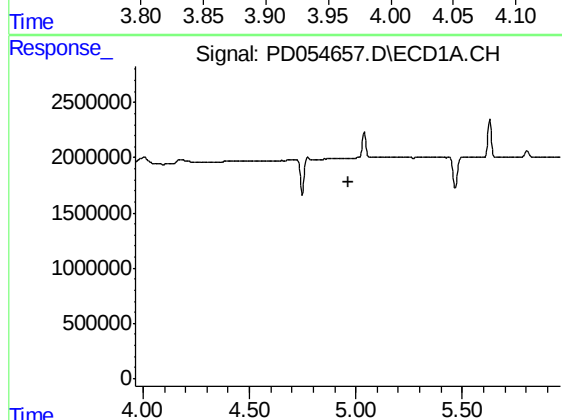


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.964 min
Response: 0
Conc: N.D.

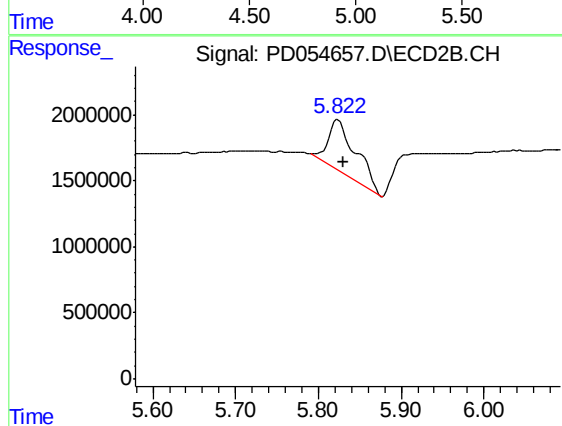

#8 Heptachlor epoxide


R.T.: 5.824 min
Delta R.T.: -0.007 min
Response: 9040745
Conc: 6.66 ng/ml

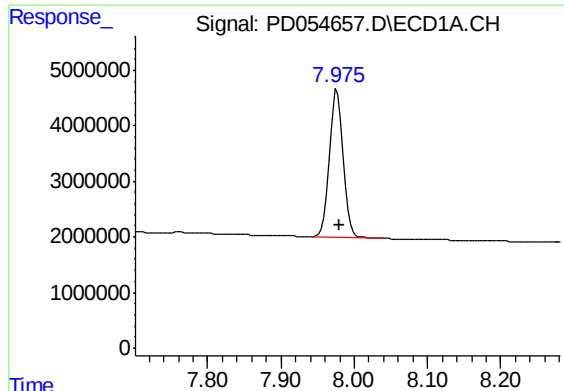

#27 Decachlorobiphenyl

R.T.: 7.977 min
Delta R.T.: -0.003 min
Response: 35623812
Conc: 32.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK15

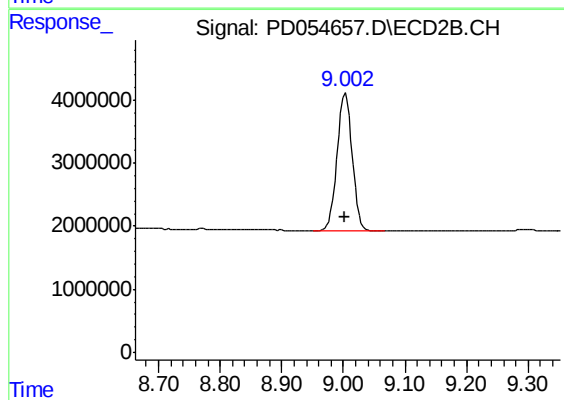

#27 Decachlorobiphenyl

R.T.: 9.004 min
Delta R.T.: 0.000 min
Response: 37282395
Conc: 33.29 ng/ml