

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091720\
 Data File : PD059234.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2020 08:25
 Operator : DD\AJ
 Sample : I.BLK
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 I.BLK

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 01:18:40 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091620.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 16 03:41:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.206	3.864	20455871	39631275	22.696	23.458
28)	SA Decachlor...	7.839	8.858	21342953	34371797	22.910	21.972
Target Compounds							
8)	B Heptachlo...	0.000	5.708	0	2946942	N.D.	1.441 #



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091720\
Data File : PD059234.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2020 08:25
Operator : DD\AJ
Sample : I.BLK
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
I.BLK

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 01:18:40 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091620.M
Quant Title : GC Extractables
QLast Update : Wed Sep 16 03:41:41 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

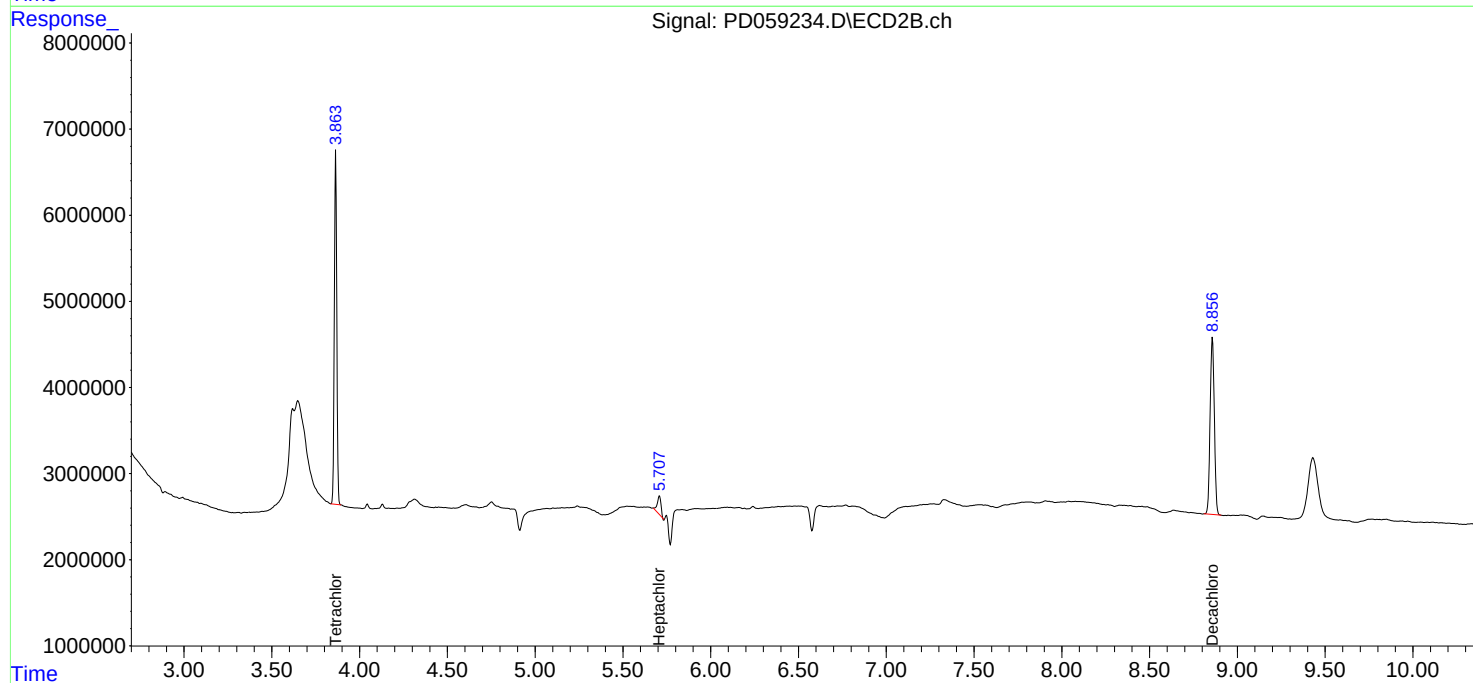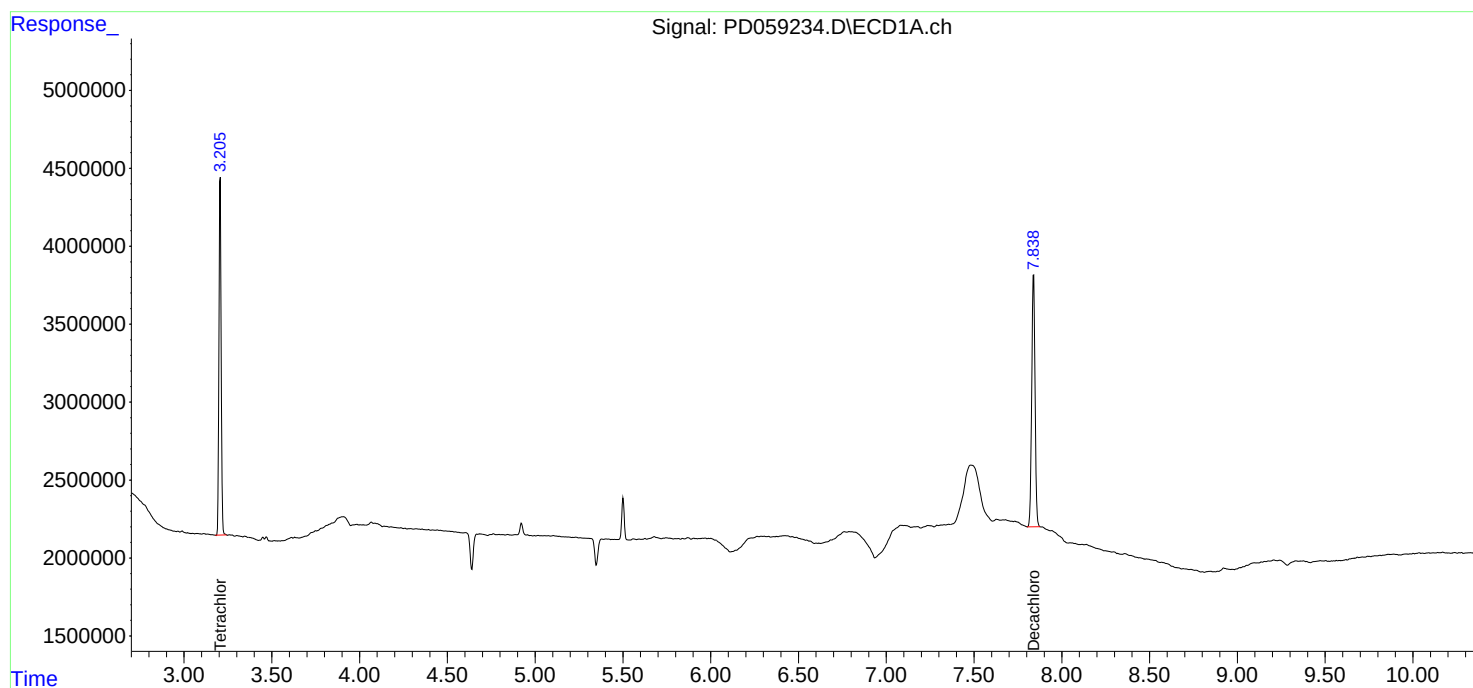


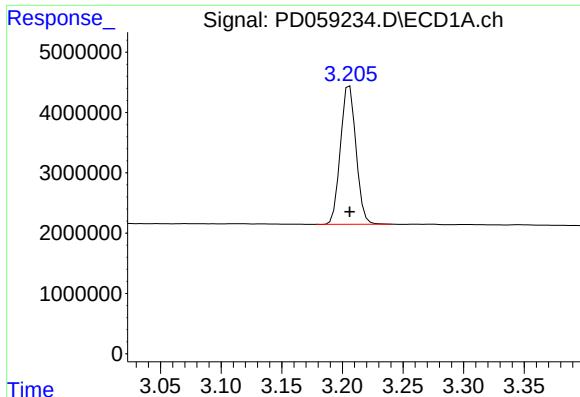

#1 Tetrachloro-m-xylene


R.T.: 3.206 min
Delta R.T.: 0.000 min
Response: 20455871
Conc: 22.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

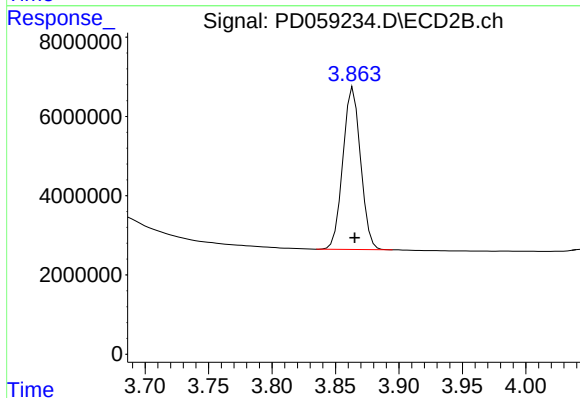


#1 Tetrachloro-m-xylene

R.T.: 3.864 min
Delta R.T.: -0.001 min
Response: 39631275
Conc: 23.46 ng/ml

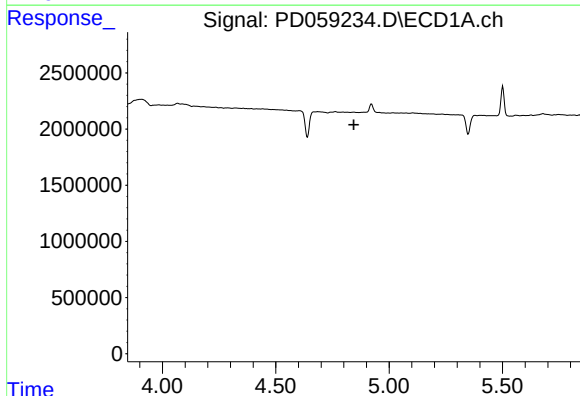


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.844 min
Response: 0
Conc: N.D.

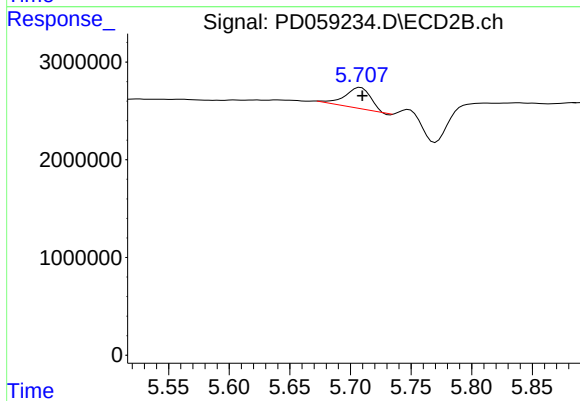

#8 Heptachlor epoxide


R.T.: 5.708 min
Delta R.T.: -0.002 min
Response: 2946942
Conc: 1.44 ng/ml

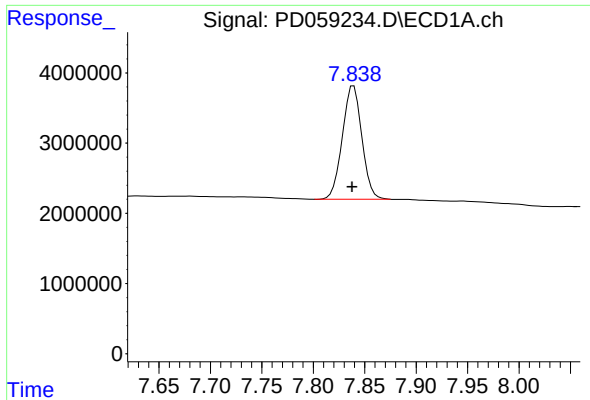

#28 Decachlorobiphenyl

R.T.: 7.839 min
Delta R.T.: 0.001 min
Response: 21342953
Conc: 22.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
I.BLK

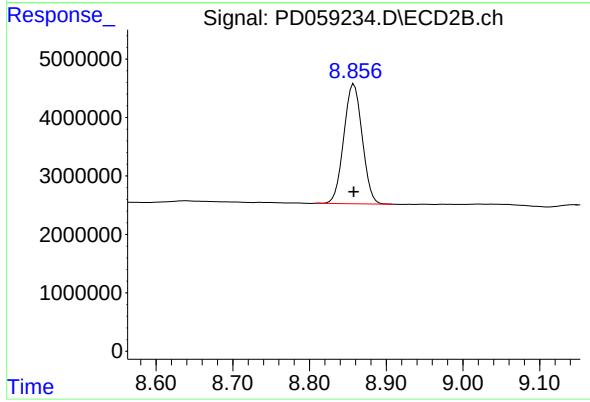

#28 Decachlorobiphenyl

R.T.: 8.858 min
Delta R.T.: 0.000 min
Response: 34371797
Conc: 21.97 ng/ml