

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091720\
 Data File : PD059255.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2020 14:39
 Operator : DD\AJ
 Sample : L3971-13DL 10X
 Misc :
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PT-TXP-WPDL

Manual Integrations
 APPROVED

Ankita
 9/17/2020 1:52:48 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 01:25:41 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX091620.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 16 04:05:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.206	3.865	1830113	3442915	2.043	2.027
7) SA Decachlor...	7.838	8.858	2097877	4468442	2.249	2.810
Target Compounds						
2) Toxaphene-1	5.589	6.409	6608906	12169222	660.816	658.131m
3) Toxaphene-2	5.964	6.703	10422597	14512635	660.330	686.801
4) Toxaphene-3	6.206	6.990	10891059	30695539	691.841	698.691
5) Toxaphene-4	6.341	7.074	4760491	18938476	711.529	683.302
6) Toxaphene-5	6.622	7.486	4244214	13829681	728.246	644.679

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091720\
Data File : PD059255.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2020 14:39
Operator : DD\AJ
Sample : L3971-13DL 10X
Misc :
ALS Vial : 21 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 01:25:41 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX091620.M
Quant Title : GC Extractables
QLast Update : Wed Sep 16 04:05:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

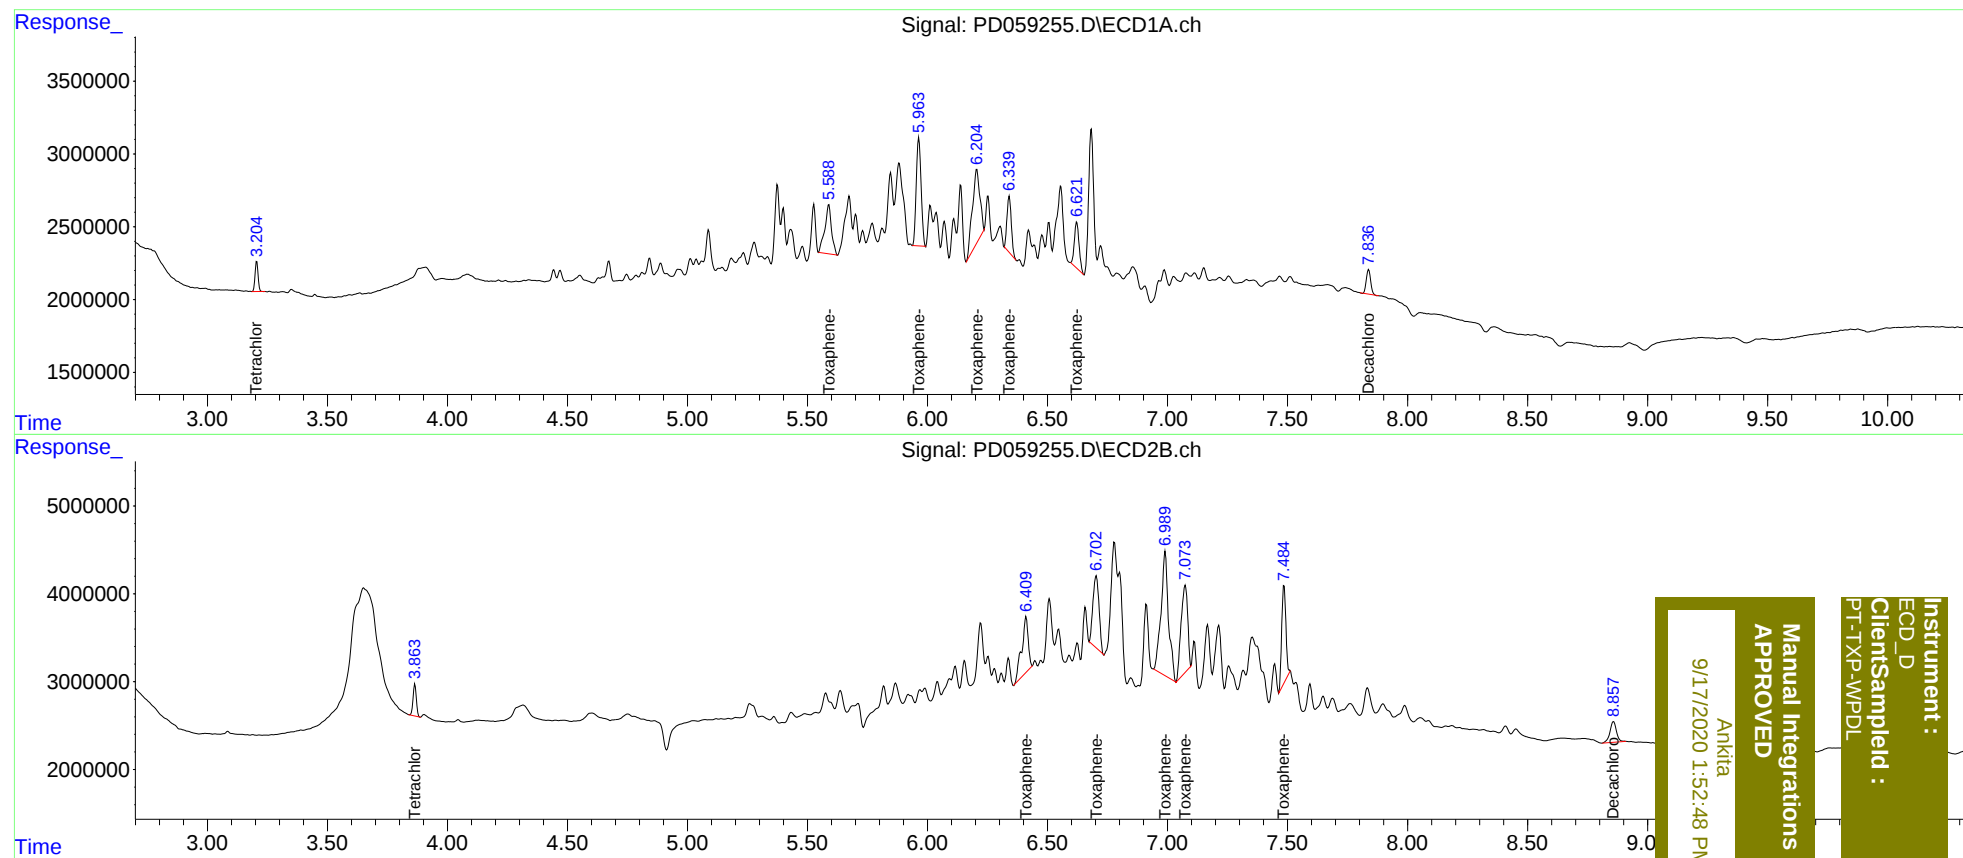

Manual Integrations
APPROVED

Ankita

9/17/2020 1:52:48 PM

Instrument :
ECD_D
ClientSampled :
PT-TXP-W/PDL