

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091720\
 Data File : PD059258.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2020 15:48
 Operator : DD\AJ
 Sample : PTOXCCC500
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PTOXCCC500

Manual Integrations
 APPROVED

Ankita
 9/17/2020 1:52:50 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 01:25:52 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX091620.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 16 04:05:05 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.212	3.866	42847222	80986814	47.843	47.671
7) SA Decachlor...	7.847	8.863	44142881	72050944	47.313	45.311
Target Compounds						
2) Toxaphene-1	5.598	6.414	4871931	8968067	487.138	485.007m
3) Toxaphene-2	5.973	6.708	7597915	9902963	481.370	468.651
4) Toxaphene-3	6.215	6.995	7807619	21481922	495.969	488.971
5) Toxaphene-4	6.348	7.078	2834507	12957880	423.661m	467.522
6) Toxaphene-5	6.630	7.489	2882865	9902245	494.658m	461.599

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091720\
Data File : PD059258.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2020 15:48
Operator : DD\AJ
Sample : PTOXCCC500
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 01:25:52 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\DTX091620.M
Quant Title : GC Extractables
QLast Update : Wed Sep 16 04:05:05 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

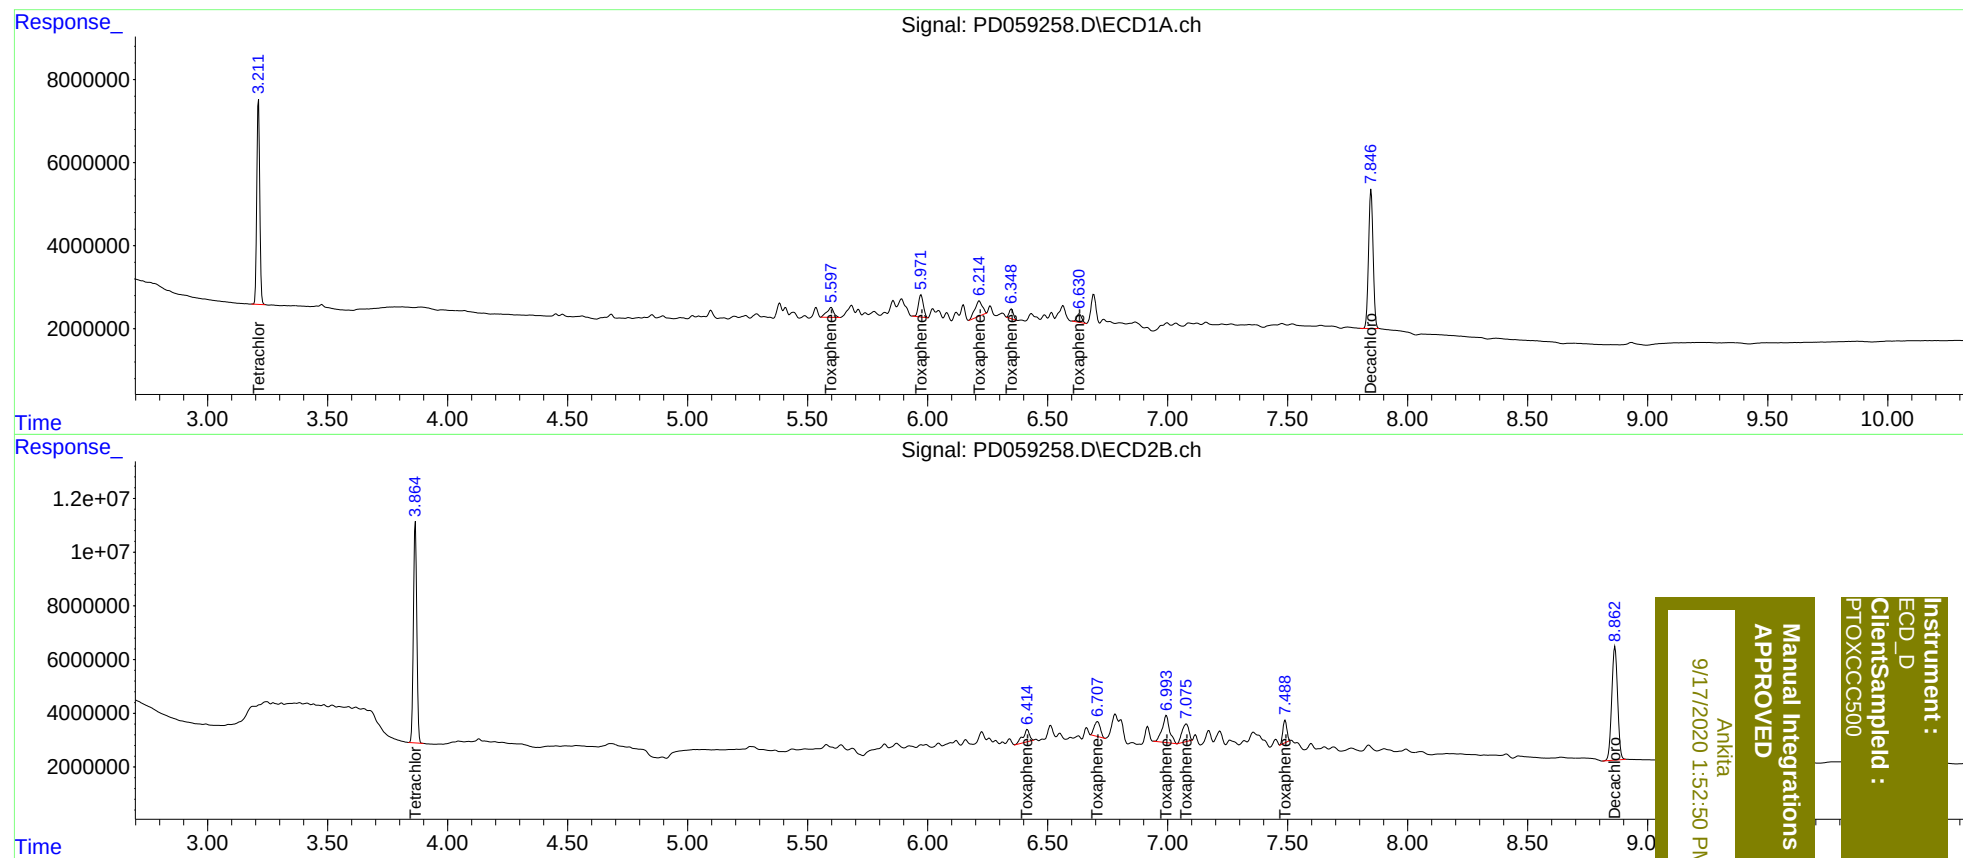

Manual Integrations
APPROVED

Ankita
9/17/2020 1:52:50 PM

Instrument :
ECD_D
Client Sampled :
PTOXCCC500