

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091720\
 Data File : PD059244.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2020 11:48
 Operator : DD\AJ
 Sample : L3971-11DL 2X
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PT-CHLR-WPDL

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 01:20:47 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091620.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 16 03:41:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.203	3.865	17100697	19362838	18.973	11.461 #
28)	SA Decachlor...	7.838	8.858	8401616	18790273	9.019	12.012 #
Target Compounds							
23)	Chlordane-1	4.033	4.841	27229988	60155617	943.906	857.525
24)	Chlordane-2	4.516	5.304	29938032	61515671	868.650	855.607
25)	Chlordane-3	5.064	5.943	106.7E6	252.8E6	1044.951	947.085
26)	Chlordane-4	5.119	6.016	95261185	290.0E6	979.875	904.566
27)	Chlordane-5	5.935	6.814	29286196	52821400	861.312	922.090



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091720\
Data File : PD059244.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2020 11:48
Operator : DD\AJ
Sample : L3971-11DL 2X
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WPDL

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 01:20:47 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091620.M
Quant Title : GC Extractables
QLast Update : Wed Sep 16 03:41:41 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

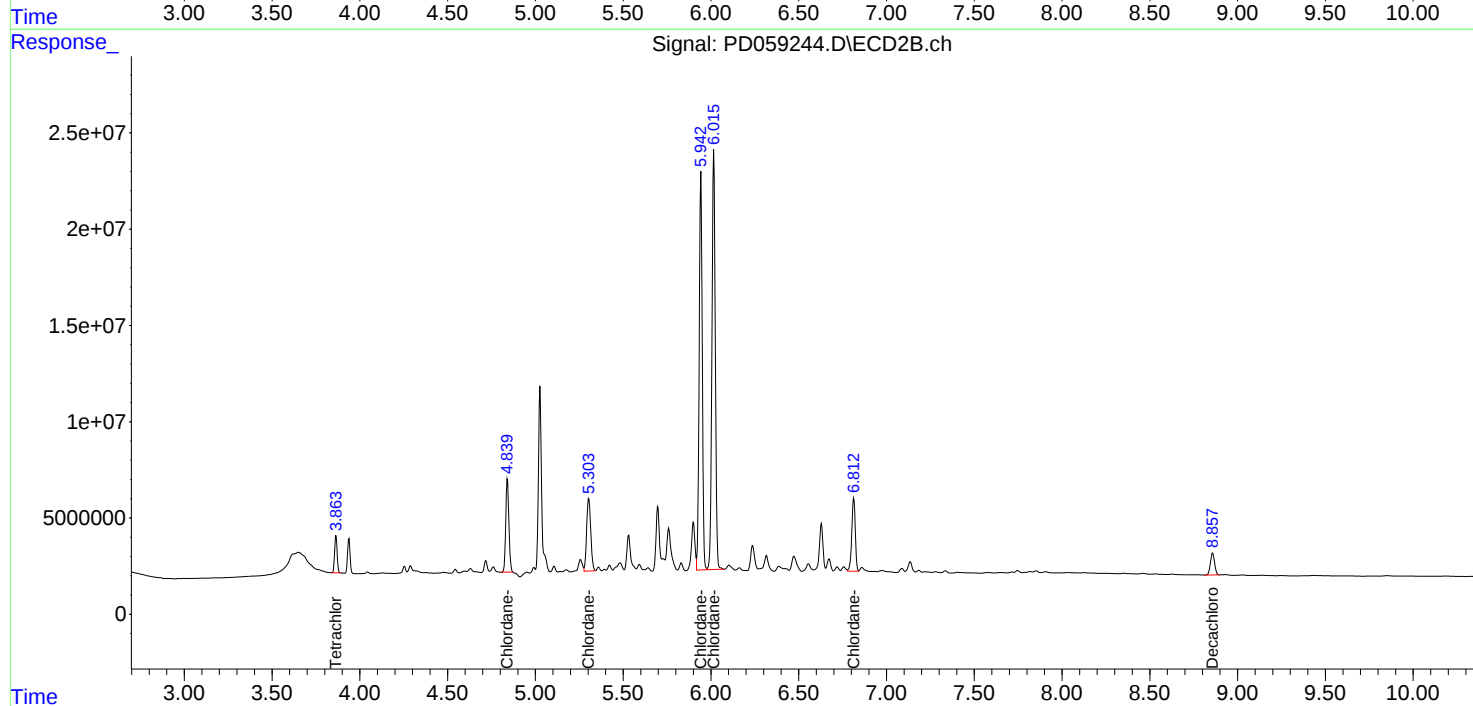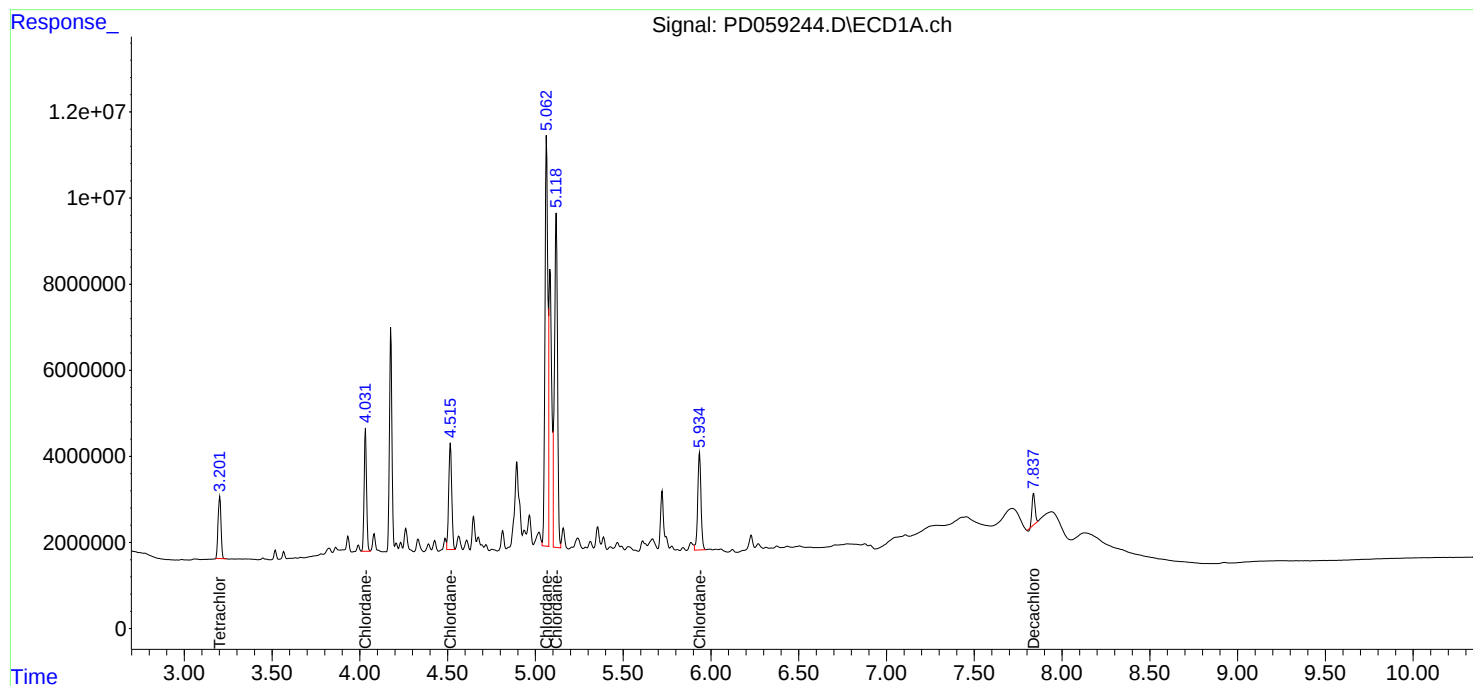


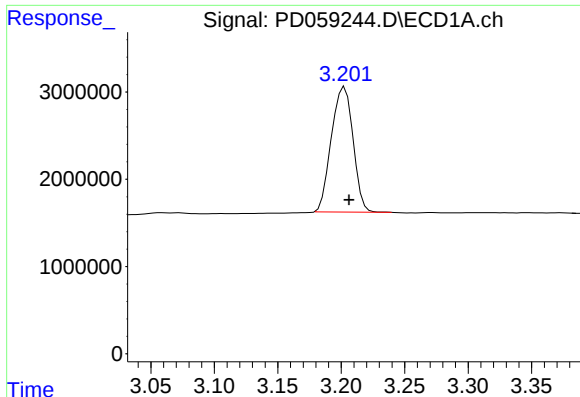

#1 Tetrachloro-m-xylene


R.T.: 3.203 min
Delta R.T.: -0.003 min
Response: 17100697
Conc: 18.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WPDL

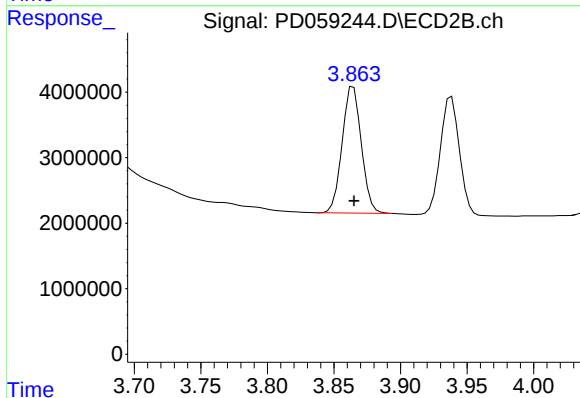


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 19362838
Conc: 11.46 ng/ml

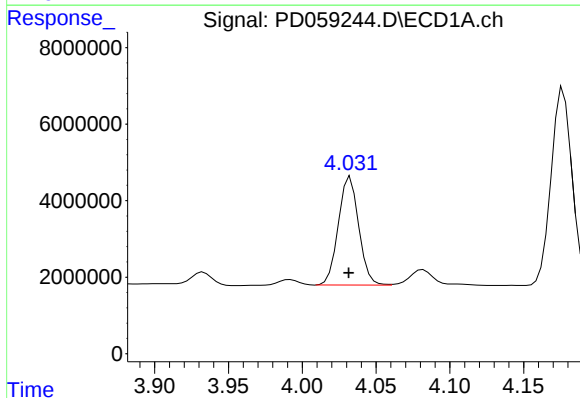


#23 Chlordane-1

R.T.: 4.033 min
Delta R.T.: 0.001 min
Response: 27229988
Conc: 943.91 ng/ml

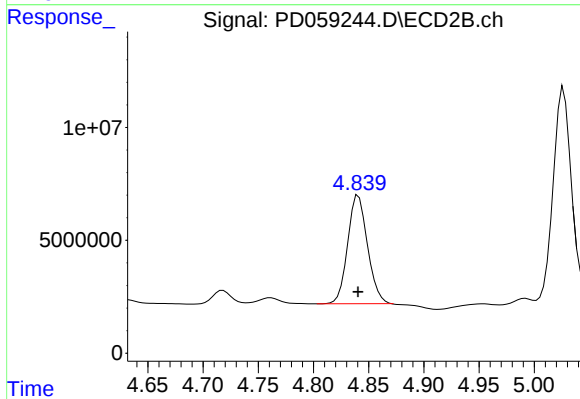

#23 Chlordane-1


R.T.: 4.841 min
Delta R.T.: 0.000 min
Response: 60155617
Conc: 857.53 ng/ml

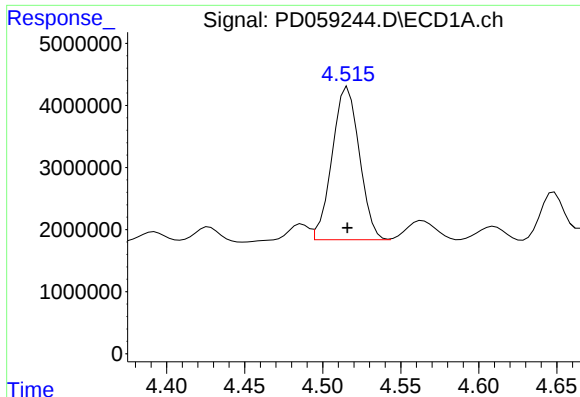

#24 Chlordane-2


R.T.: 4.516 min
Delta R.T.: 0.000 min
Response: 29938032
Conc: 868.65 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WPDL

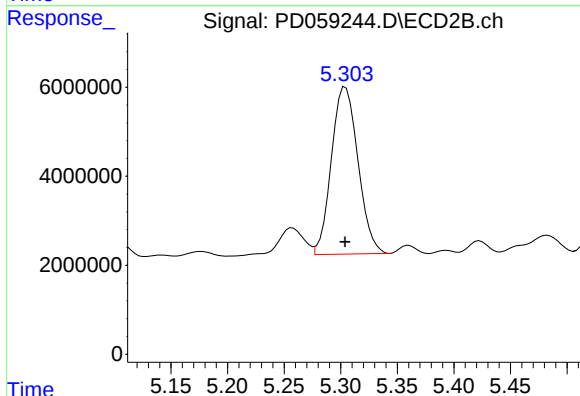


#24 Chlordane-2

R.T.: 5.304 min
Delta R.T.: 0.000 min
Response: 61515671
Conc: 855.61 ng/ml

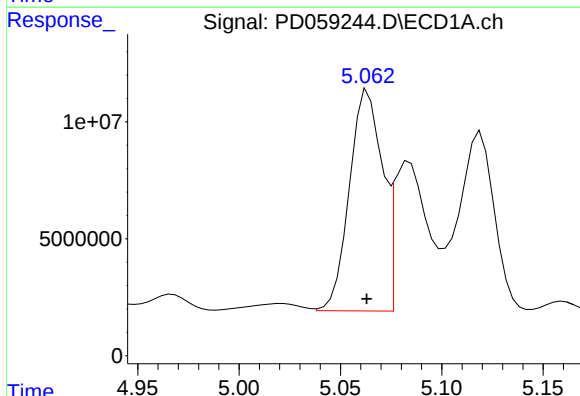


#25 Chlordane-3

R.T.: 5.064 min
Delta R.T.: 0.000 min
Response: 106664754
Conc: 1044.95 ng/ml

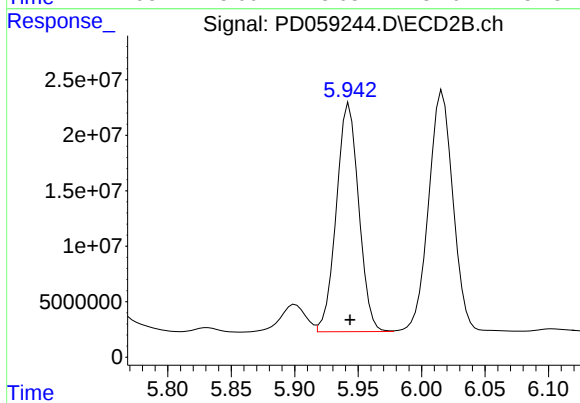

#25 Chlordane-3


R.T.: 5.943 min
Delta R.T.: 0.000 min
Response: 252829448
Conc: 947.09 ng/ml

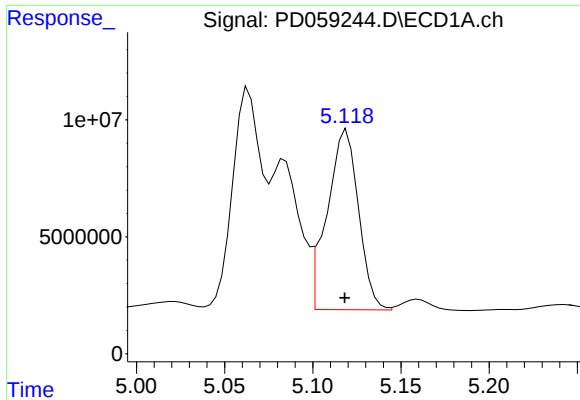

#26 Chlordane-4


R.T.: 5.119 min
Delta R.T.: 0.001 min
Response: 95261185
Conc: 979.88 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WPDL

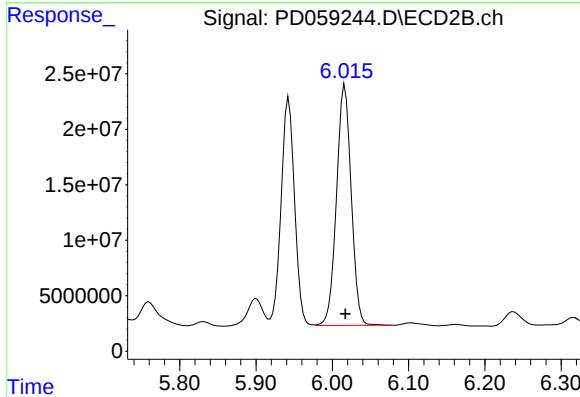


#26 Chlordane-4

R.T.: 6.016 min
Delta R.T.: 0.000 min
Response: 289988547
Conc: 904.57 ng/ml

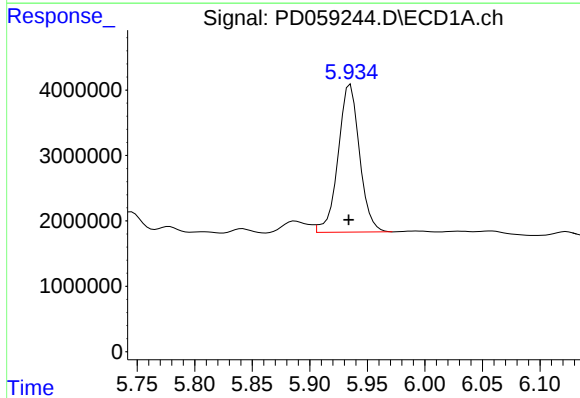


#27 Chlordane-5

R.T.: 5.935 min
Delta R.T.: 0.001 min
Response: 29286196
Conc: 861.31 ng/ml

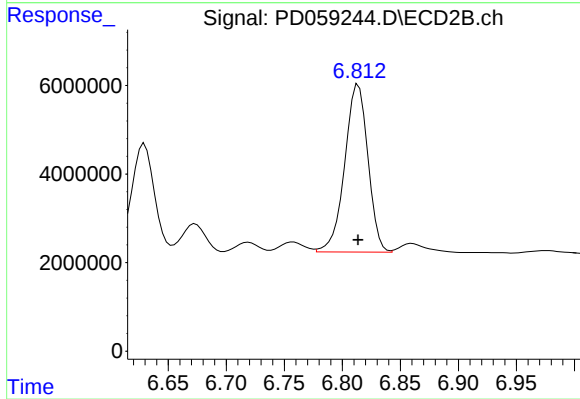

#27 Chlordane-5


R.T.: 6.814 min
Delta R.T.: 0.000 min
Response: 52821400
Conc: 922.09 ng/ml

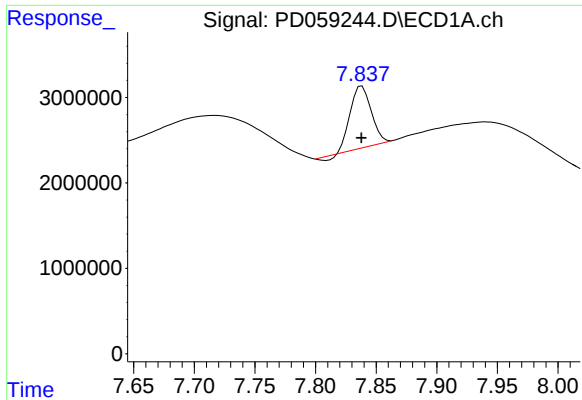

#28 Decachlorobiphenyl

R.T.: 7.838 min
Delta R.T.: 0.000 min
Response: 8401616
Conc: 9.02 ng/ml

Instrument :
ECD_D
ClientSampleId :
PT-CHLR-WPDL

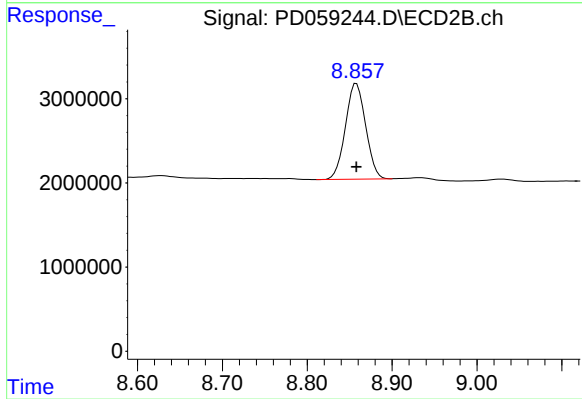

#28 Decachlorobiphenyl

R.T.: 8.858 min
Delta R.T.: 0.000 min
Response: 18790273
Conc: 12.01 ng/ml