

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091720\
 Data File : PD059249.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2020 13:12
 Operator : DD\AJ
 Sample : PCHLORCCC500
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORCCC500

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 01:21:46 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091620.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 16 03:41:41 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.205	3.864	49698035	85532046	55.141	50.627
28)	SA Decachlor...	7.837	8.858	45962823	73376158	49.338	46.906
Target Compounds							
23)	Chlordane-1	4.032	4.841	14576540	30944096	505.284	441.112
24)	Chlordane-2	4.516	5.304	16448191	33379122	477.243	464.262
25)	Chlordane-3	5.064	5.944	49958342	132.6E6	489.421	496.771
26)	Chlordane-4	5.119	6.017	47589942	157.8E6	489.520	492.373
27)	Chlordane-5	5.934	6.814	17051512	28395129	501.488	495.686



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091720\
Data File : PD059249.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2020 13:12
Operator : DD\AJ
Sample : PCHLORCCC500
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 01:21:46 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091620.M
Quant Title : GC Extractables
QLast Update : Wed Sep 16 03:41:41 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

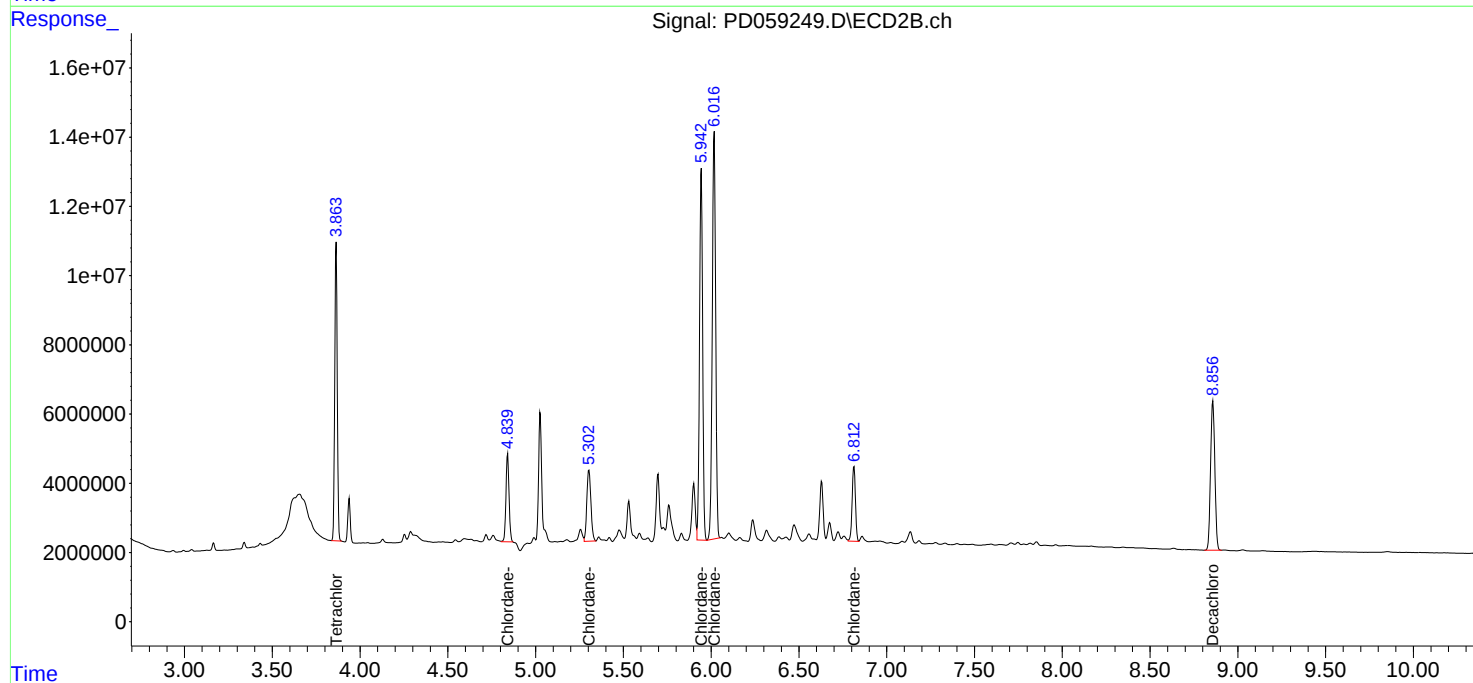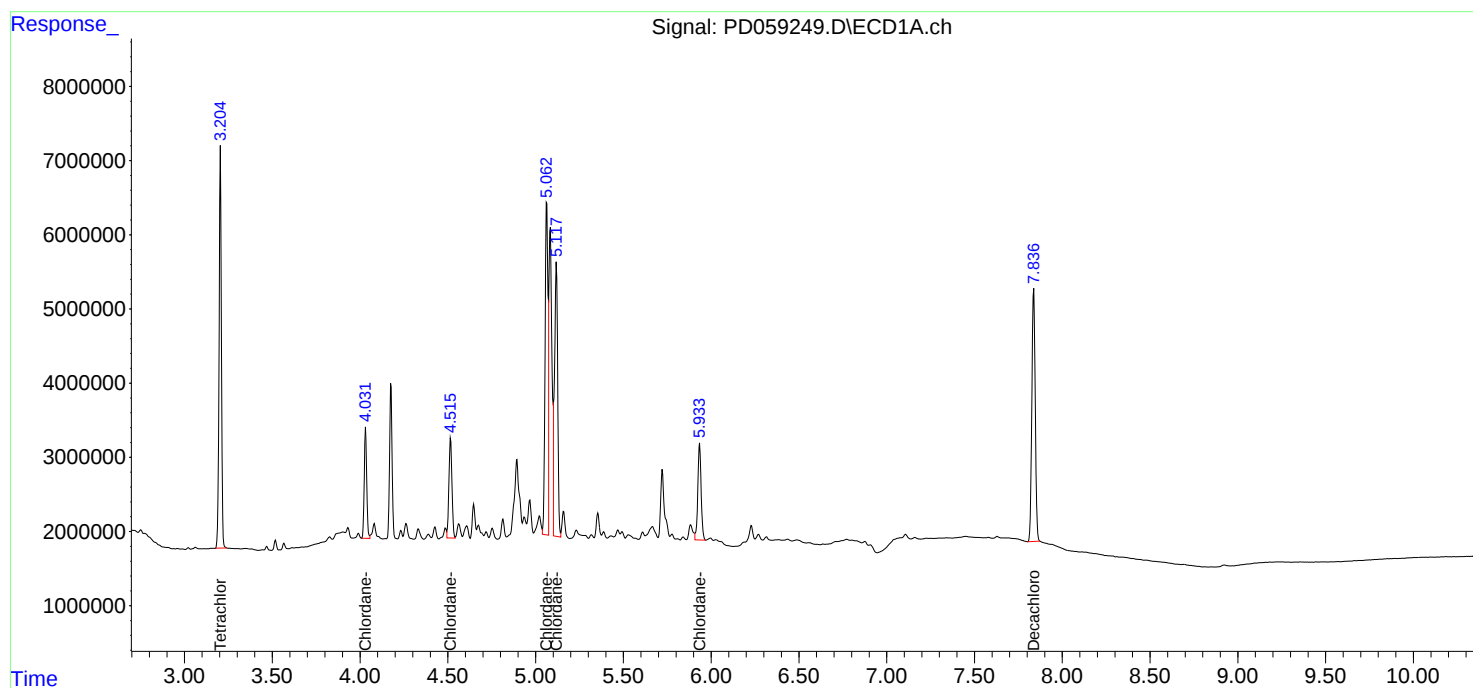


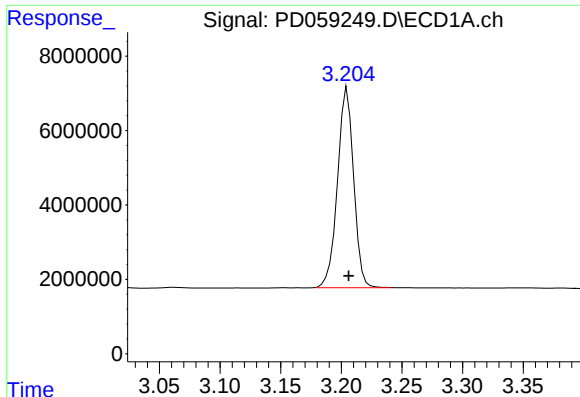

#1 Tetrachloro-m-xylene


R.T.: 3.205 min
Delta R.T.: 0.000 min
Response: 49698035
Conc: 55.14 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

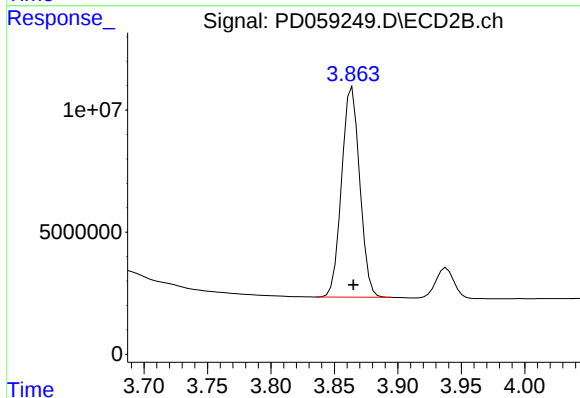


#1 Tetrachloro-m-xylene

R.T.: 3.864 min
Delta R.T.: 0.000 min
Response: 85532046
Conc: 50.63 ng/ml

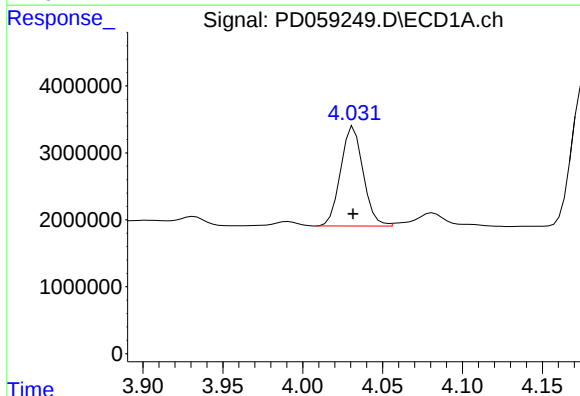


#23 Chlordane-1

R.T.: 4.032 min
Delta R.T.: 0.000 min
Response: 14576540
Conc: 505.28 ng/ml

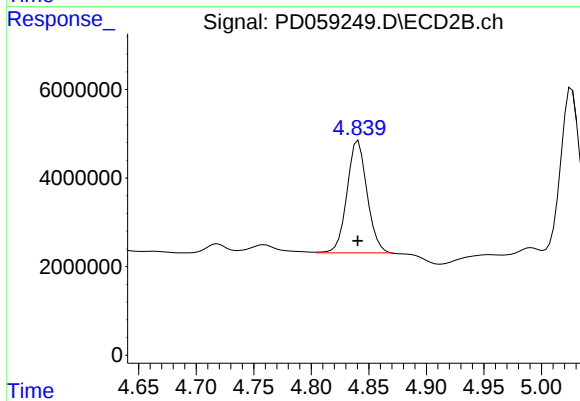

#23 Chlordane-1


R.T.: 4.841 min
Delta R.T.: 0.000 min
Response: 30944096
Conc: 441.11 ng/ml

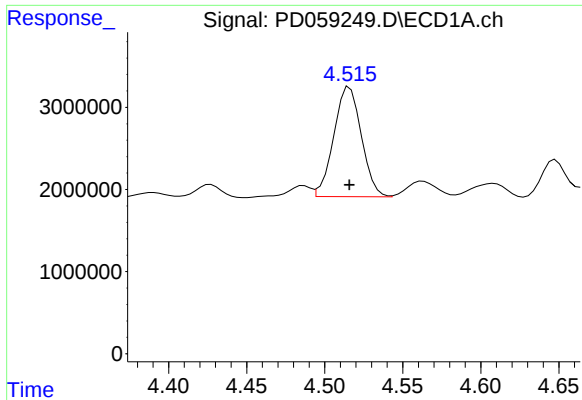

#24 Chlordane-2


R.T.: 4.516 min
Delta R.T.: 0.000 min
Response: 16448191
Conc: 477.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

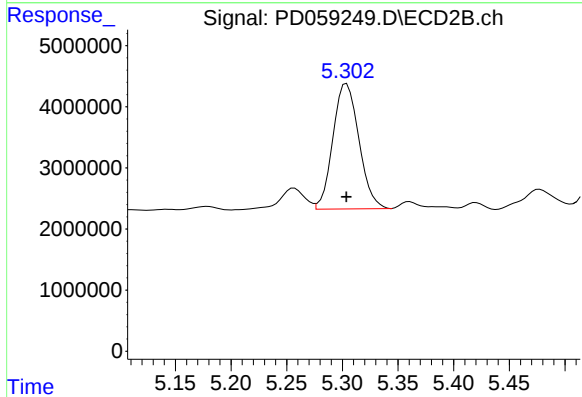


#24 Chlordane-2

R.T.: 5.304 min
Delta R.T.: 0.000 min
Response: 33379122
Conc: 464.26 ng/ml

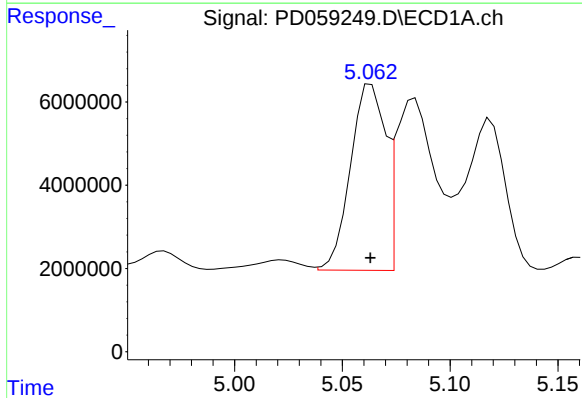


#25 Chlordane-3

R.T.: 5.064 min
Delta R.T.: 0.000 min
Response: 49958342
Conc: 489.42 ng/ml

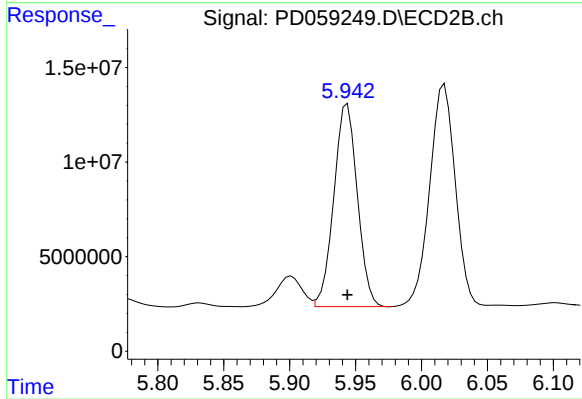

#25 Chlordane-3


R.T.: 5.944 min
Delta R.T.: 0.000 min
Response: 132615679
Conc: 496.77 ng/ml

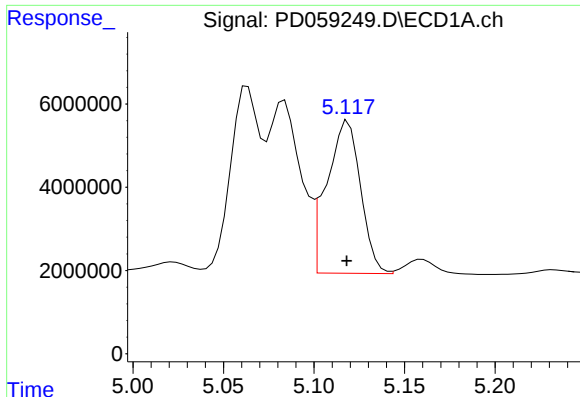

#26 Chlordane-4


R.T.: 5.119 min
Delta R.T.: 0.000 min
Response: 47589942
Conc: 489.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

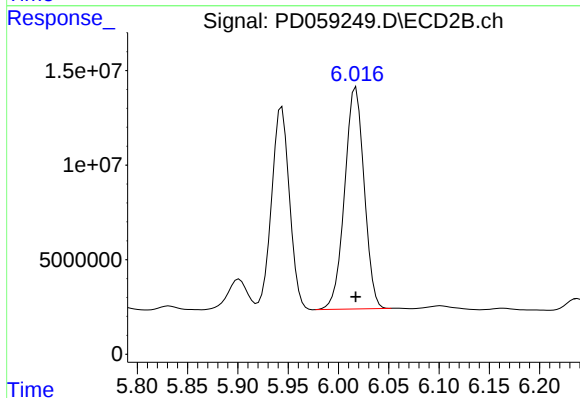


#26 Chlordane-4

R.T.: 6.017 min
Delta R.T.: 0.000 min
Response: 157846381
Conc: 492.37 ng/ml

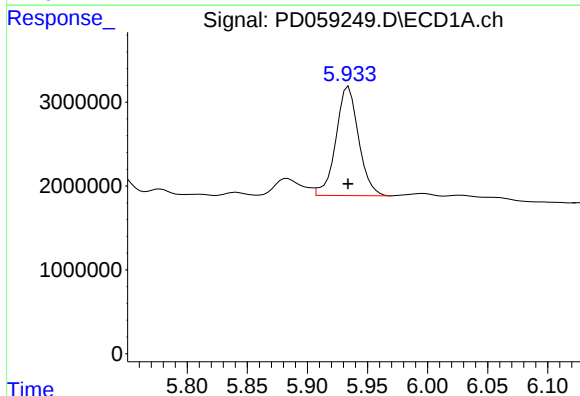


#27 Chlordane-5

R.T.: 5.934 min
Delta R.T.: 0.000 min
Response: 17051512
Conc: 501.49 ng/ml

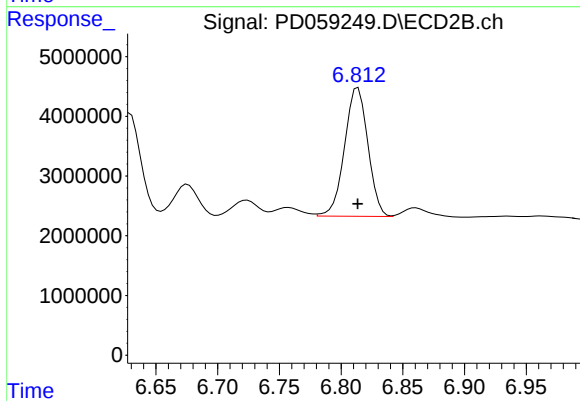

#27 Chlordane-5


R.T.: 6.814 min
Delta R.T.: 0.000 min
Response: 28395129
Conc: 495.69 ng/ml

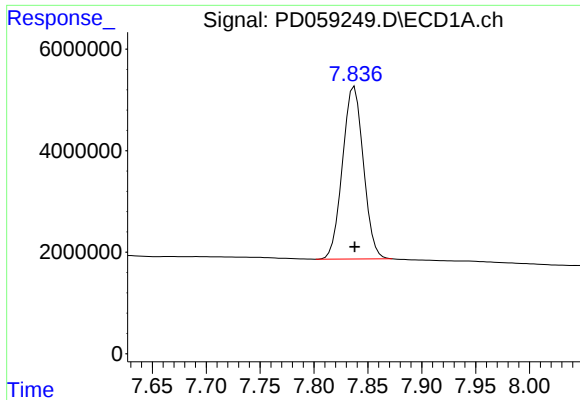

#28 Decachlorobiphenyl

R.T.: 7.837 min
Delta R.T.: 0.000 min
Response: 45962823
Conc: 49.34 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORCCC500

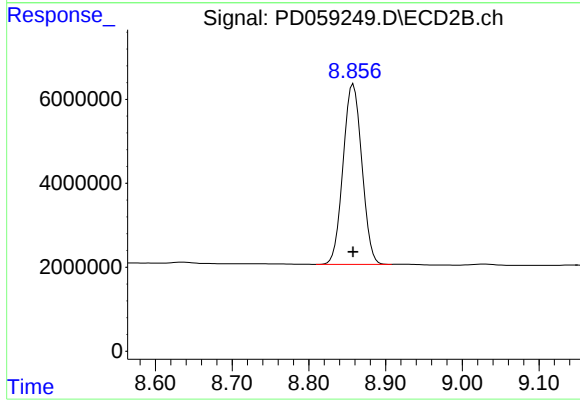

#28 Decachlorobiphenyl

R.T.: 8.858 min
Delta R.T.: 0.000 min
Response: 73376158
Conc: 46.91 ng/ml