

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091724\
 Data File : PD085252.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2024 19:27
 Operator : AR\AJ
 Sample : P3997-03
 Misc :
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 23:47:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.537	2.903	22434428	64012354	22.181	18.089
2)	SA Decachlor...	9.034	8.101	21639451	52867324	16.569	15.204
Target Compounds							
7)	B delta-BHC	4.763	0.000	4631350	0	2.824	N.D. #
14)	MA Endrin	6.584	0.000	1893009	0	1.678	N.D. #
20)	A Methoxychlor	7.488	0.000	1776937	0	3.411	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091724\
Data File : PD085252.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2024 19:27
Operator : AR\AJ
Sample : P3997-03
Misc :
ALS Vial : 18 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 23:47:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

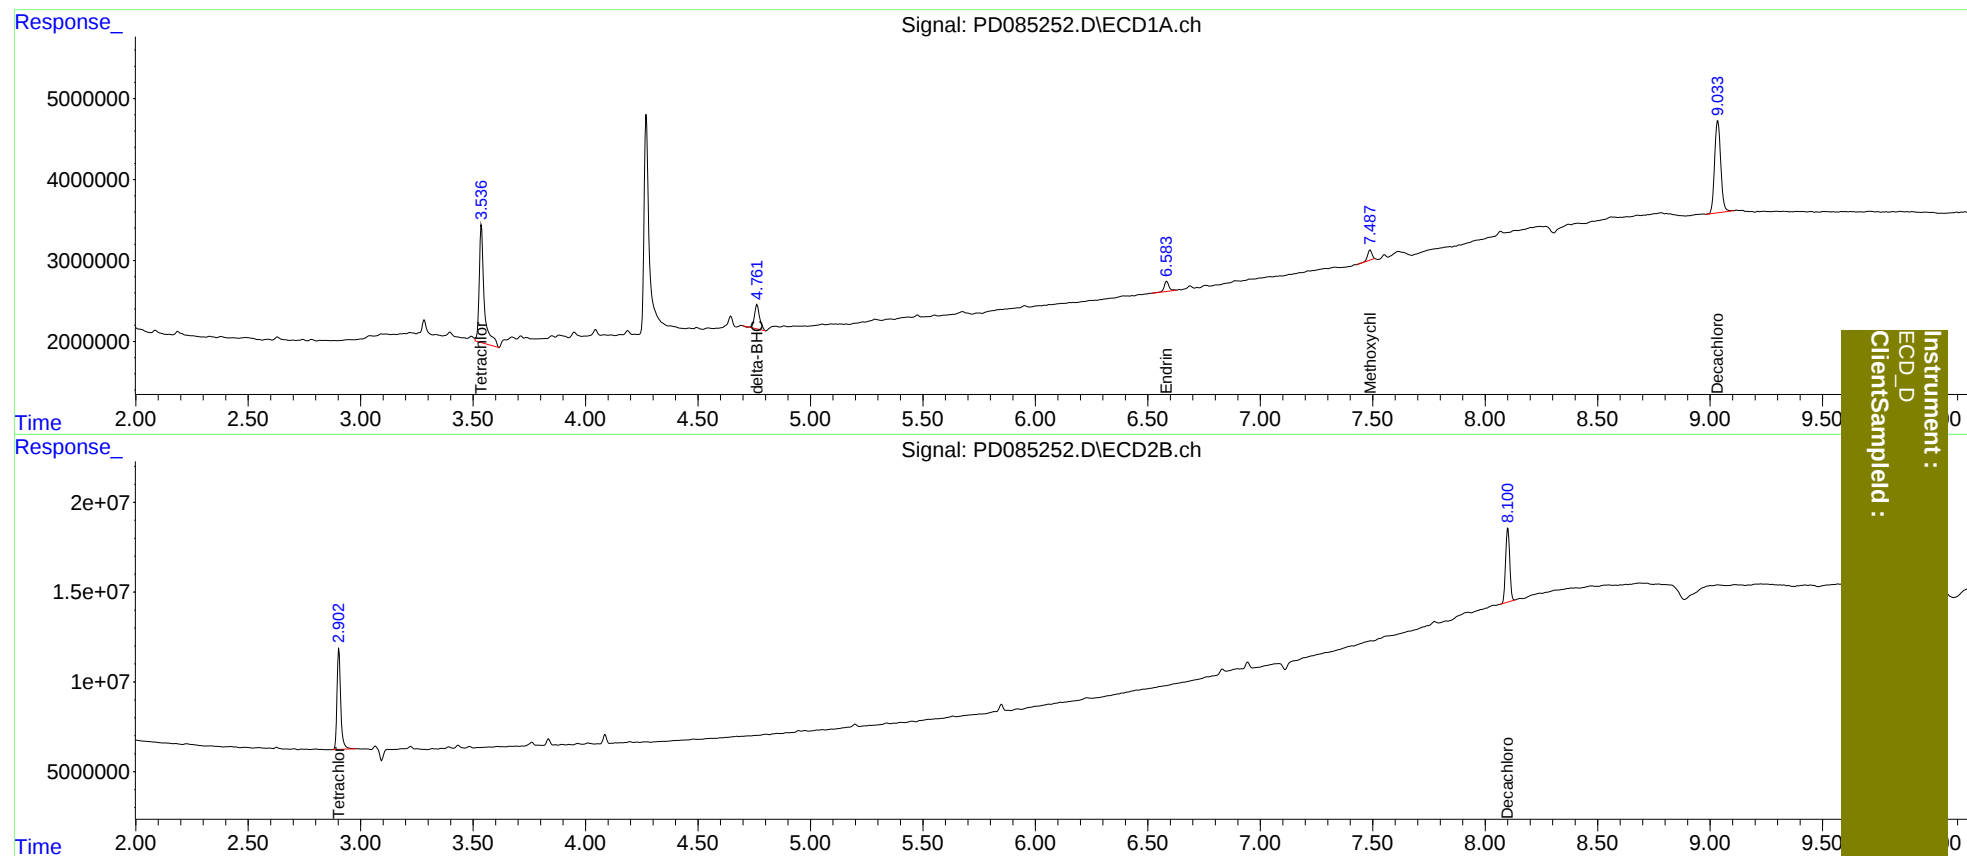


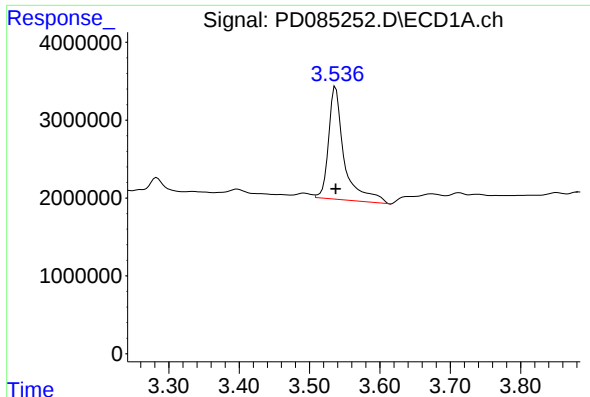

#1 Tetrachloro-m-xylene


R.T.: 3.537 min
Delta R.T.: 0.000 min
Response: 22434428
Conc: 22.18 ng/ml

Instrument :
ECD_D
ClientSampleId :

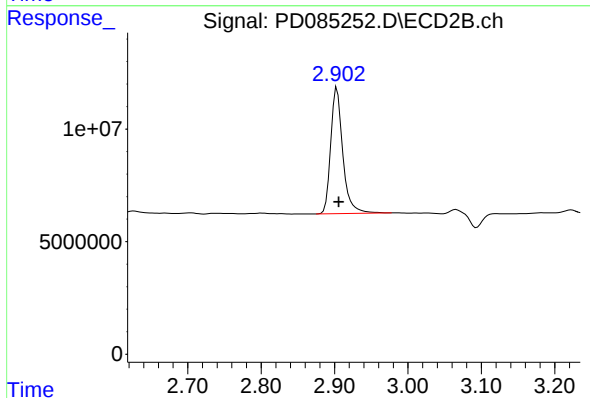


#1 Tetrachloro-m-xylene

R.T.: 2.903 min
Delta R.T.: -0.002 min
Response: 64012354
Conc: 18.09 ng/ml

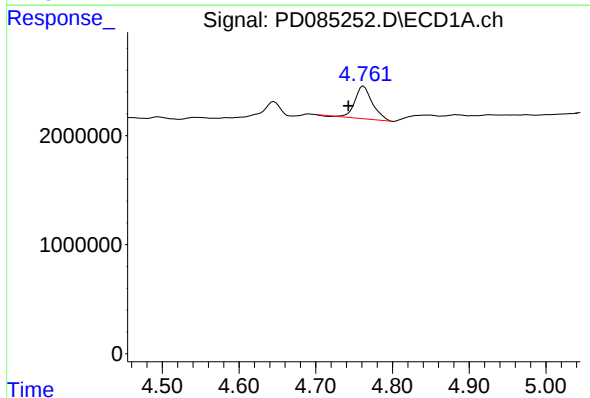


#7 delta-BHC

R.T.: 4.763 min
Delta R.T.: 0.020 min
Response: 4631350
Conc: 2.82 ng/ml

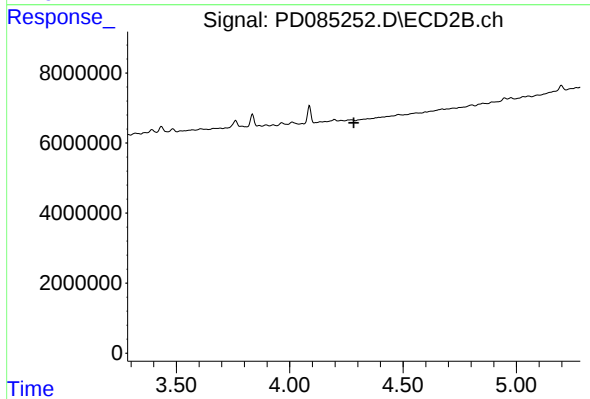

#7 delta-BHC


R.T.: 0.000 min
Exp R.T. : 4.283 min
Response: 0
Conc: N.D.

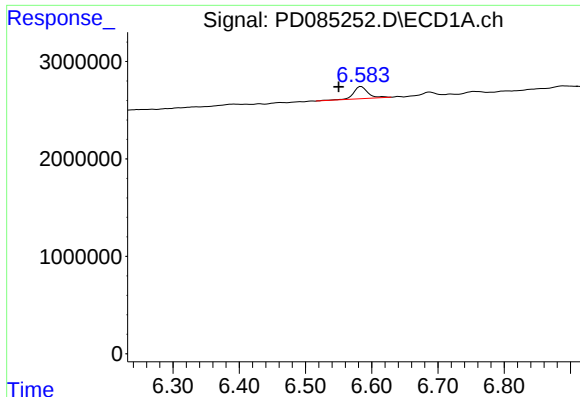

#14 Endrin


R.T.: 6.584 min
Delta R.T.: 0.034 min
Response: 1893009
Conc: 1.68 ng/ml

Instrument :
ECD_D
ClientSampleId :

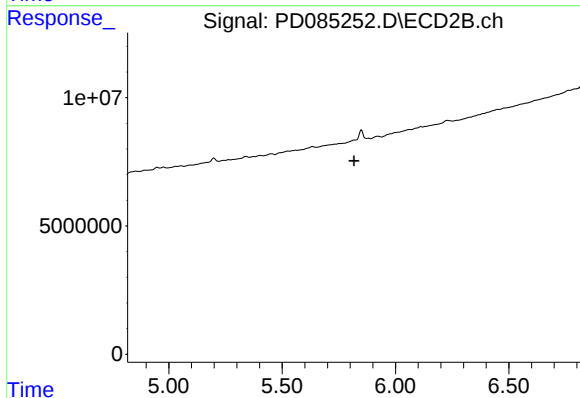


#14 Endrin

R.T.: 0.000 min
Exp R.T. : 5.817 min
Response: 0
Conc: N.D.

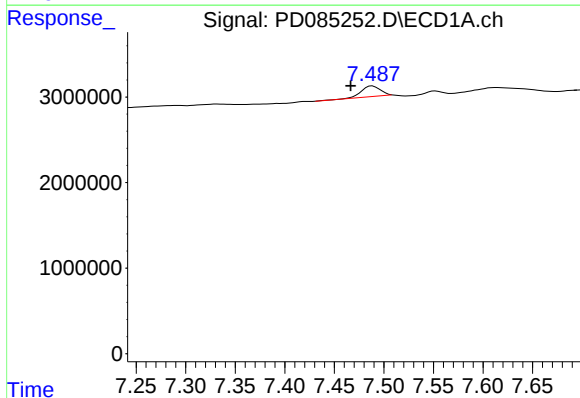


#20 Methoxychlor

R.T.: 7.488 min
Delta R.T.: 0.022 min
Response: 1776937
Conc: 3.41 ng/ml

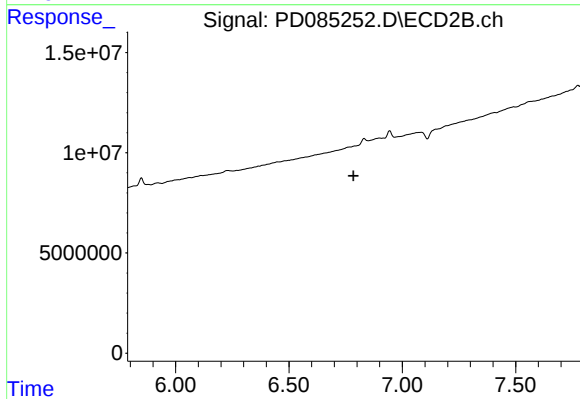

#20 Methoxychlor


R.T.: 0.000 min
Exp R.T. : 6.785 min
Response: 0
Conc: N.D.

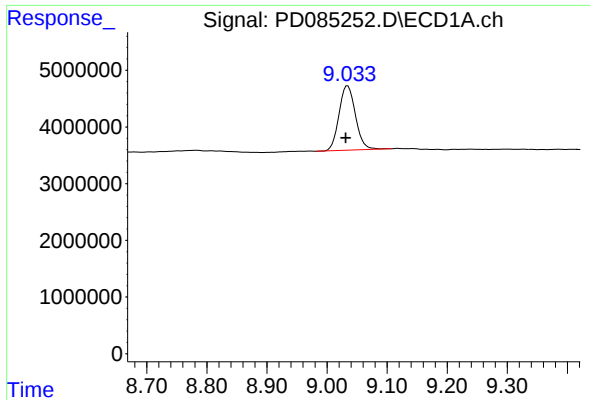

#27 Decachlorobiphenyl

R.T.: 9.034 min
Delta R.T.: 0.003 min
Response: 21639451
Conc: 16.57 ng/ml

Instrument :
ECD_D
ClientSampleId :

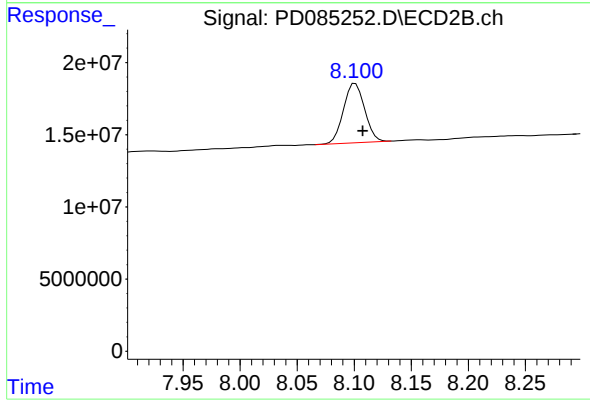

#27 Decachlorobiphenyl

R.T.: 8.101 min
Delta R.T.: -0.006 min
Response: 52867324
Conc: 15.20 ng/ml