

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091724\
 Data File : PD085271.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2024 23:41
 Operator : AR\AJ
 Sample : P4013-02
 Misc :
 ALS Vial : 37 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 01:10:27 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.538	2.903	21414995	70790615	21.174	20.004
27)	SA Decachlor...	9.035	8.101	25817883	65993970	19.768	18.979
Target Compounds							
4)	MA Heptachlor	4.897	0.000	4108353	0	2.670	N.D. #
5)	MB Aldrin	0.000	4.399	0	21439968	N.D.	4.827
6)	B beta-BHC	0.000	4.006f	0	5567516	N.D.	2.568
7)	B delta-BHC	4.758	0.000	55338071	0	33.743	N.D. #
10)	B trans-Chl...	5.908	0.000	2158518	0	1.530	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091724\
Data File : PD085271.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2024 23:41
Operator : AR\AJ
Sample : P4013-02
Misc :
ALS Vial : 37 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 01:10:27 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

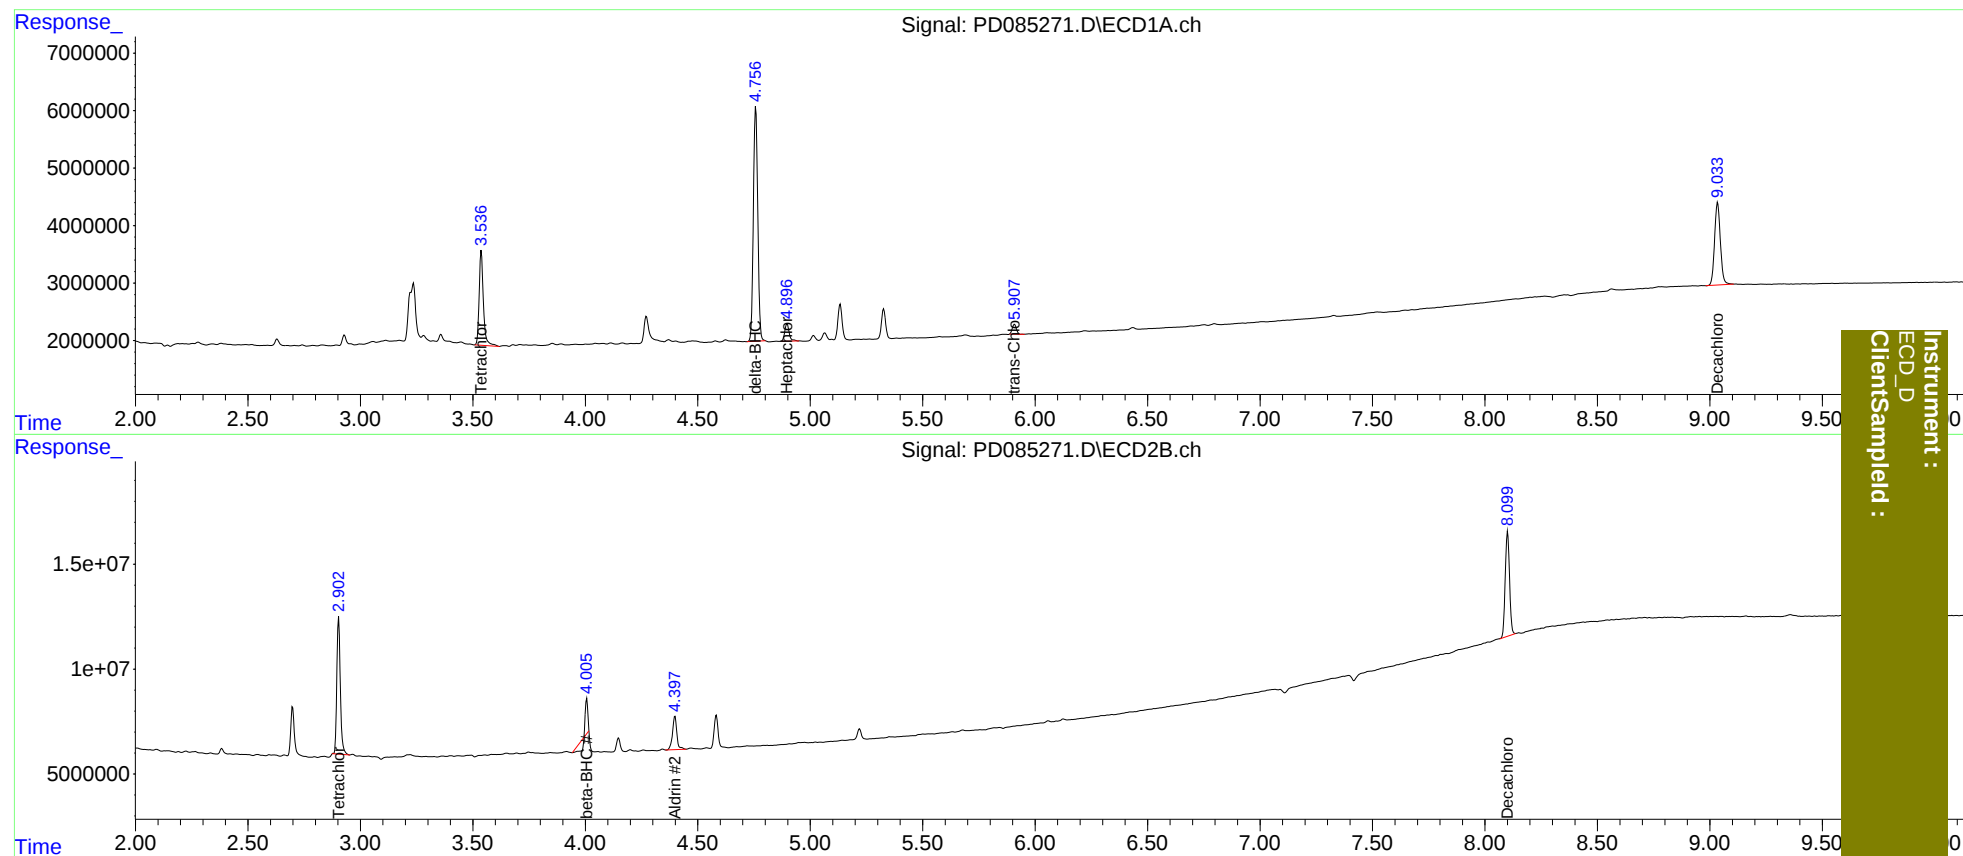


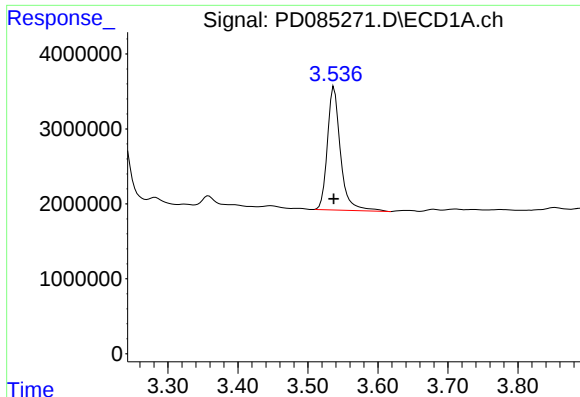

#1 Tetrachloro-m-xylene


R.T.: 3.538 min
Delta R.T.: 0.000 min
Response: 21414995
Conc: 21.17 ng/ml

Instrument :
ECD_D
ClientSampleId :

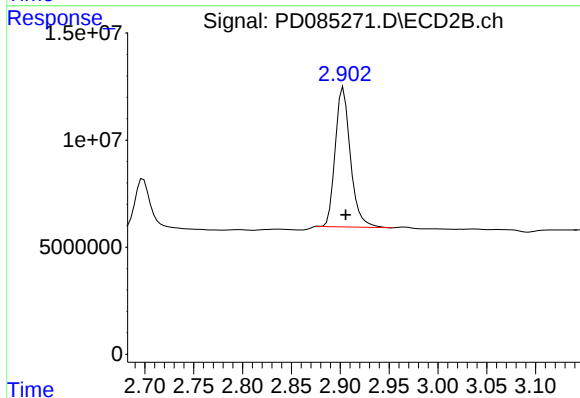


#1 Tetrachloro-m-xylene

R.T.: 2.903 min
Delta R.T.: -0.003 min
Response: 70790615
Conc: 20.00 ng/ml

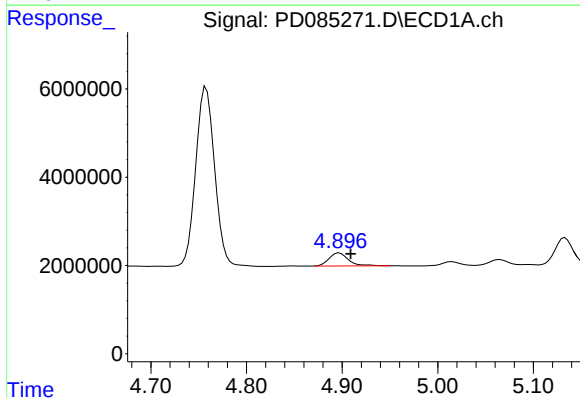


#4 Heptachlor

R.T.: 4.897 min
Delta R.T.: -0.012 min
Response: 4108353
Conc: 2.67 ng/ml

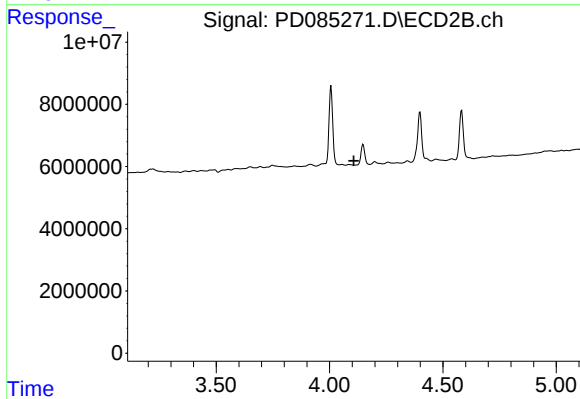

#4 Heptachlor


R.T.: 0.000 min
Exp R.T. : 4.107 min
Response: 0
Conc: N.D.

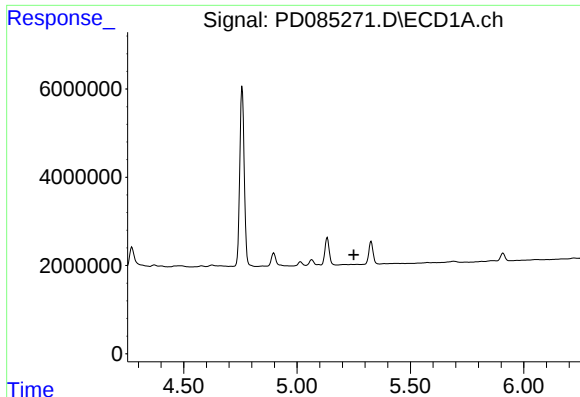

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.250 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

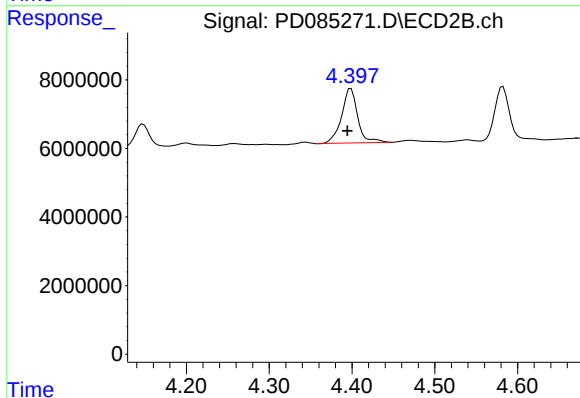


#5 Aldrin

R.T.: 4.399 min
Delta R.T.: 0.004 min
Response: 21439968
Conc: 4.83 ng/ml

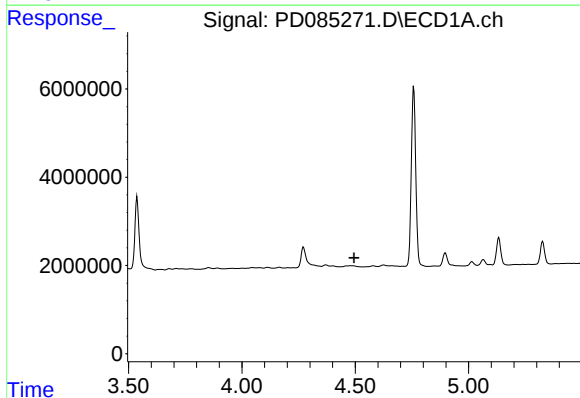


#6 beta-BHC

R.T.: 0.000 min
Exp R.T.: 4.495 min
Response: 0
Conc: N.D.

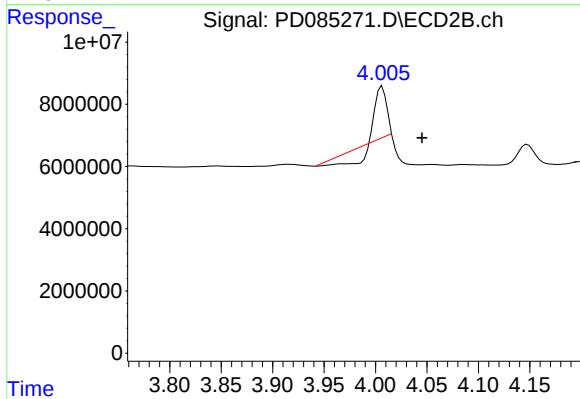

#6 beta-BHC


R.T.: 4.006 min
Delta R.T.: -0.039 min
Response: 5567516
Conc: 2.57 ng/ml

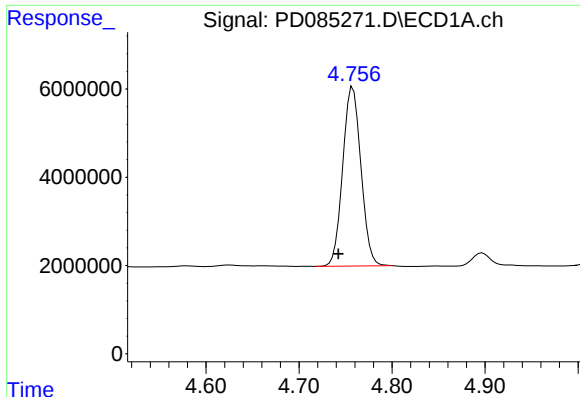

#7 delta-BHC


R.T.: 4.758 min
Delta R.T.: 0.015 min
Response: 55338071
Conc: 33.74 ng/ml

Instrument :
ECD_D
ClientSampleId :

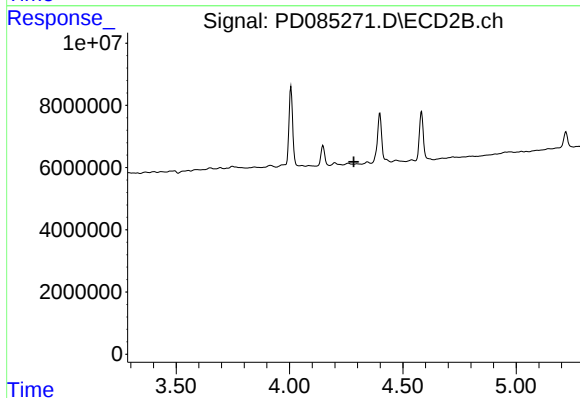


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.283 min
Response: 0
Conc: N.D.

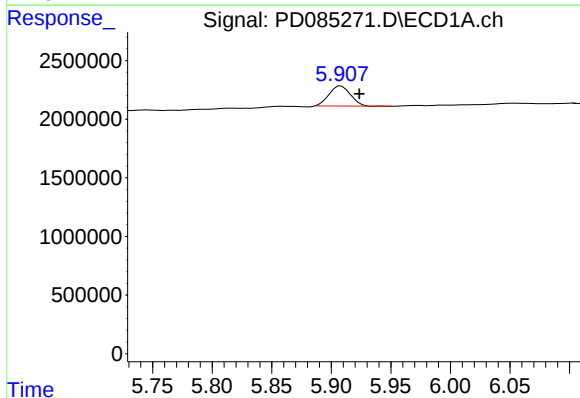


#10 trans-Chlordane

R.T.: 5.908 min
Delta R.T.: -0.015 min
Response: 2158518
Conc: 1.53 ng/ml

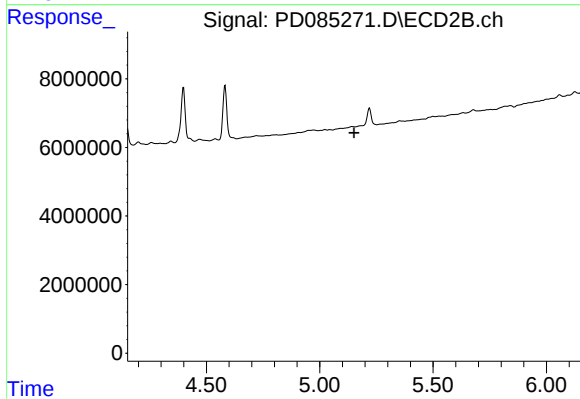

#10 trans-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.152 min
Response: 0
Conc: N.D.

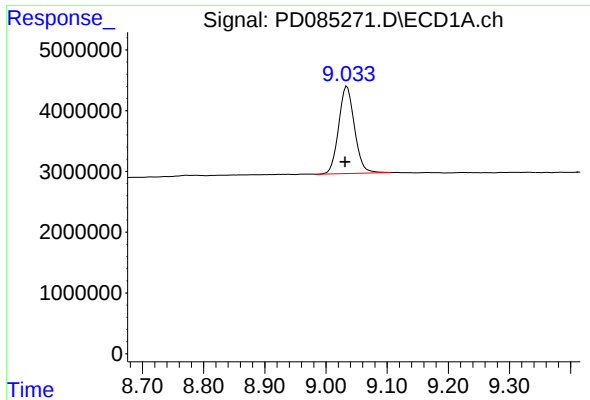

#27 Decachlorobiphenyl

R.T.: 9.035 min
Delta R.T.: 0.003 min
Response: 25817883
Conc: 19.77 ng/ml

Instrument :
ECD_D
ClientSampleId :

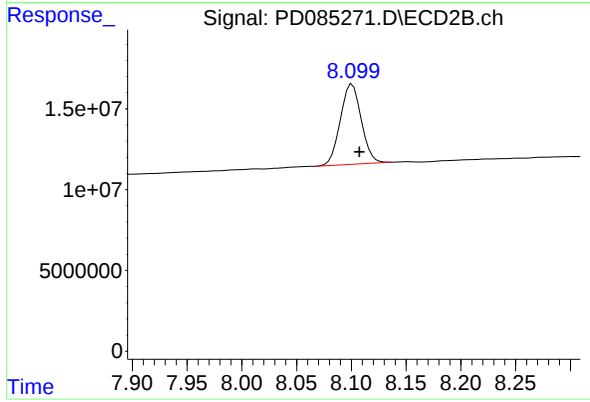

#27 Decachlorobiphenyl

R.T.: 8.101 min
Delta R.T.: -0.007 min
Response: 65993970
Conc: 18.98 ng/ml