

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091724\
 Data File : PD085275.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2024 00:34
 Operator : AR\AJ
 Sample : P4013-06
 Misc :
 ALS Vial : 41 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 01:11:10 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.538	2.903	21279754	75971866	21.040	21.468
2) SA Decachlor...	9.035	8.101	16378134	42068154	12.540	12.098
Target Compounds						
4) MA Heptachlor	4.897	0.000	4617808	0	3.001	N.D. #
5) MB Aldrin	0.000	4.400	0	9018479	N.D.	2.031

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091724\
Data File : PD085275.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2024 00:34
Operator : AR\AJ
Sample : P4013-06
Misc :
ALS Vial : 41 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 01:11:10 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

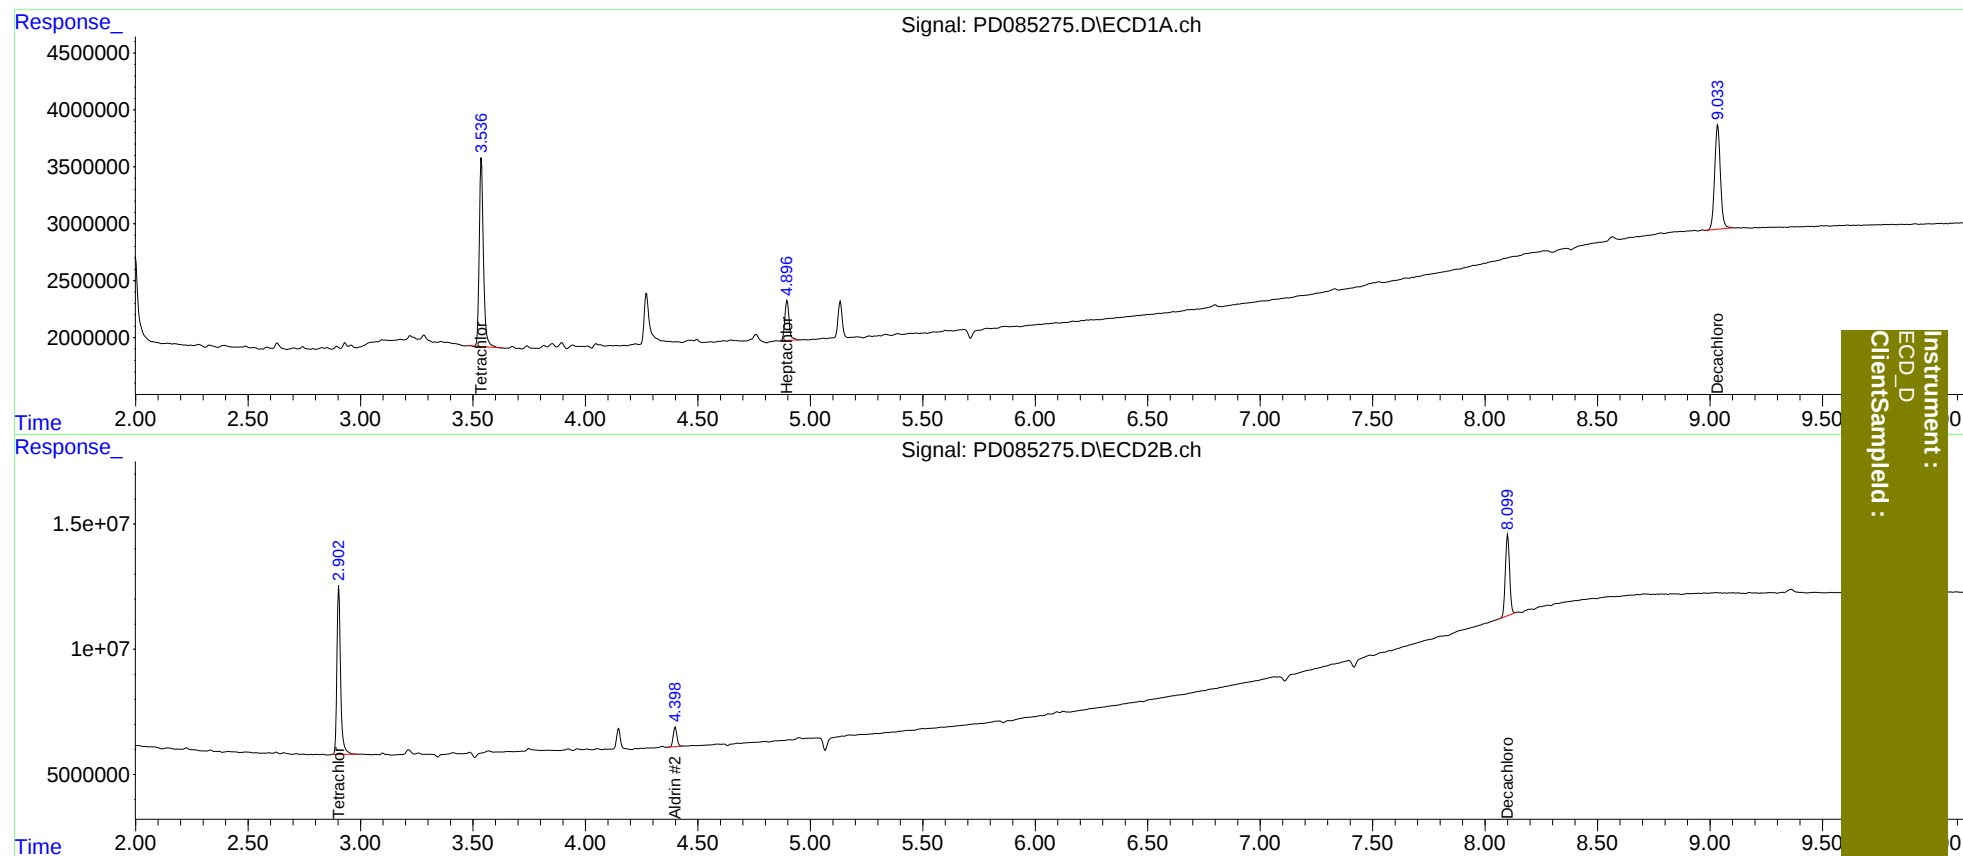


Instrument :
ECD_D
ClientSampled :
0

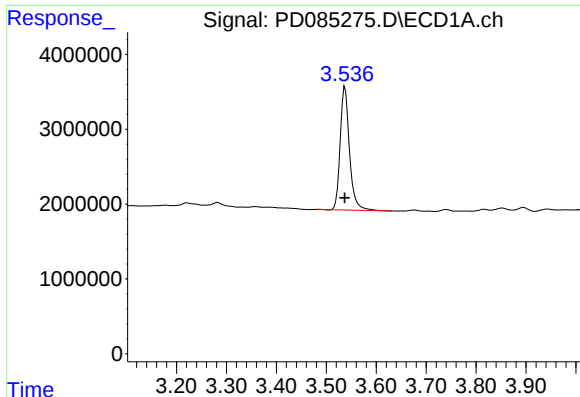

#1 Tetrachloro-m-xylene


R.T.: 3.538 min
Delta R.T.: 0.000 min
Response: 21279754
Conc: 21.04 ng/ml

Instrument :
ECD_D
ClientSampleId :

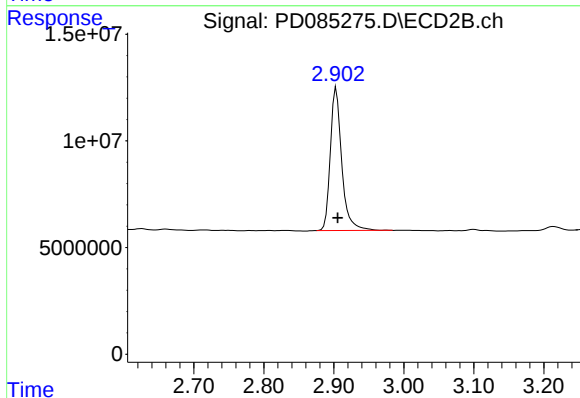


#1 Tetrachloro-m-xylene

R.T.: 2.903 min
Delta R.T.: -0.002 min
Response: 75971866
Conc: 21.47 ng/ml

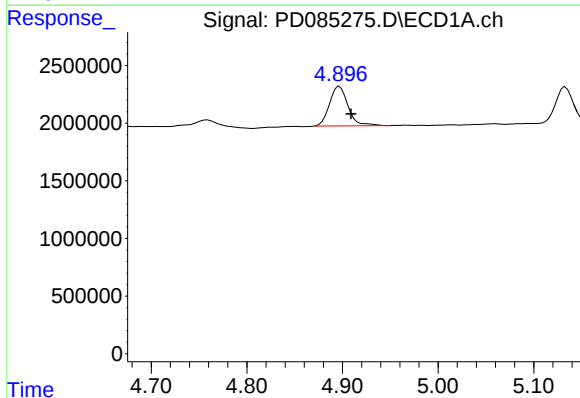


#4 Heptachlor

R.T.: 4.897 min
Delta R.T.: -0.012 min
Response: 4617808
Conc: 3.00 ng/ml

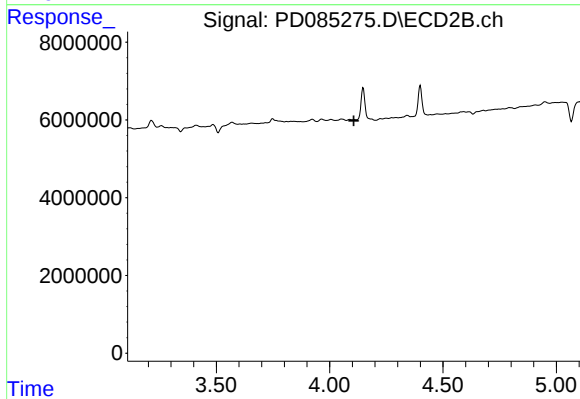

#4 Heptachlor


R.T.: 0.000 min
Exp R.T.: 4.107 min
Response: 0
Conc: N.D.

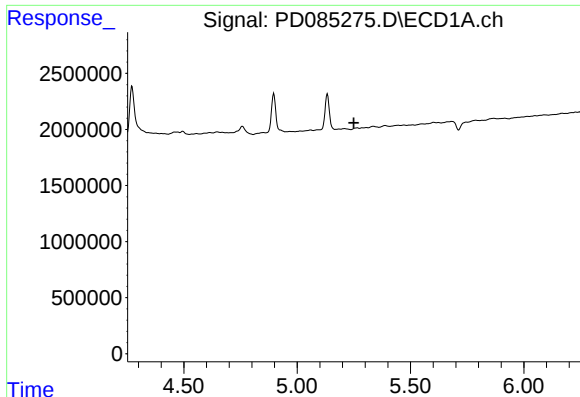

#5 Aldrin


R.T.: 0.000 min
Exp R.T.: 5.250 min
Response: 0
Conc: N.D.

Instrument :
ECD_D
ClientSampleId :

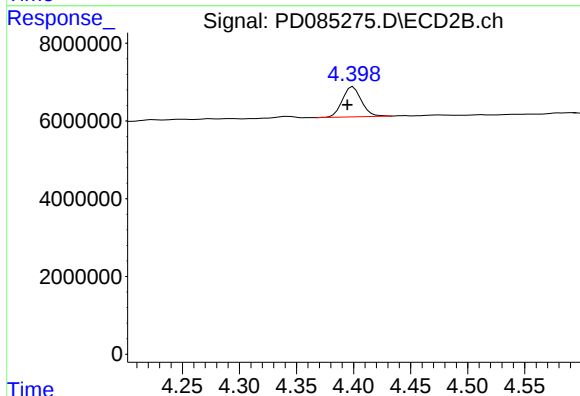


#5 Aldrin

R.T.: 4.400 min
Delta R.T.: 0.005 min
Response: 9018479
Conc: 2.03 ng/ml

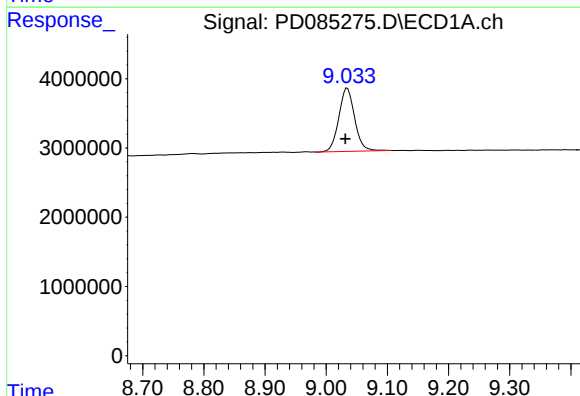

#27 Decachlorobiphenyl

R.T.: 9.035 min
Delta R.T.: 0.003 min
Response: 16378134
Conc: 12.54 ng/ml

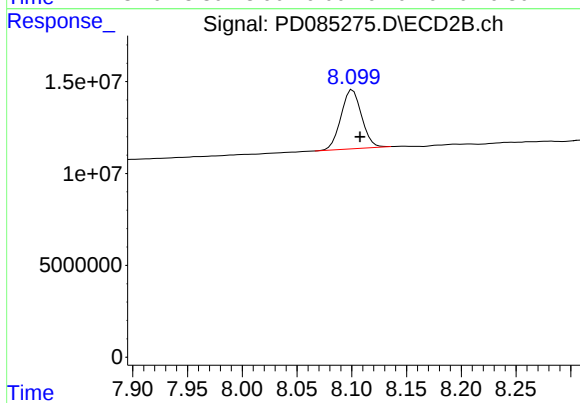

#27 Decachlorobiphenyl

R.T.: 8.101 min
Delta R.T.: -0.007 min
Response: 42068154
Conc: 12.10 ng/ml