

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091724\
 Data File : PD085288.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2024 03:28
 Operator : AR\AJ
 Sample : P3910-01
 Misc :
 ALS Vial : 49 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDC74

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/19/2024
 Supervised By :Ankita Jodhani 09/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 04:36:32 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.527	2.914	14015271	217.9E6	13.857m	61.566 #
2) SA Decachlor...	9.033	8.101	16751549	45330589	12.826	13.037
Target Compounds						
2) A alpha-BHC	3.982	3.411	19008130	43846486	11.180	8.648
6) B beta-BHC	4.493	4.041	13165460	31702695	18.125m	14.623
9) A Endosulfan I	6.054	5.262	8780376	7182514	6.382	1.874m#
14) MA Endrin	6.561	5.817	1422842	14390196	1.261m	3.887m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091724\
Data File : PD085288.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2024 03:28
Operator : AR\AJ
Sample : P3910-01
Misc :
ALS Vial : 49 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 04:36:32 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

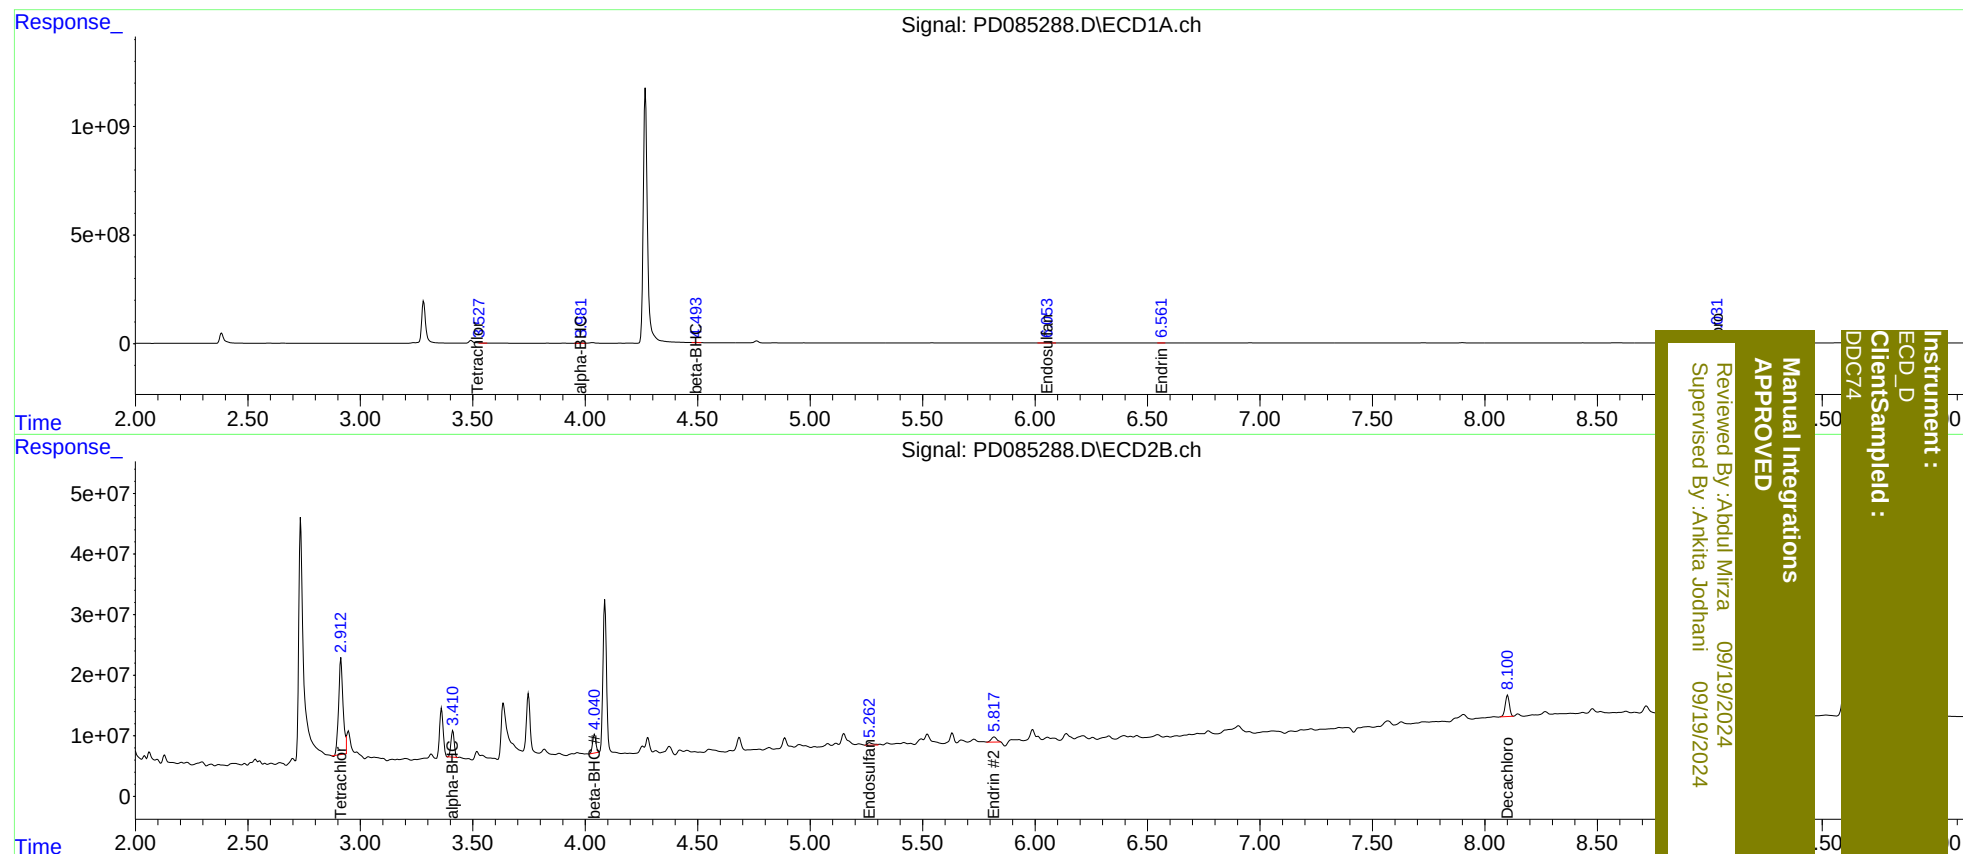

Reviewed By: Abdul Mirza 09/19/2024
Supervised By: Ankita Jodhani 09/19/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
DDC74