

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091724\
 Data File : PD085308.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2024 07:55
 Operator : AR\AJ
 Sample : P3910-21MS
 Misc :
 ALS Vial : 69 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDC66MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/19/2024
 Supervised By :Ankita Jodhani 09/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 08:52:22 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.915	15443024	290.8E6	15.269m	82.179 #
27)	SA Decachlor...	9.034	8.100	30759732	45372449	23.552	13.049m#
Target Compounds							
2)	A alpha-BHC	3.982	3.413	99415315	245.8E6	58.474	48.488
3)	MA gamma-BHC...	4.299	3.748	188.1E6	222.4E6	116.280m	45.888 #
4)	MA Heptachlor	4.909	4.087	78273695	732.7E6	50.873	172.107m#
5)	MB Aldrin	5.250	4.388	84353985	200.7E6	52.742	45.181
6)	B beta-BHC	4.493	4.041	32534478	87881903	44.790m	40.537
7)	B delta-BHC	4.744	4.279	61823306	256.4E6	37.697m	51.646 #
8)	B Heptachlo...	5.669	4.892	72641979	188.1E6	48.705	44.404
9)	A Endosulfan I	6.050	5.268	64188014	168.5E6	46.655m	43.966
10)	B trans-Chl...	5.924	5.144	70188496	188.0E6	49.766	45.701m
11)	B cis-Chlor...	6.003	5.211	76669930	185.0E6	51.855m	44.093
12)	B 4,4'-DDE	6.173	5.396	134.0E6	362.9E6	107.437	92.509
13)	MA Dieldrin	6.324	5.535	149.8E6	386.9E6	101.564	90.061
14)	MA Endrin	6.551	5.813	129.2E6	341.3E6	114.483	92.180
15)	B Endosulfa...	6.762	6.104	120.7E6	320.4E6	91.463	86.411
16)	A 4,4'-DDD	6.681	5.952	111.7E6	324.1E6	113.170	95.518
17)	MA 4,4'-DDT	6.996	6.208	87943900	257.4E6	98.247	80.468
18)	B Endrin al...	6.891	6.284	93707886	237.5E6	103.762	83.179
19)	B Endosulfa...	7.124	6.508	118.5E6	306.1E6	102.860	85.693
20)	A Methoxychlor	7.467	6.780	265.8E6	610.0E6	510.271	368.725 #
21)	B Endrin ke...	7.605	7.019	127.0E6	368.5E6	103.912	83.688

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091724\
Data File : PD085308.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2024 07:55
Operator : AR\AJ
Sample : P3910-21MS
Misc :
ALS Vial : 69 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 08:52:22 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

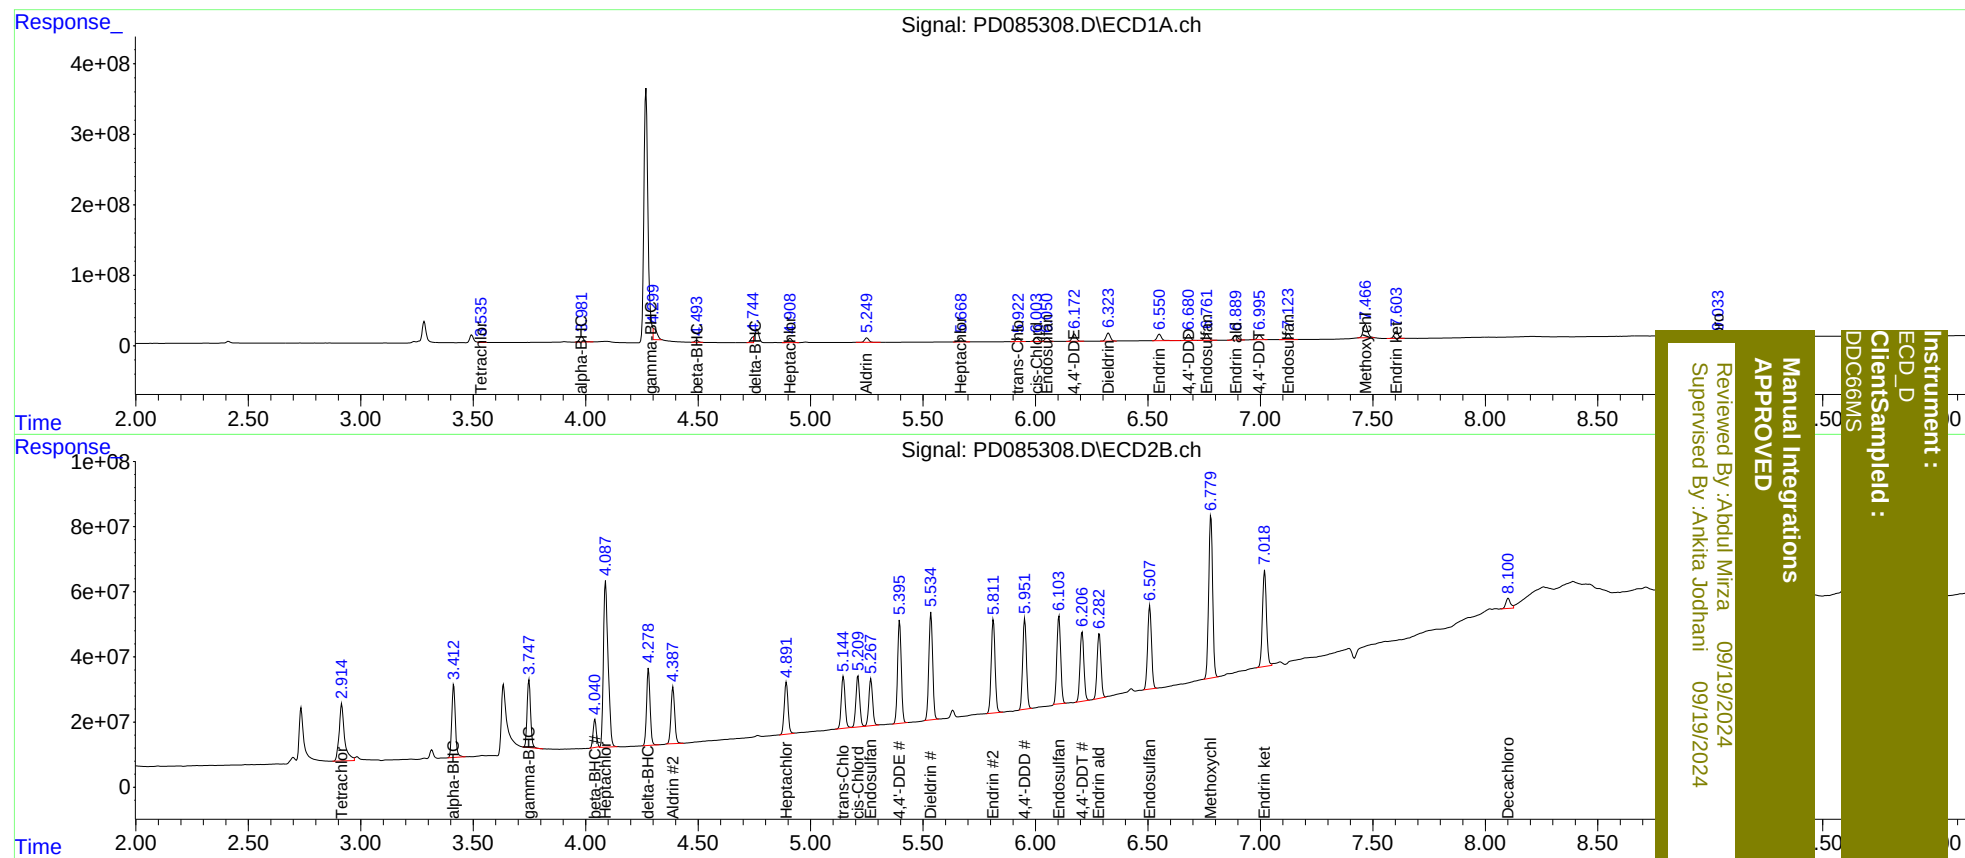

Reviewed By: Abdul Mirza 09/19/2024
Supervised By: Ankita Jodhani 09/19/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
DDC66MS