

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091724\
 Data File : PD085309.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2024 08:09
 Operator : AR\AJ
 Sample : P3910-22MSD
 Misc :
 ALS Vial : 70 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDC66MSD

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/19/2024
 Supervised By :Ankita Jodhani 09/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 08:52:41 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.535	2.938f	14409059	282.5E6	14.247m	79.824 #
27)	SA Decachlor...	9.034	8.124	24791623	60292741	18.982	17.339m
Target Compounds							
2)	A alpha-BHC	3.983	3.437	93117141	244.5E6	54.770	48.226
3)	MA gamma-BHC...	4.300	3.771	183.2E6	224.2E6	113.254m	46.277 #
4)	MA Heptachlor	4.909	4.110	77847431	747.3E6	50.596	175.539m#
5)	MB Aldrin	5.250	4.412	80865753	205.9E6	50.561	46.369
6)	B beta-BHC	4.493	4.063	31122215	96878887	42.846m	44.687m
7)	B delta-BHC	4.745	4.303	76585915	257.5E6	46.699m	51.874
8)	B Heptachlo...	5.669	4.915	73390267	190.1E6	49.207	44.883
9)	A Endosulfan I	6.051	5.291	70457455	179.4E6	51.212m	46.811
10)	B trans-Chl...	5.924	5.168	71085705	191.2E6	50.402	46.494m
11)	B cis-Chlor...	6.003	5.234	72756339	193.7E6	49.208m	46.165
12)	B 4,4'-DDE	6.173	5.419	134.6E6	370.1E6	107.932	94.349
13)	MA Dieldrin	6.324	5.559	149.6E6	395.9E6	101.440	92.160
14)	MA Endrin	6.551	5.836	124.5E6	349.7E6	110.369	94.457
15)	B Endosulfa...	6.762	6.127	122.0E6	334.6E6	92.448	90.238m
16)	A 4,4'-DDD	6.681	5.976	115.7E6	333.1E6	117.200	98.166
17)	MA 4,4'-DDT	6.997	6.232	89216632	258.1E6	99.669	80.695
18)	B Endrin al...	6.891	6.308	92196502	249.3E6	102.088	87.330
19)	B Endosulfa...	7.124	6.532	117.9E6	313.0E6	102.367	87.639
20)	A Methoxychlor	7.468	6.803	256.4E6	618.6E6	492.250	373.972
21)	B Endrin ke...	7.605	7.043	130.9E6	369.9E6	107.031	84.001

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091724\
Data File : PD085309.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2024 08:09
Operator : AR\AJ
Sample : P3910-22MSD
Misc :
ALS Vial : 70 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 08:52:41 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

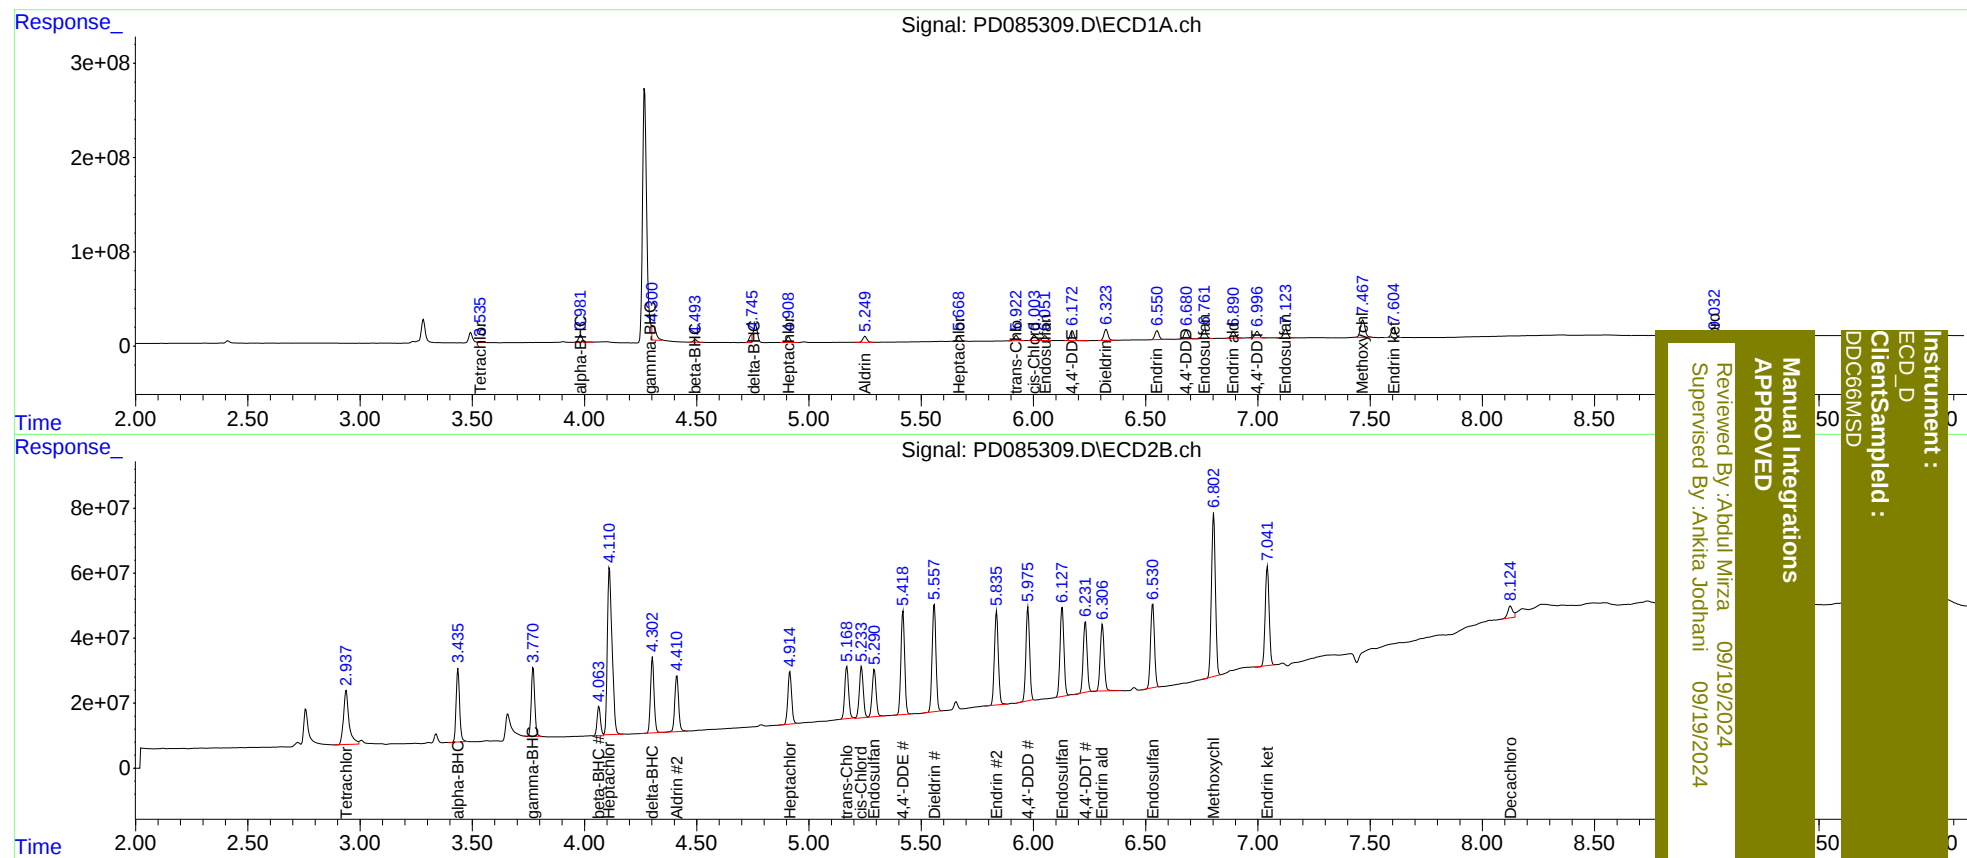

Reviewed By: Abdul Miza 09/19/2024
Supervised By: Ankita Jodhani 09/19/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
DDC66MSD