Quantitation Report (Qedit)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091724\
Data File : PD085253.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2024 19:41
Operator : AR\AJ
Sample : P3997-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 23:47:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Instrument :
ECD_D
ClientSampleId :
C0AN9

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 09/18/2024
Supervised By :Ankita Jodhani 09/18/2024

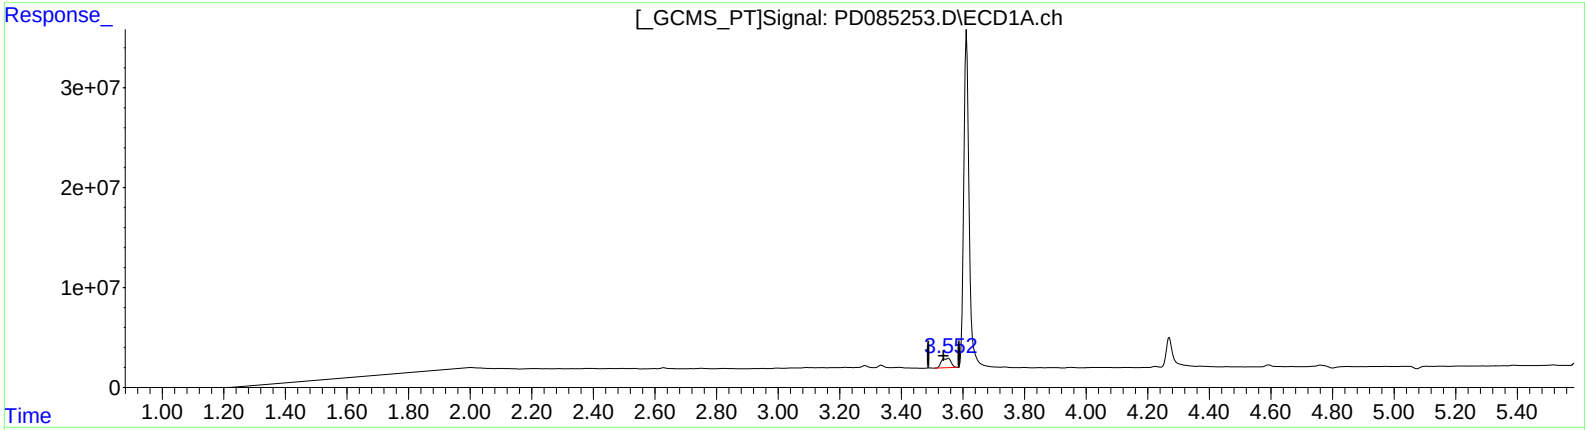

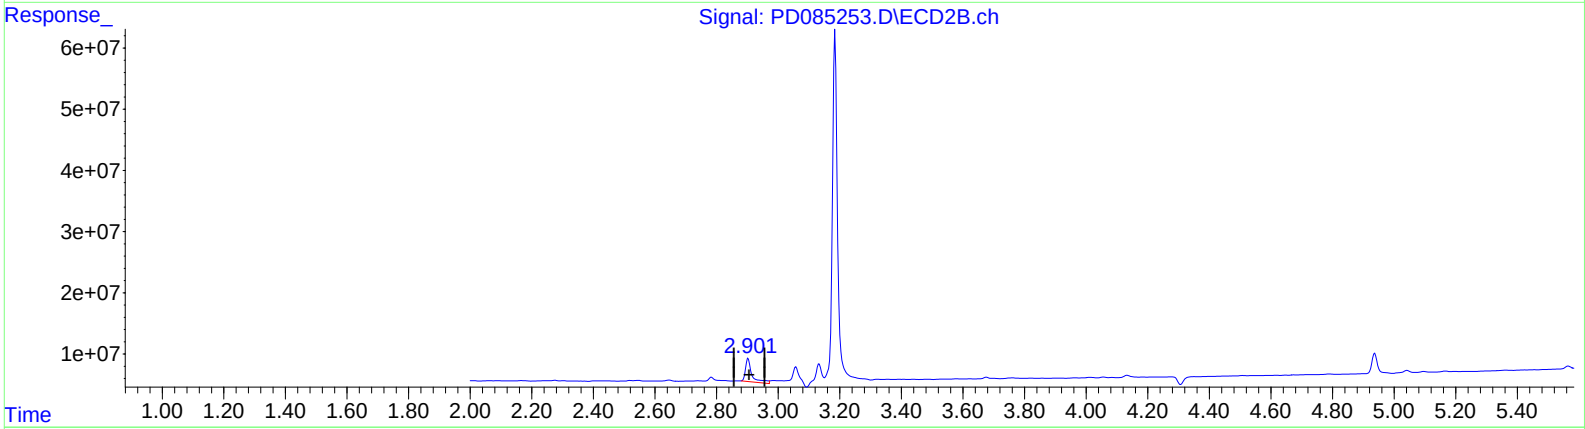

QEdit

(1) Tetrachloro-m-xylene (SA)

3.553min 20.079 ng/ml

response 20307625

(1) Tetrachloro-m-xylene #2 (SA)

2.902min 15.668 ng/ml

response 55444424

(+) = Expected Retention Time

Quantitation Report (Qedit)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091724\
Data File : PD085253.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2024 19:41
Operator : AR\AJ
Sample : P3997-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 23:47:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Instrument :
ECD_D
ClientSampleId :
C0AN9

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 09/18/2024
Supervised By :Ankita Jodhani 09/18/2024

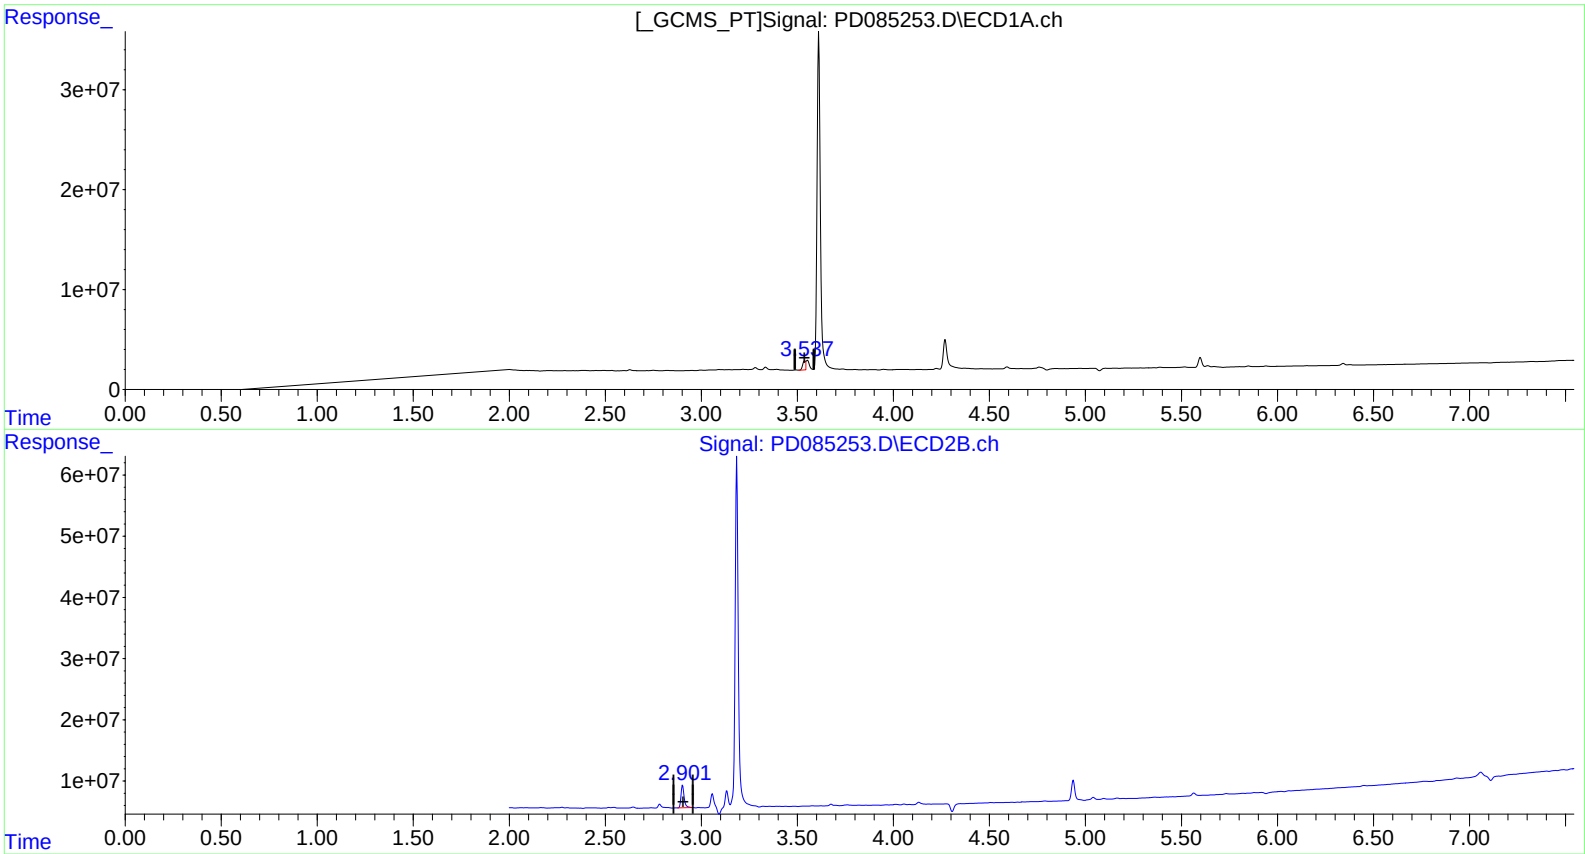

QEdit

(1) Tetrachloro-m-xylene (SA)

3.537min 10.781 ng/ml m

response 10903942

(1) Tetrachloro-m-xylene #2 (SA)

2.901min 11.866 ng/ml m

response 41991483

(+) = Expected Retention Time

Quantitation Report (Qedit)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091724\
Data File : PD085253.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2024 19:41
Operator : AR\AJ
Sample : P3997-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0AN9

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 09/18/2024
Supervised By :Ankita Jodhani 09/18/2024

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 23:47:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

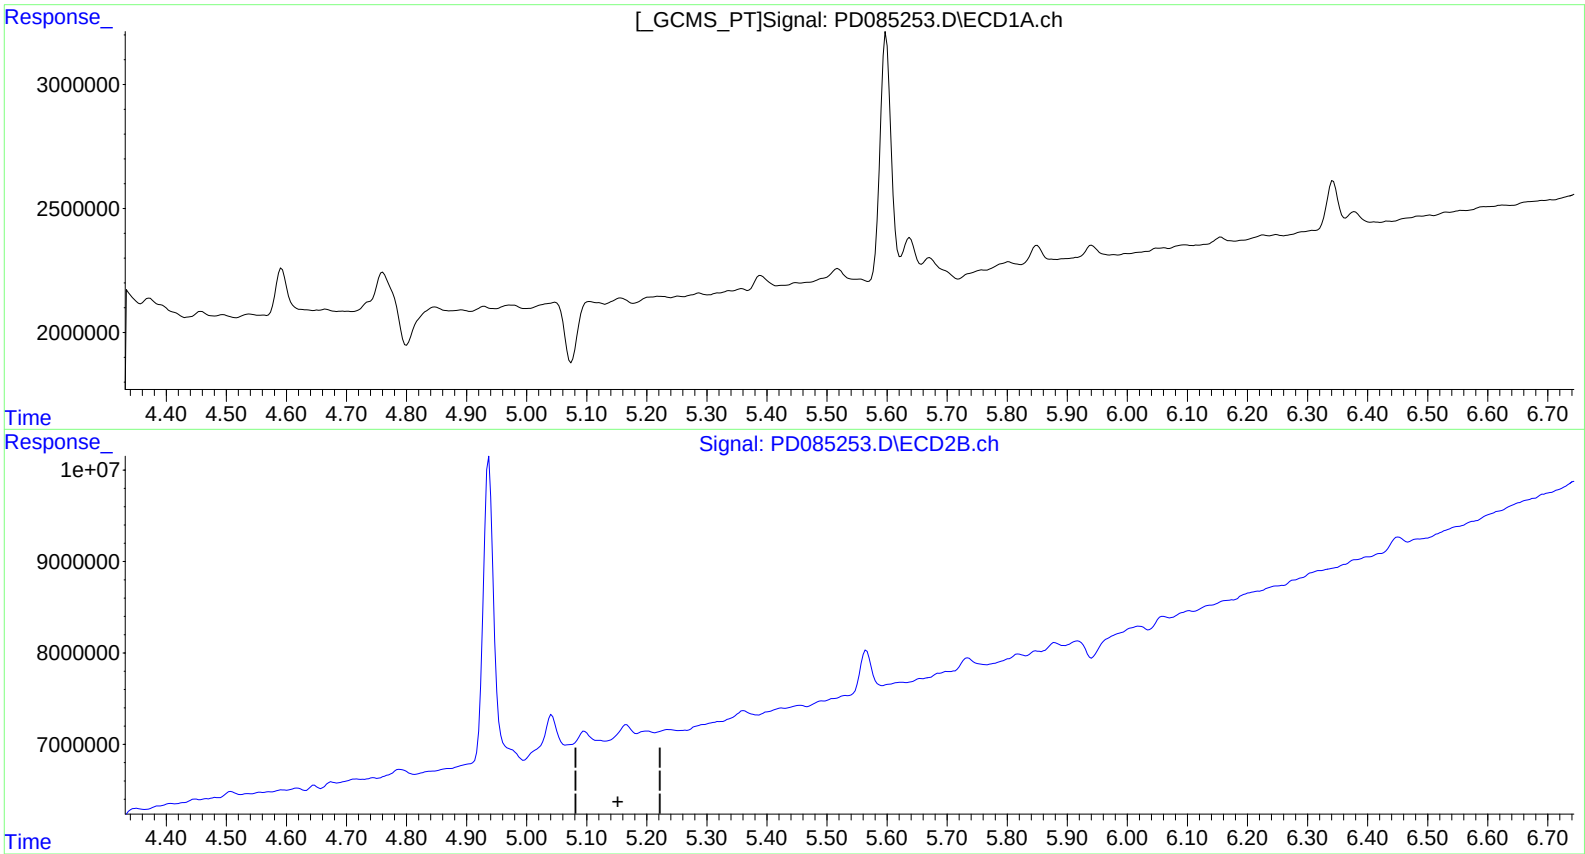

QEdit

(10) trans-Chlordane (B)

0.000min 0.000 ng/ml

response 0

(10) trans-Chlordane #2 (B)

0.000min 0.000 ng/ml

response 0

(+) = Expected Retention Time

Quantitation Report (Qedit)

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091724\
Data File : PD085253.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2024 19:41
Operator : AR\AJ
Sample : P3997-04
Misc :
ALS Vial : 19 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 23:47:53 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Instrument :
ECD_D
ClientSampleId :
C0AN9

Manual IntegrationsAPPROVED

Reviewed By :Abdul Mirza 09/18/2024
Supervised By :Ankita Jodhani 09/18/2024

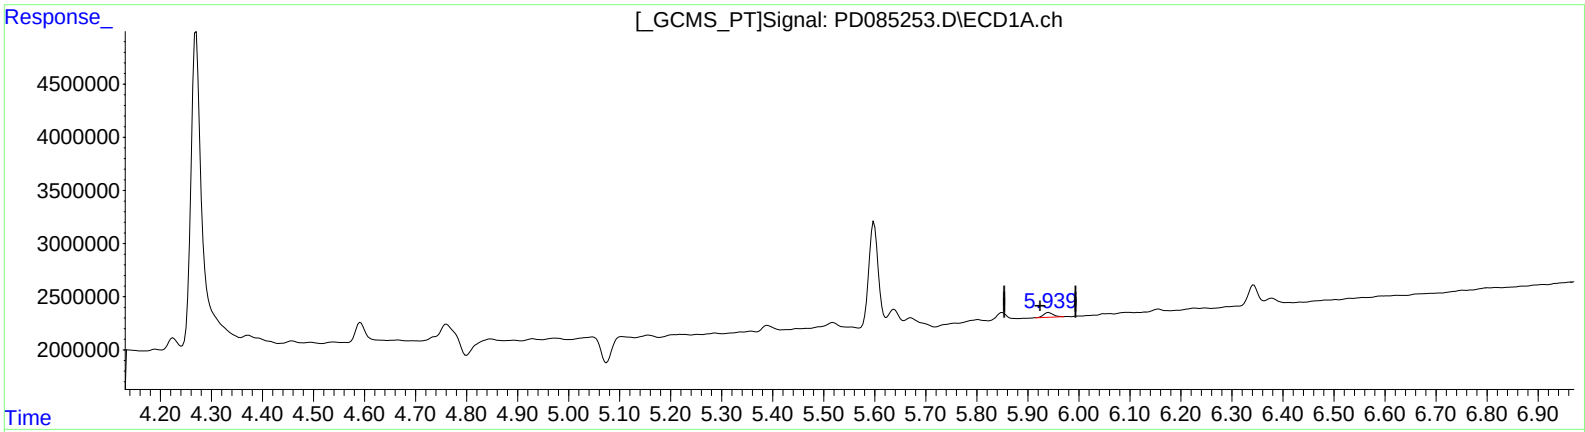

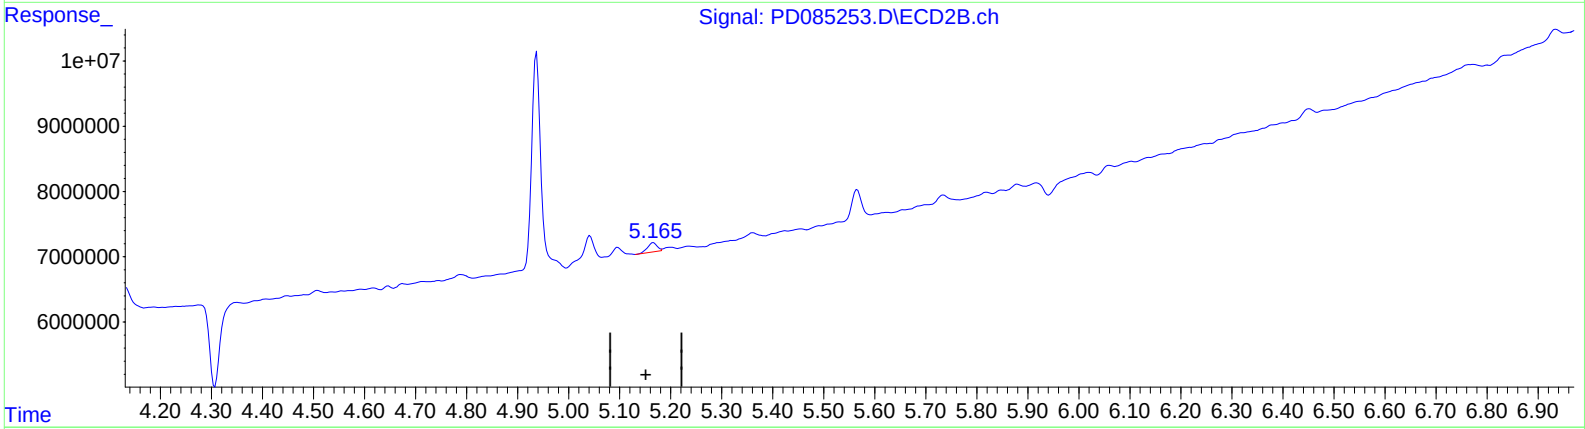

QEdit

(10) trans-Chlordane (B)

5.939min 0.414 ng/ml m

response 583955

(10) trans-Chlordane #2 (B)

5.165min 0.452 ng/ml m

response 1859174

(+) = Expected Retention Time