

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091724\
 Data File : PD085240.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2024 15:15
 Operator : AR\AJ
 Sample : P3878-16DL 2X
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDC05DL

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/20/2024
 Supervised By :Ankita Jodhani 09/20/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 23:21:47 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.530	2.914	13819291	824.5E6	13.663m	232.996m#
2)	SA Decachlor...	9.031	8.095	13998229	24268250	10.718m	6.979m#
Target Compounds							
2)	A alpha-BHC	3.982	3.412	81681180	170.6E6	48.043	33.646 #
7)	B delta-BHC	4.740	4.277	96963633	231.7E6	59.124m	46.685m
9)	A Endosulfan I	6.054	5.278	34795359	70521812	25.291m	18.397m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091724\
Data File : PD085240.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2024 15:15
Operator : AR\AJ
Sample : P3878-16DL 2X
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 23:21:47 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

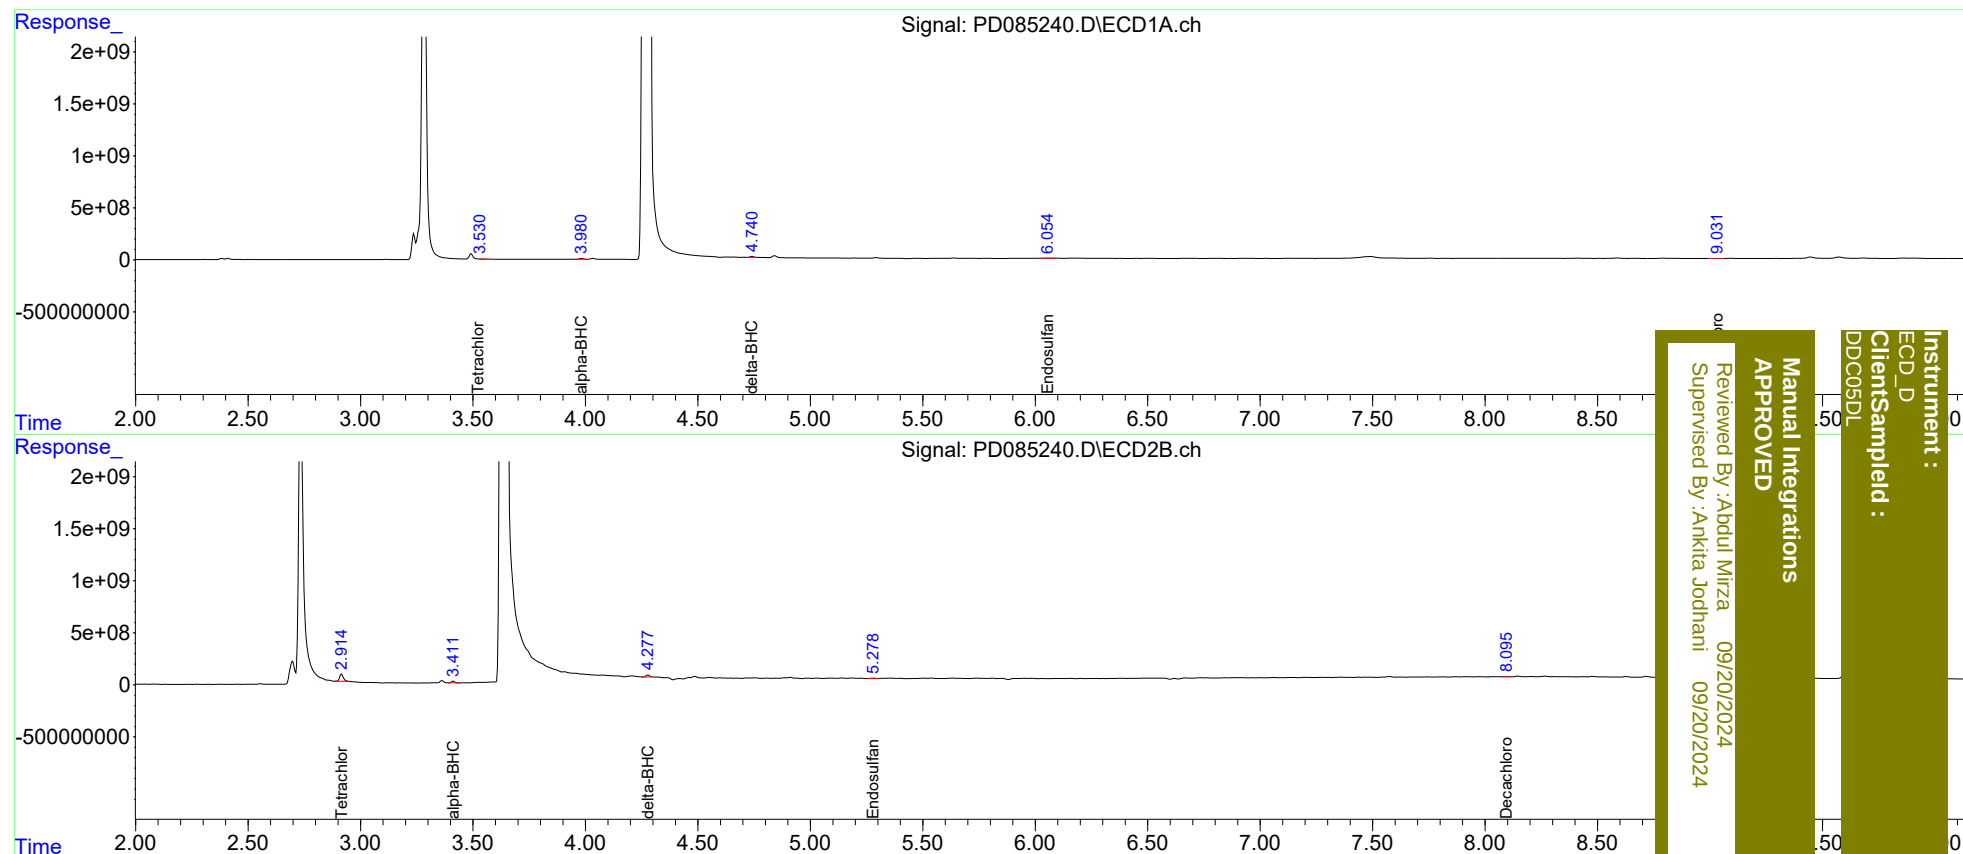

Reviewed By: Abdul Mirza 09/20/2024
Supervised By: Ankita Jodhani 09/20/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
DDC05DL