

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091725\
 Data File : PD090314.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2025 12:46
 Operator : AR\AJ
 Sample : INDA101
 Misc :
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA1085

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 07:33:51 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091725CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 18 07:32:47 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.545	2.876	14264280	129.7E6	5.588	5.782
27)	SA Decachlor...	9.065	8.063	45394207	276.4E6	11.515	11.309
Target Compounds							
2)	A alpha-BHC	3.994	3.388	26533982	203.0E6	5.010	5.559
3)	MA gamma-BHC...	4.325	3.724	27401589	188.1E6	5.281	5.629
4)	MA Heptachlor	4.923	4.076	27661642	196.8E6	5.320	5.649
9)	A Endosulfan I	6.069	5.240	23885822	165.8E6	5.386	5.609
13)	MA Dieldrin	6.341	5.505	48232363	359.6E6	10.159	11.225
14)	MA Endrin	6.568	5.782	40893658	341.6E6	10.255	11.617
16)	A 4,4'-DDD	6.700	5.922	33293830	294.3E6	10.055	11.168
17)	MA 4,4'-DDT	7.016	6.176	34249112	293.5E6	9.967	10.724
20)	A Methoxychlor	7.488	6.746	97255604	716.2E6	52.847	58.855


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091725\
Data File : PD090314.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2025 12:46
Operator : AR\AJ
Sample : INDA101
Misc :
ALS Vial : 9 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 07:33:51 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091725CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 18 07:32:47 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

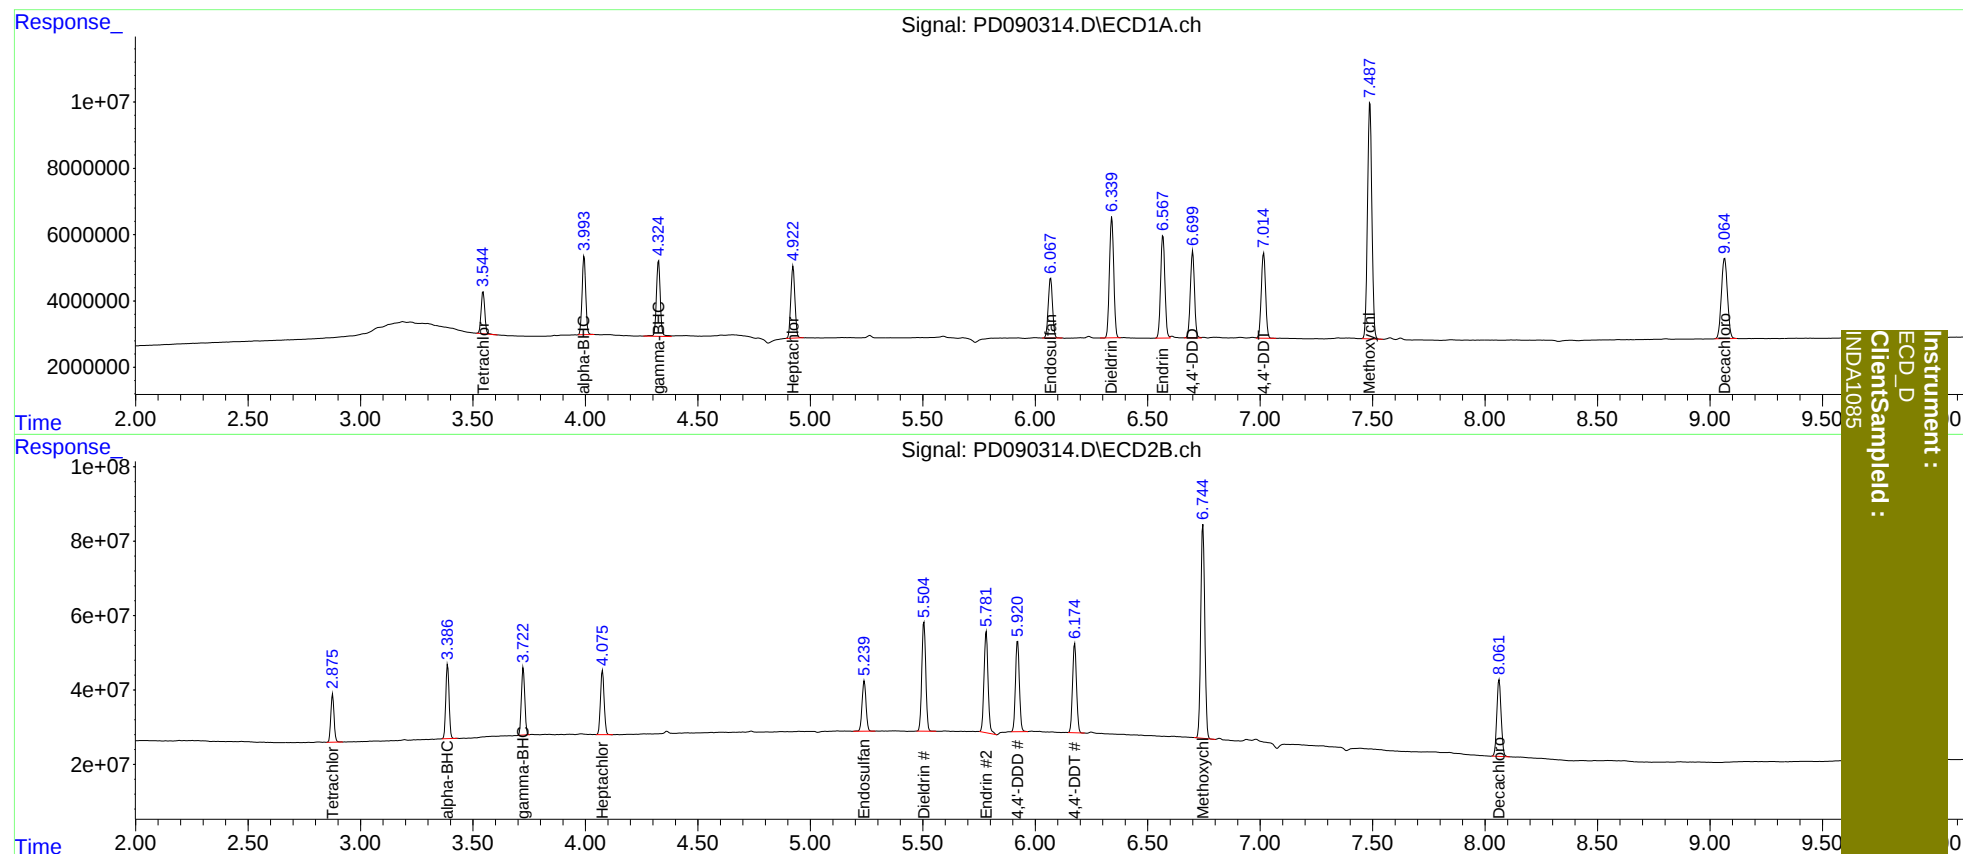


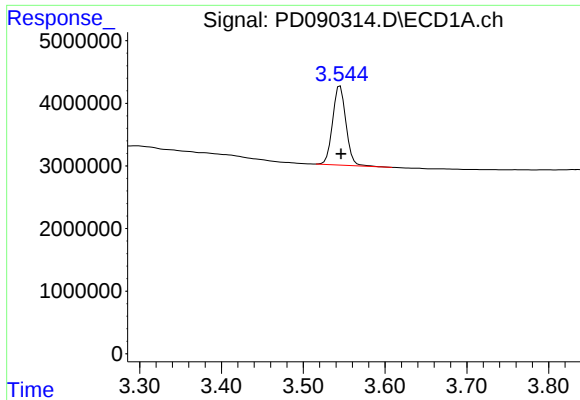

#1 Tetrachloro-m-xylene


R.T.: 3.545 min
Delta R.T.: 0.000 min
Response: 14264280
Conc: 5.59 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA1085

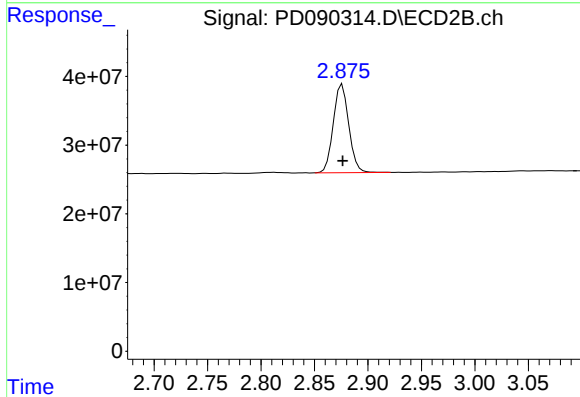


#1 Tetrachloro-m-xylene

R.T.: 2.876 min
Delta R.T.: 0.000 min
Response: 129732608
Conc: 5.78 ng/ml

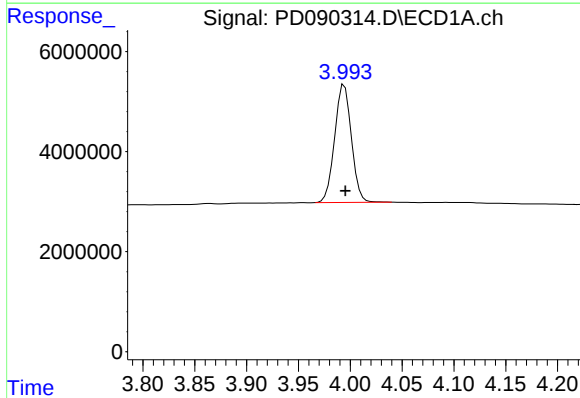


#2 alpha-BHC

R.T.: 3.994 min
Delta R.T.: 0.000 min
Response: 26533982
Conc: 5.01 ng/ml

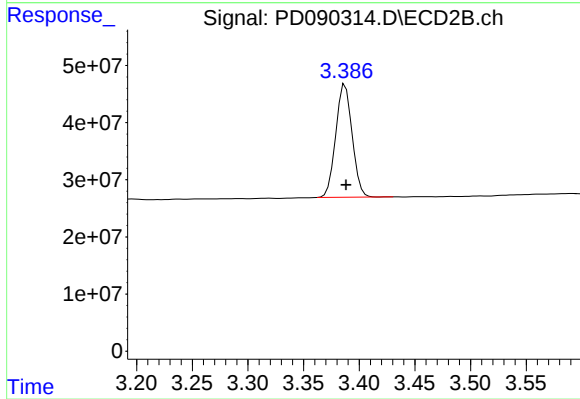

#2 alpha-BHC


R.T.: 3.388 min
Delta R.T.: 0.000 min
Response: 202962011
Conc: 5.56 ng/ml

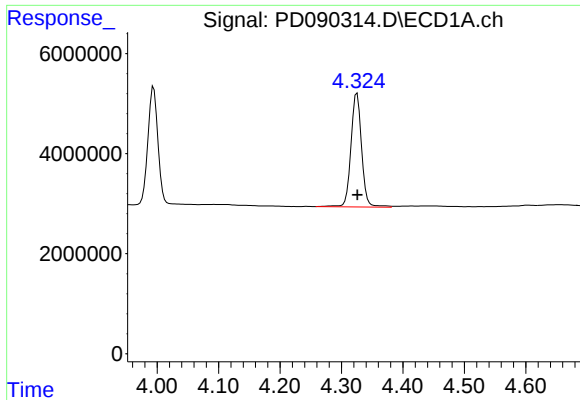

#3 gamma-BHC (Lindane)


R.T.: 4.325 min
Delta R.T.: 0.000 min
Response: 27401589
Conc: 5.28 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA1085

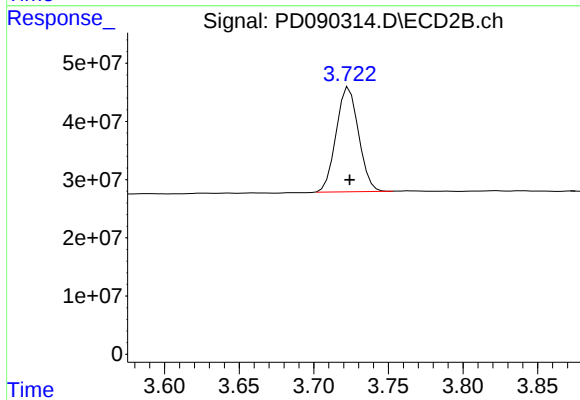


#3 gamma-BHC (Lindane)

R.T.: 3.724 min
Delta R.T.: 0.000 min
Response: 188104085
Conc: 5.63 ng/ml

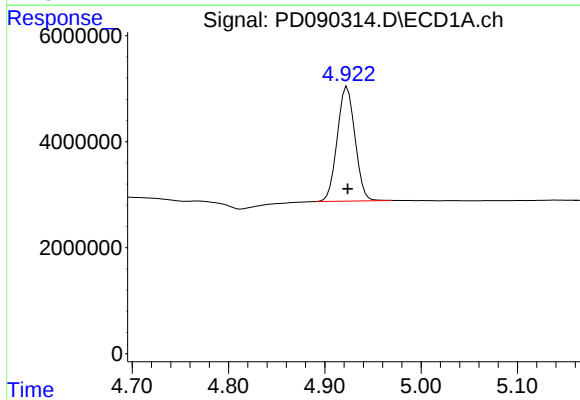


#4 Heptachlor

R.T.: 4.923 min
Delta R.T.: 0.000 min
Response: 27661642
Conc: 5.32 ng/ml

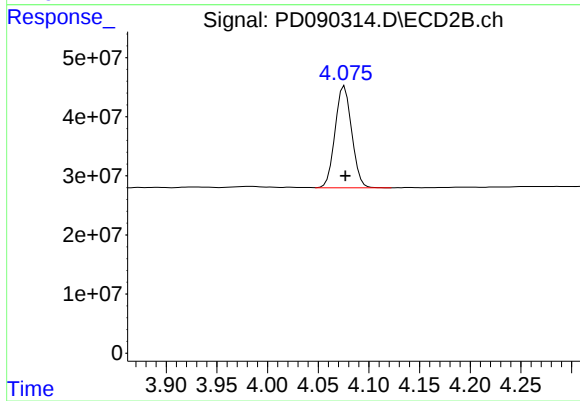

#4 Heptachlor


R.T.: 4.076 min
Delta R.T.: 0.000 min
Response: 196814562
Conc: 5.65 ng/ml

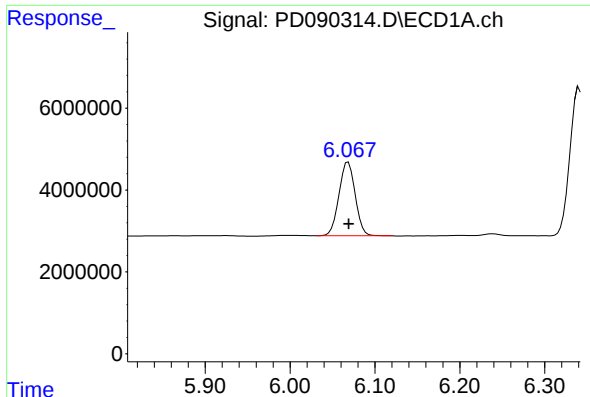

#9 Endosulfan I


R.T.: 6.069 min
Delta R.T.: 0.000 min
Response: 23885822
Conc: 5.39 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA1085

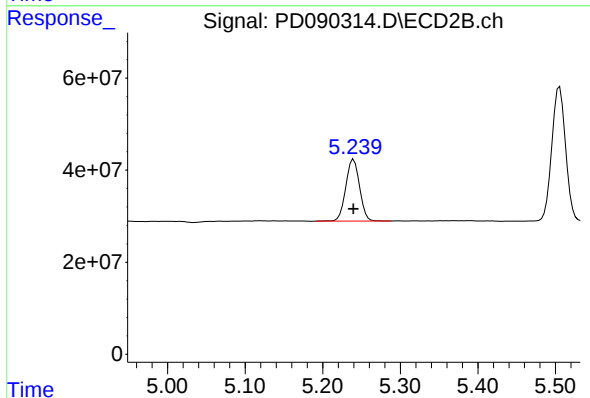


#9 Endosulfan I

R.T.: 5.240 min
Delta R.T.: 0.000 min
Response: 165820677
Conc: 5.61 ng/ml

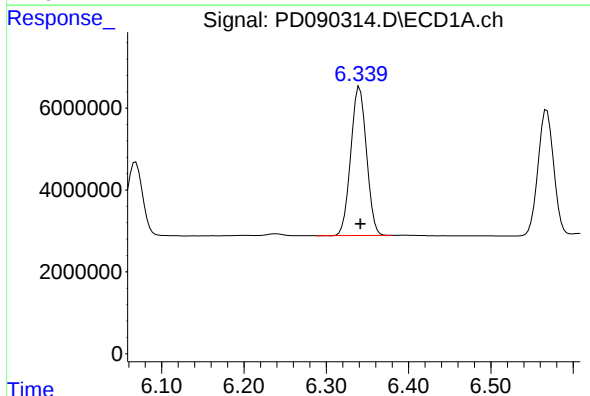


#13 Dieldrin

R.T.: 6.341 min
Delta R.T.: 0.000 min
Response: 48232363
Conc: 10.16 ng/ml

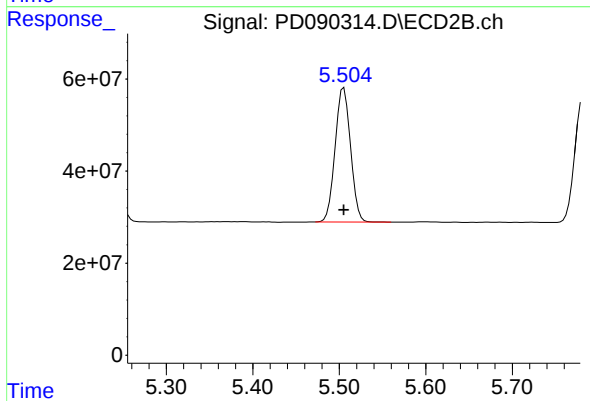

#13 Dieldrin


R.T.: 5.505 min
Delta R.T.: 0.000 min
Response: 359586252
Conc: 11.22 ng/ml

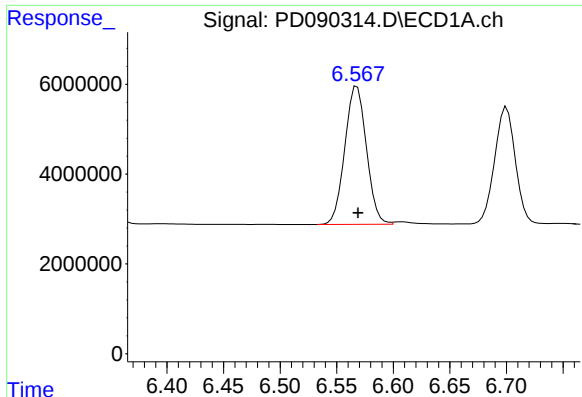

#14 Endrin


R.T.: 6.568 min
Delta R.T.: 0.000 min
Response: 40893658
Conc: 10.25 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA1085

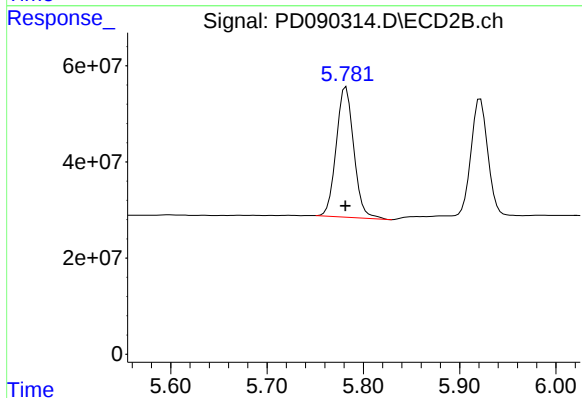


#14 Endrin

R.T.: 5.782 min
Delta R.T.: 0.000 min
Response: 341631748
Conc: 11.62 ng/ml

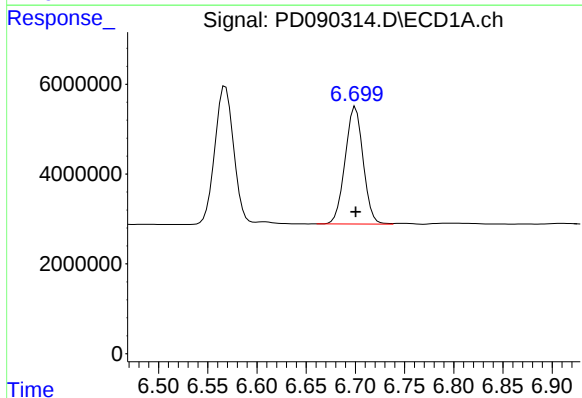


#16 4,4'-DDD

R.T.: 6.700 min
Delta R.T.: 0.000 min
Response: 33293830
Conc: 10.05 ng/ml

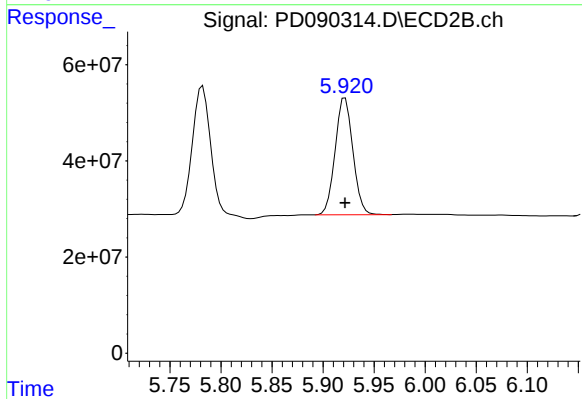

#16 4,4'-DDD


R.T.: 5.922 min
Delta R.T.: 0.000 min
Response: 294295630
Conc: 11.17 ng/ml

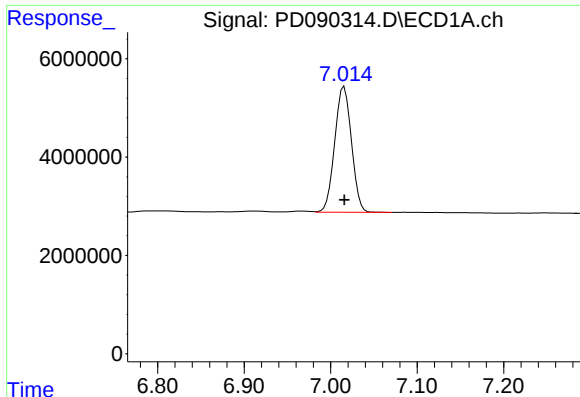

#17 4,4'-DDT


R.T.: 7.016 min
Delta R.T.: 0.000 min
Response: 34249112
Conc: 9.97 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA1085

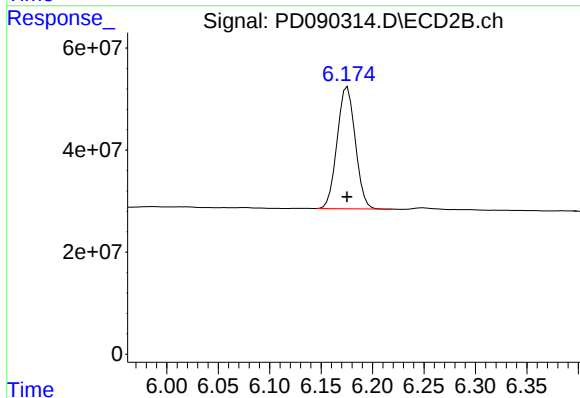


#17 4,4'-DDT

R.T.: 6.176 min
Delta R.T.: 0.000 min
Response: 293460693
Conc: 10.72 ng/ml

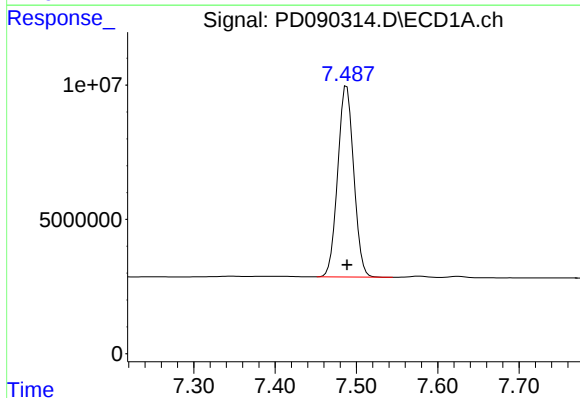


#20 Methoxychlor

R.T.: 7.488 min
Delta R.T.: 0.000 min
Response: 97255604
Conc: 52.85 ng/ml

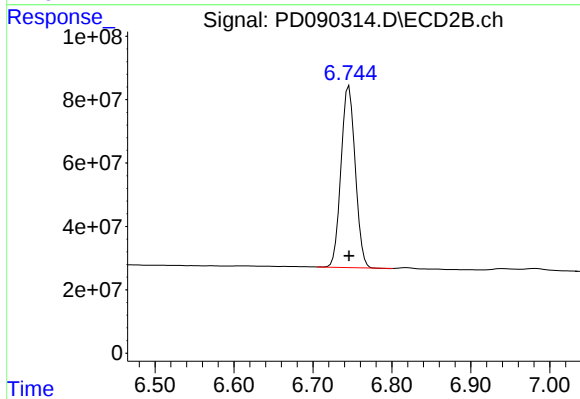

#20 Methoxychlor


R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 716247755
Conc: 58.86 ng/ml

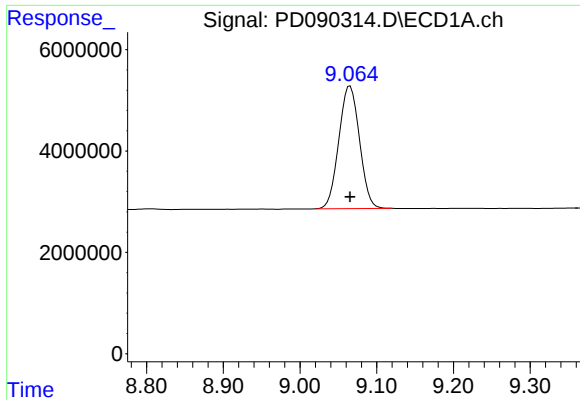

#27 Decachlorobiphenyl

R.T.: 9.065 min
Delta R.T.: 0.000 min
Response: 45394207
Conc: 11.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA1085

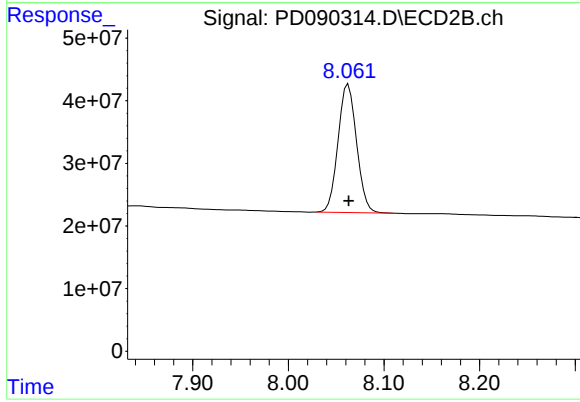

#27 Decachlorobiphenyl

R.T.: 8.063 min
Delta R.T.: 0.000 min
Response: 276383489
Conc: 11.31 ng/ml