

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091725\
 Data File : PD090316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2025 13:14
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA2087

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 07:33:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091725CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 18 07:32:47 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.876	27483773	241.5E6	10.767	10.762
27)	SA Decachlor...	9.065	8.063	84790632	508.2E6	21.508	20.792
Target Compounds							
2)	A alpha-BHC	3.995	3.388	53443749	389.8E6	10.092	10.677
3)	MA gamma-BHC...	4.326	3.724	52380939	359.8E6	10.094	10.766
4)	MA Heptachlor	4.924	4.076	53762109	373.8E6	10.340	10.730
9)	A Endosulfan I	6.069	5.240	46363267	311.4E6	10.454	10.532
13)	MA Dieldrin	6.341	5.505	95772231	678.9E6	20.172	21.193
14)	MA Endrin	6.569	5.782	80607348	641.4E6	20.213	21.810
16)	A 4,4'-DDD	6.700	5.922	66757699	556.4E6	20.161	21.112
17)	MA 4,4'-DDT	7.016	6.176	68209193	565.8E6	19.851	20.675
20)	A Methoxychlor	7.488	6.746	188.6E6	1322.8E6	102.466	108.698

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091725\
Data File : PD090316.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2025 13:14
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 07:33:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091725CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 18 07:32:47 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

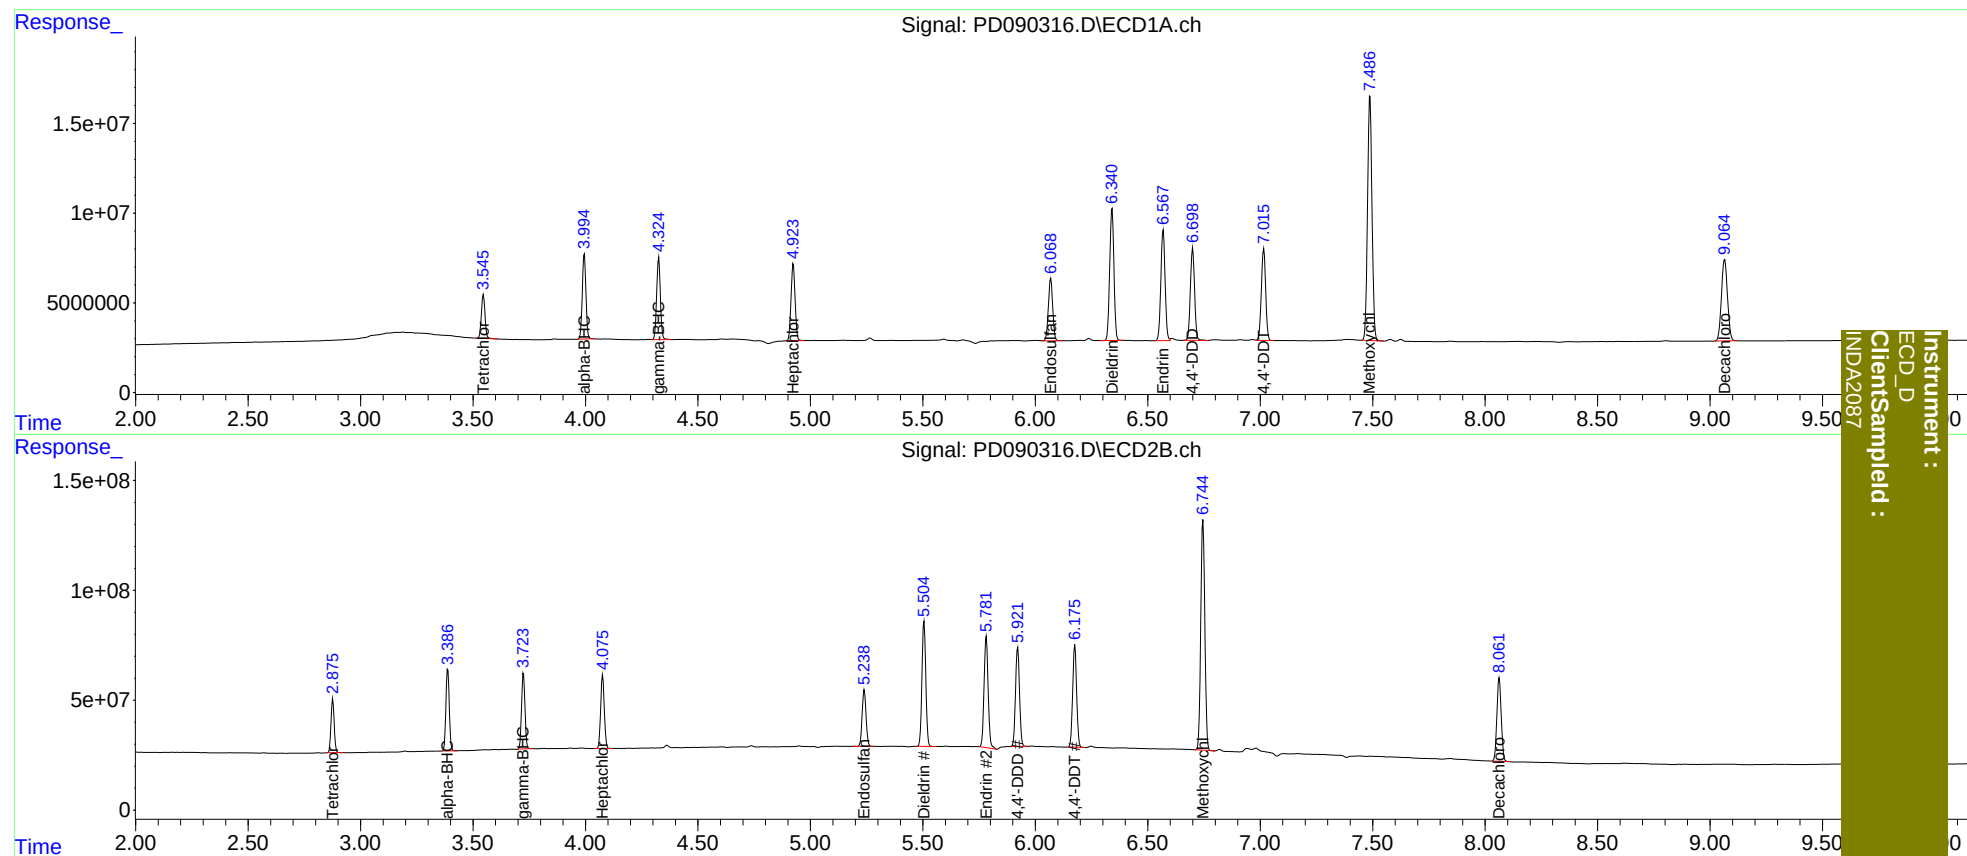


Instrument :
ECD_D
ClientSampled :
INDA2087

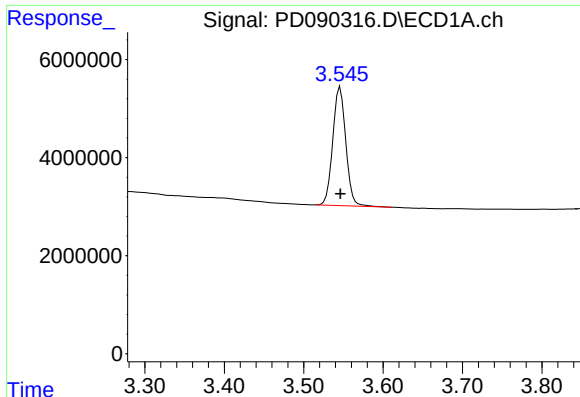

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 27483773
Conc: 10.77 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA2087

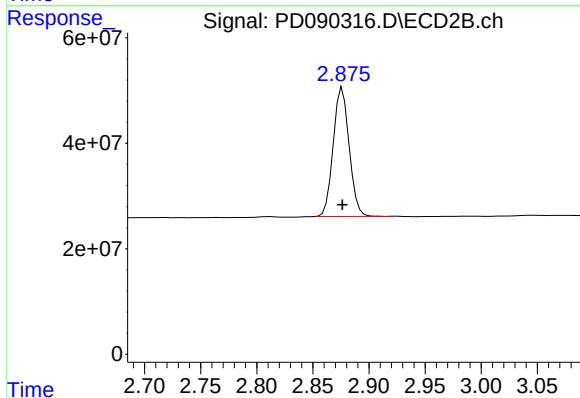


#1 Tetrachloro-m-xylene

R.T.: 2.876 min
Delta R.T.: 0.000 min
Response: 241476128
Conc: 10.76 ng/ml

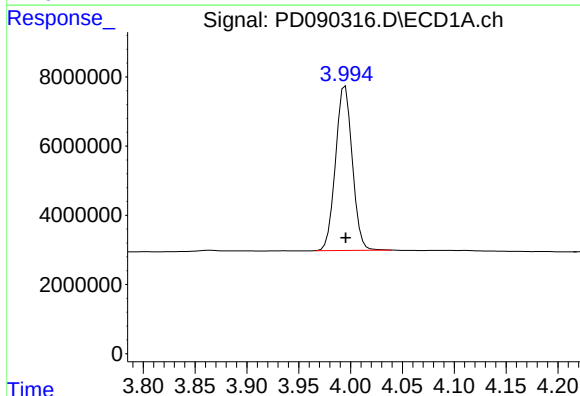


#2 alpha-BHC

R.T.: 3.995 min
Delta R.T.: 0.000 min
Response: 53443749
Conc: 10.09 ng/ml

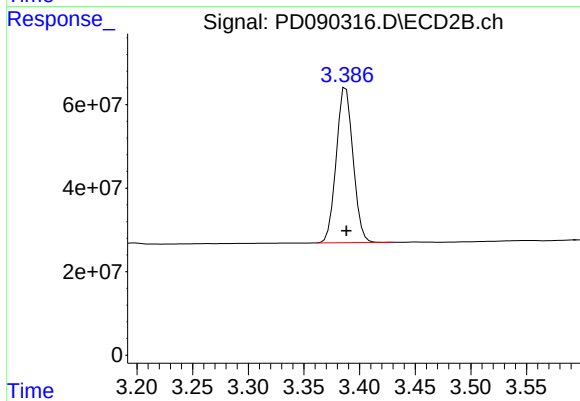

#2 alpha-BHC


R.T.: 3.388 min
Delta R.T.: 0.000 min
Response: 389842091
Conc: 10.68 ng/ml

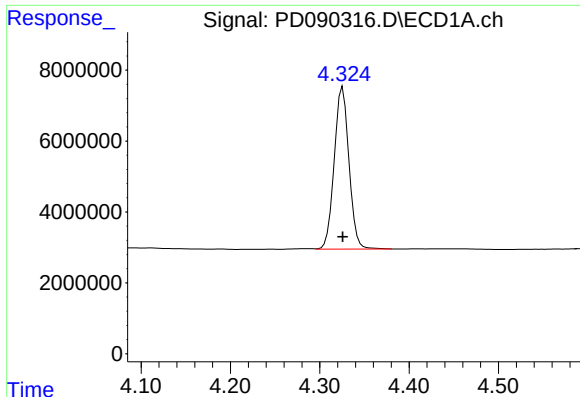

#3 gamma-BHC (Lindane)


R.T.: 4.326 min
Delta R.T.: 0.000 min
Response: 52380939
Conc: 10.09 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA2087

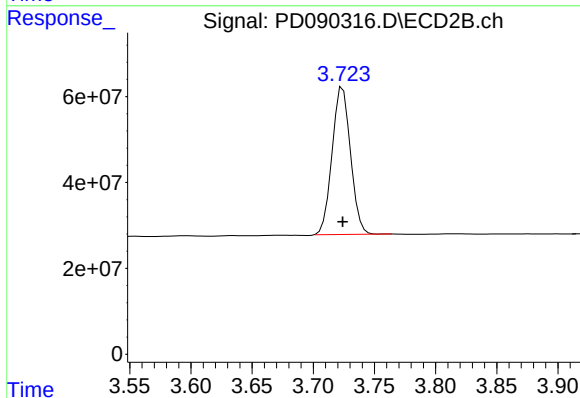


#3 gamma-BHC (Lindane)

R.T.: 3.724 min
Delta R.T.: 0.000 min
Response: 359794136
Conc: 10.77 ng/ml

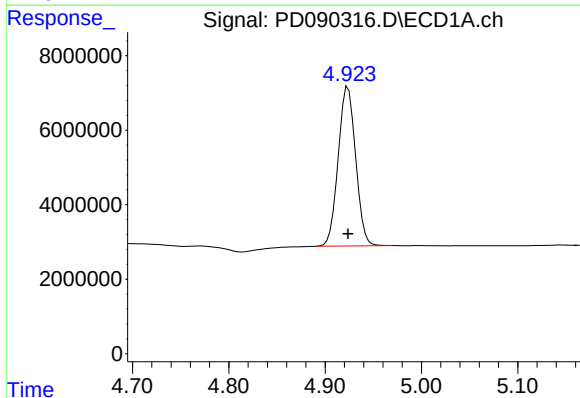


#4 Heptachlor

R.T.: 4.924 min
Delta R.T.: 0.000 min
Response: 53762109
Conc: 10.34 ng/ml

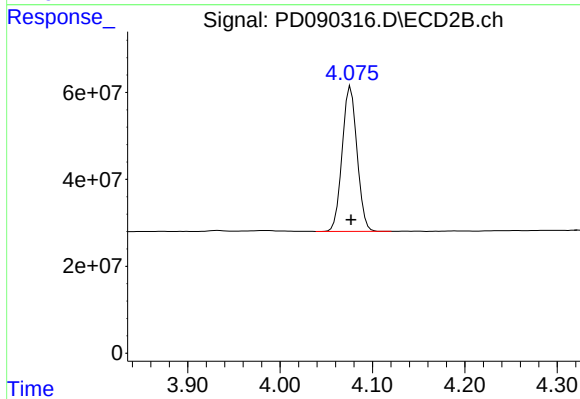

#4 Heptachlor


R.T.: 4.076 min
Delta R.T.: 0.000 min
Response: 373840720
Conc: 10.73 ng/ml

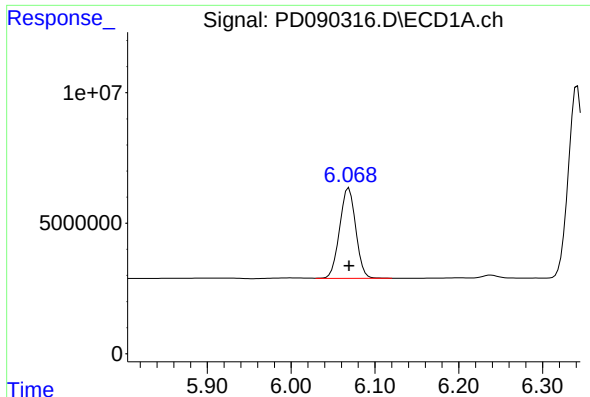

#9 Endosulfan I


R.T.: 6.069 min
Delta R.T.: 0.000 min
Response: 46363267
Conc: 10.45 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA2087

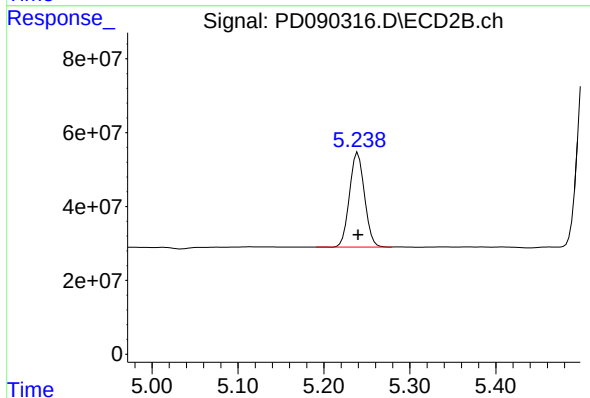


#9 Endosulfan I

R.T.: 5.240 min
Delta R.T.: 0.000 min
Response: 311351144
Conc: 10.53 ng/ml

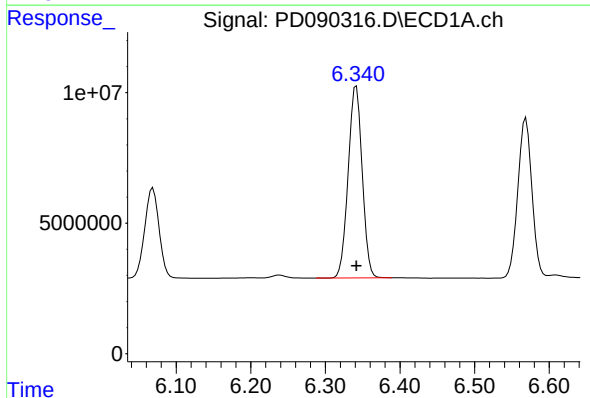


#13 Dieldrin

R.T.: 6.341 min
Delta R.T.: 0.000 min
Response: 95772231
Conc: 20.17 ng/ml

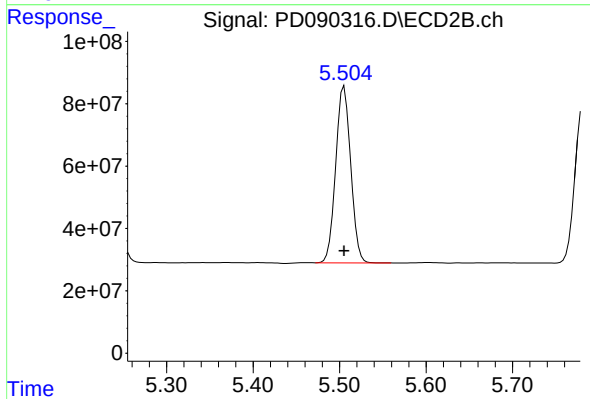

#13 Dieldrin


R.T.: 5.505 min
Delta R.T.: 0.000 min
Response: 678929702
Conc: 21.19 ng/ml

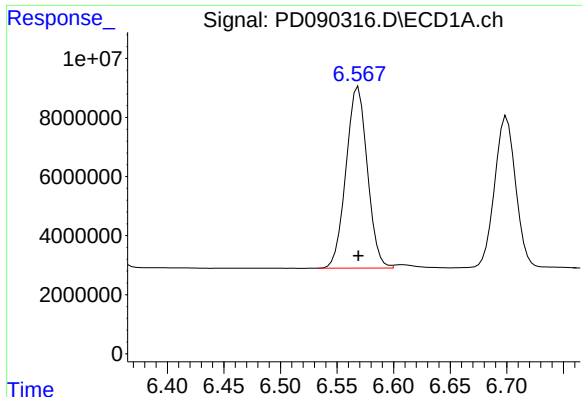

#14 Endrin


R.T.: 6.569 min
Delta R.T.: 0.000 min
Response: 80607348
Conc: 20.21 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA2087

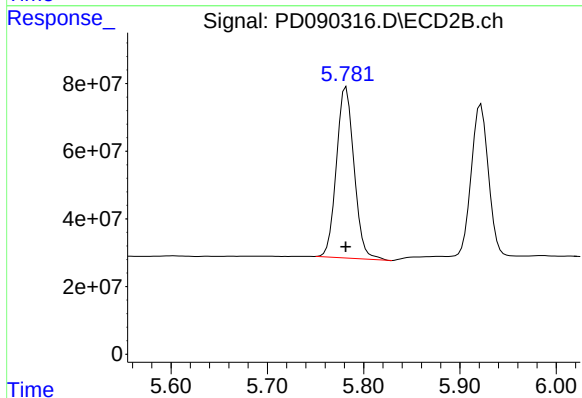


#14 Endrin

R.T.: 5.782 min
Delta R.T.: 0.000 min
Response: 641401372
Conc: 21.81 ng/ml

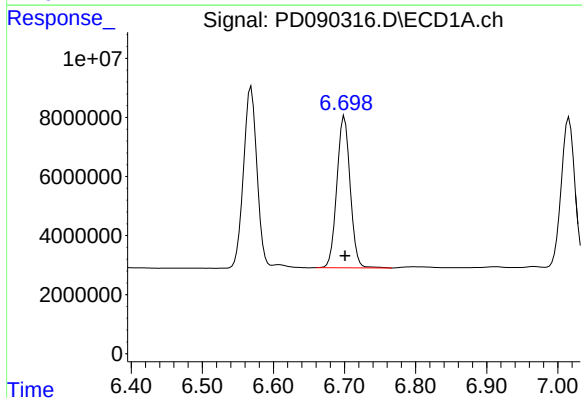


#16 4,4'-DDD

R.T.: 6.700 min
Delta R.T.: 0.000 min
Response: 66757699
Conc: 20.16 ng/ml

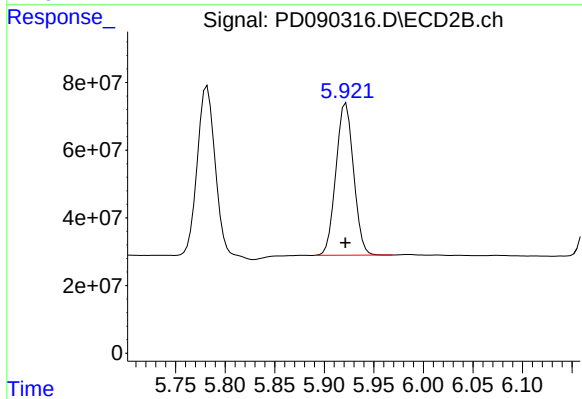

#16 4,4'-DDD


R.T.: 5.922 min
Delta R.T.: 0.000 min
Response: 556354152
Conc: 21.11 ng/ml

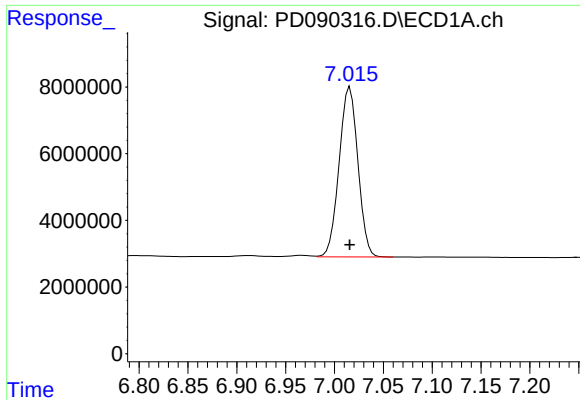

#17 4,4'-DDT


R.T.: 7.016 min
Delta R.T.: 0.000 min
Response: 68209193
Conc: 19.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA2087

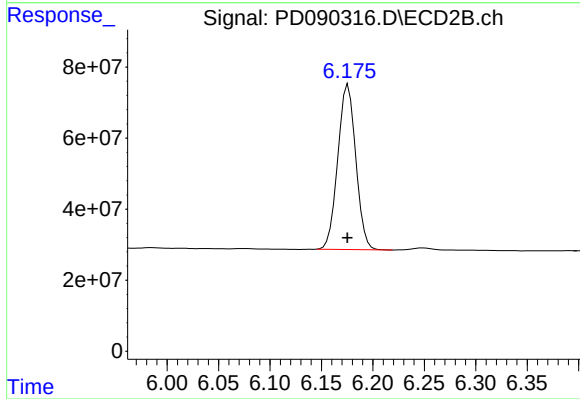


#17 4,4'-DDT

R.T.: 6.176 min
Delta R.T.: 0.000 min
Response: 565757850
Conc: 20.67 ng/ml

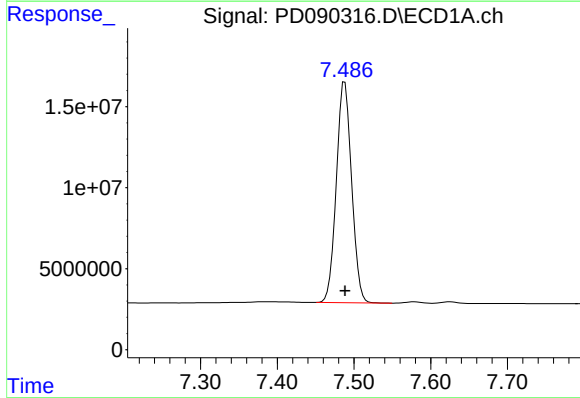


#20 Methoxychlor

R.T.: 7.488 min
Delta R.T.: 0.000 min
Response: 188569980
Conc: 102.47 ng/ml

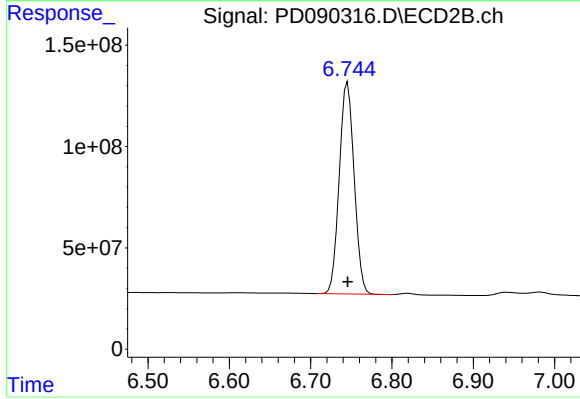

#20 Methoxychlor


R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 1322820090
Conc: 108.70 ng/ml

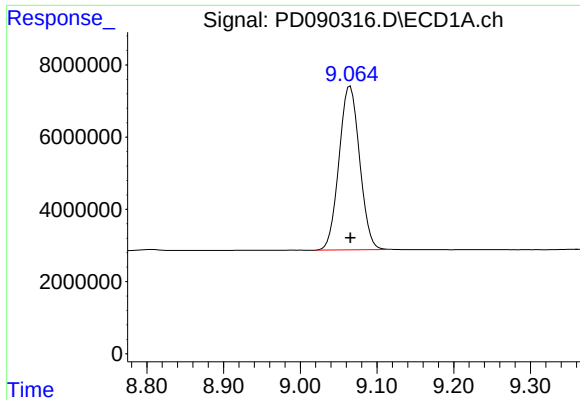

#27 Decachlorobiphenyl

R.T.: 9.065 min
Delta R.T.: 0.000 min
Response: 84790632
Conc: 21.51 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA2087

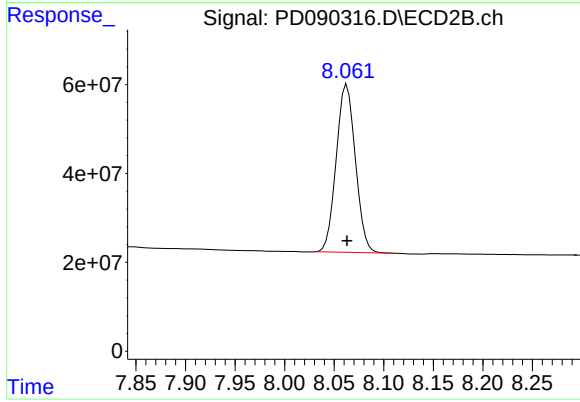

#27 Decachlorobiphenyl

R.T.: 8.063 min
Delta R.T.: 0.000 min
Response: 508158543
Conc: 20.79 ng/ml