

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091725\
 Data File : PD090318.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2025 13:41
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA3089

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 07:34:06 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091725CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 18 07:32:47 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.876	51049666	448.7E6	20.000	20.000
27)	SA Decachlor...	9.065	8.063	157.7E6	977.6E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.995	3.388	105.9E6	730.3E6	20.000	20.000
3)	MA gamma-BHC...	4.326	3.724	103.8E6	668.4E6	20.000	20.000
4)	MA Heptachlor	4.924	4.077	104.0E6	696.8E6	20.000	20.000
9)	A Endosulfan I	6.069	5.240	88695355	591.3E6	20.000	20.000
13)	MA Dieldrin	6.342	5.505	189.9E6	1281.4E6	40.000	40.000
14)	MA Endrin	6.569	5.782	159.5E6	1176.3E6	40.000	40.000
16)	A 4,4'-DDD	6.700	5.922	132.4E6	1054.1E6	40.000	40.000
17)	MA 4,4'-DDT	7.016	6.175	137.4E6	1094.6E6	40.000	40.000
20)	A Methoxychlor	7.488	6.746	368.1E6	2433.9E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091725\
Data File : PD090318.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2025 13:41
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 07:34:06 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091725CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 18 07:32:47 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

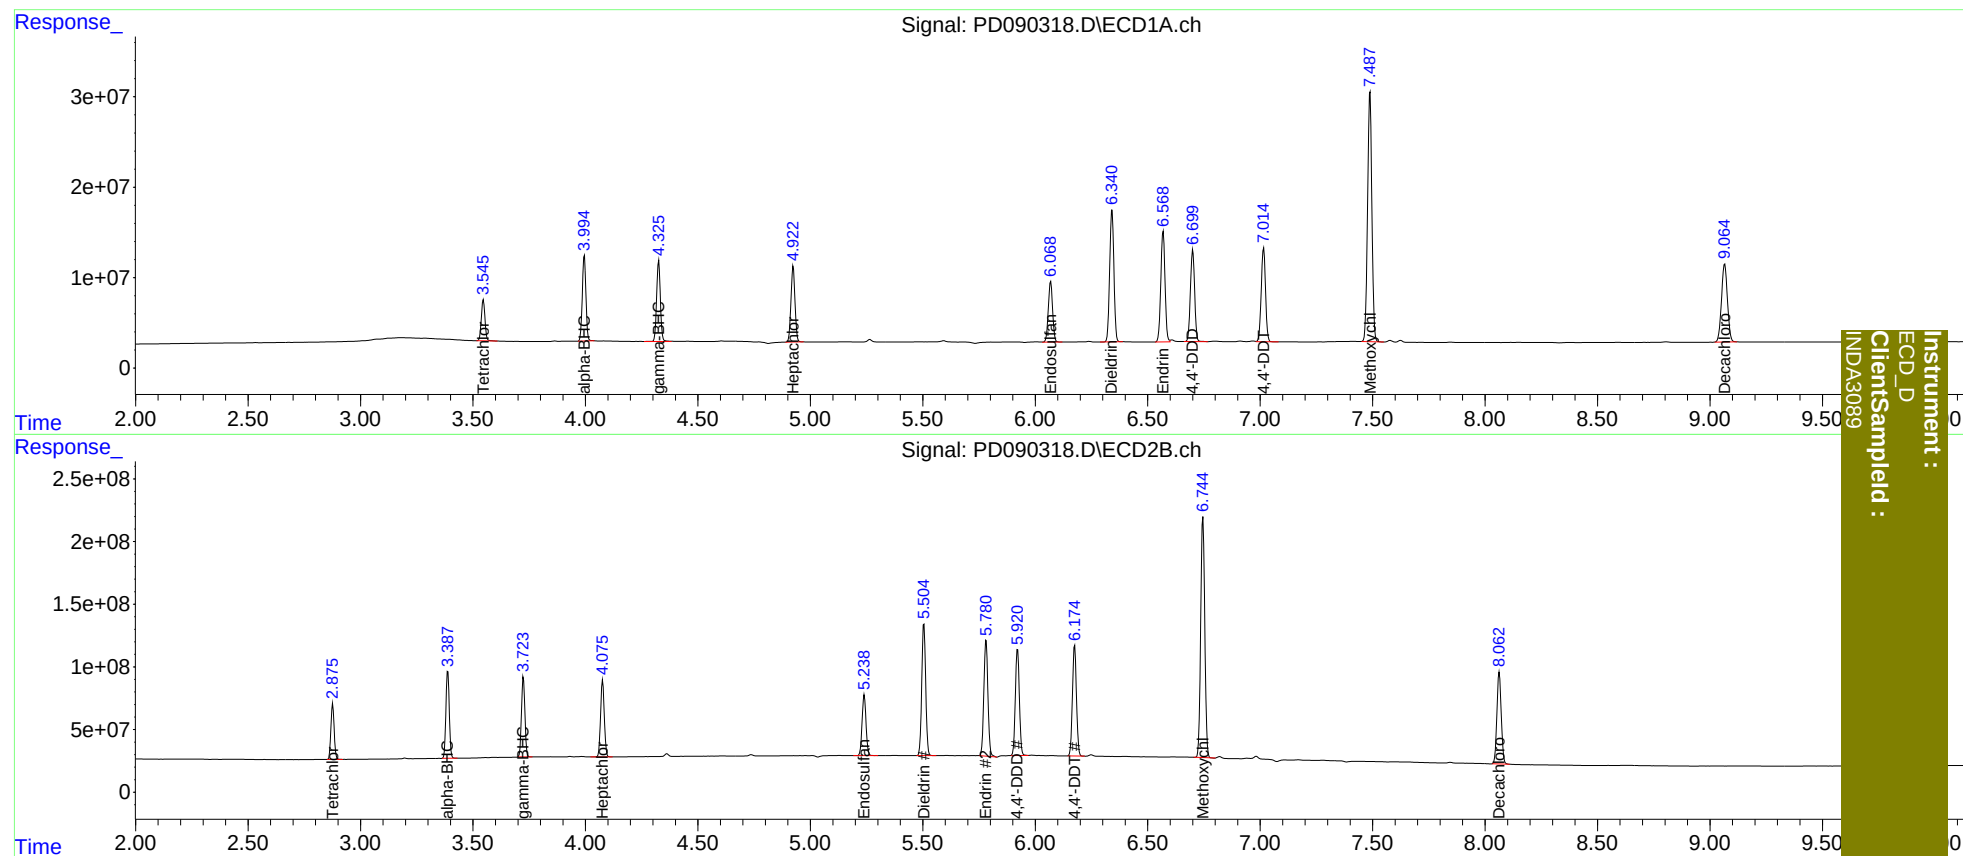


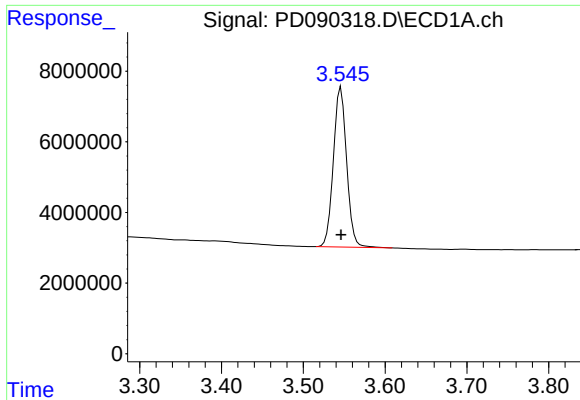

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 51049666
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3089

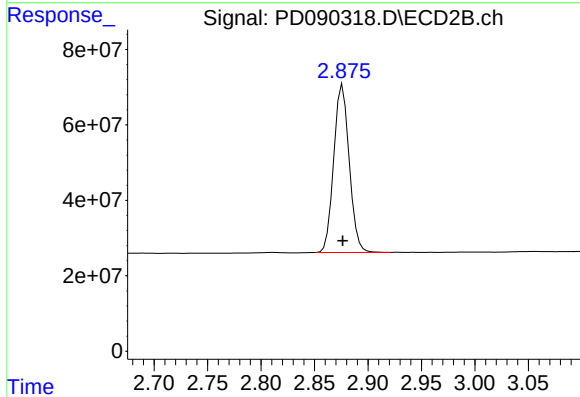


#1 Tetrachloro-m-xylene

R.T.: 2.876 min
Delta R.T.: 0.000 min
Response: 448743008
Conc: 20.00 ng/ml

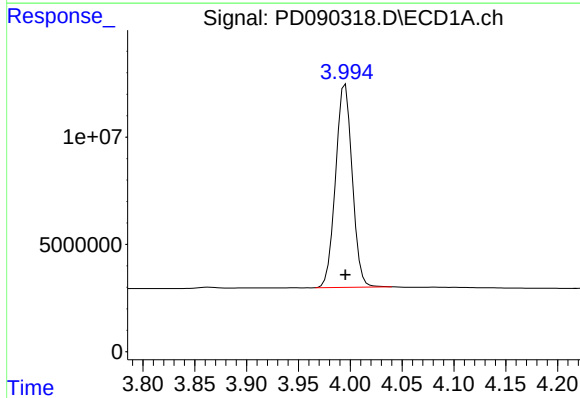


#2 alpha-BHC

R.T.: 3.995 min
Delta R.T.: 0.000 min
Response: 105916542
Conc: 20.00 ng/ml

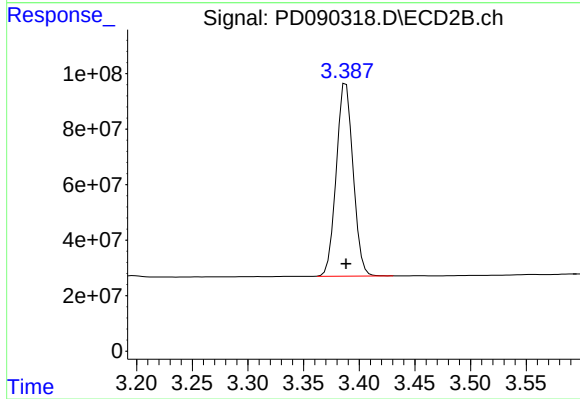

#2 alpha-BHC


R.T.: 3.388 min
Delta R.T.: 0.000 min
Response: 730263605
Conc: 20.00 ng/ml

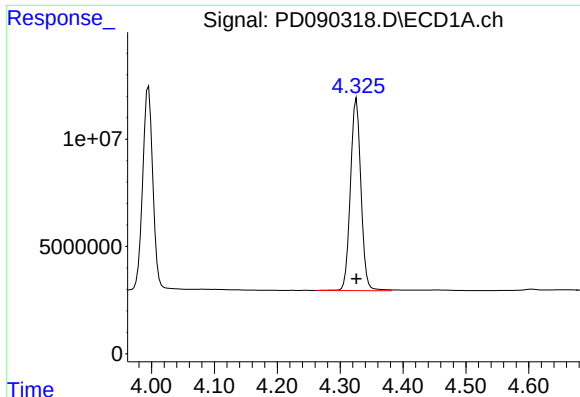

#3 gamma-BHC (Lindane)


R.T.: 4.326 min
Delta R.T.: 0.000 min
Response: 103782055
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3089

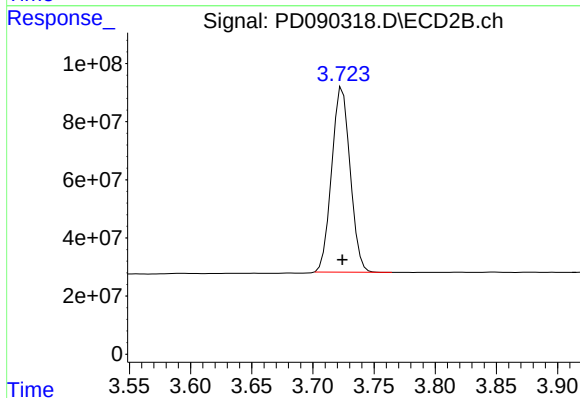


#3 gamma-BHC (Lindane)

R.T.: 3.724 min
Delta R.T.: 0.000 min
Response: 668366564
Conc: 20.00 ng/ml

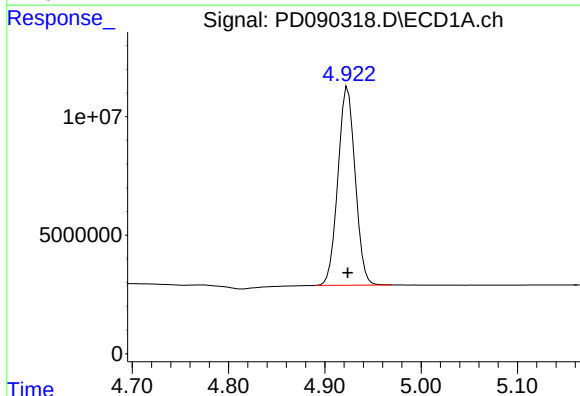


#4 Heptachlor

R.T.: 4.924 min
Delta R.T.: 0.000 min
Response: 103987426
Conc: 20.00 ng/ml

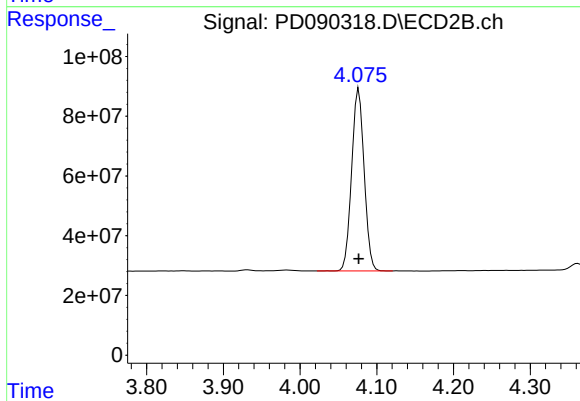

#4 Heptachlor


R.T.: 4.077 min
Delta R.T.: 0.000 min
Response: 696791045
Conc: 20.00 ng/ml

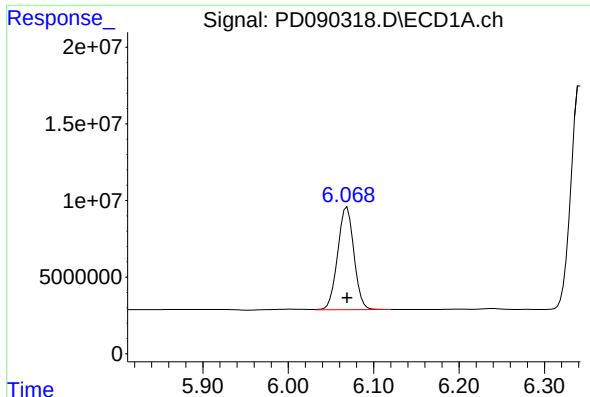

#9 Endosulfan I


R.T.: 6.069 min
Delta R.T.: 0.000 min
Response: 88695355
Conc: 20.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3089

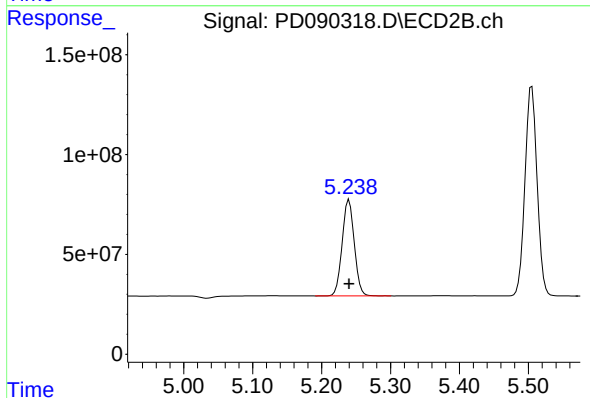


#9 Endosulfan I

R.T.: 5.240 min
Delta R.T.: 0.000 min
Response: 591273141
Conc: 20.00 ng/ml

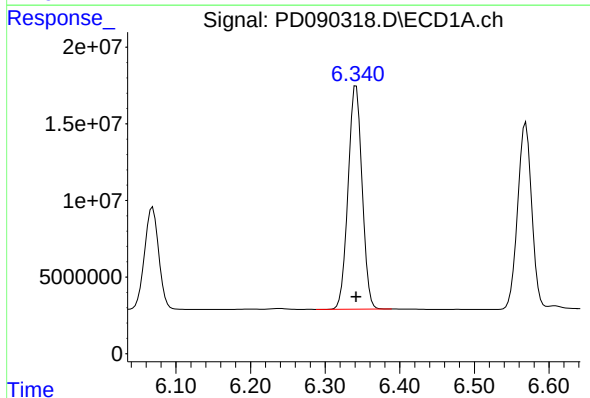


#13 Dieldrin

R.T.: 6.342 min
Delta R.T.: 0.000 min
Response: 189912268
Conc: 40.00 ng/ml

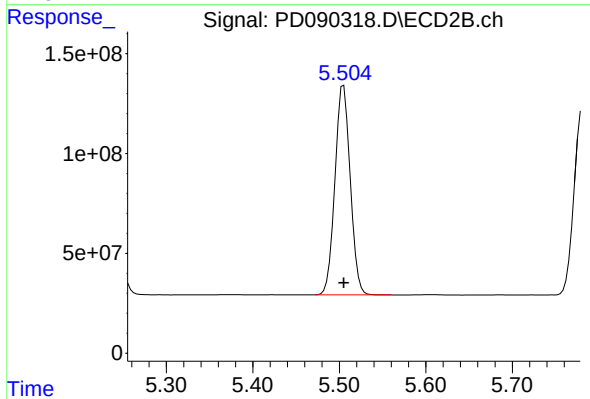

#13 Dieldrin


R.T.: 5.505 min
Delta R.T.: 0.000 min
Response: 1281432093
Conc: 40.00 ng/ml

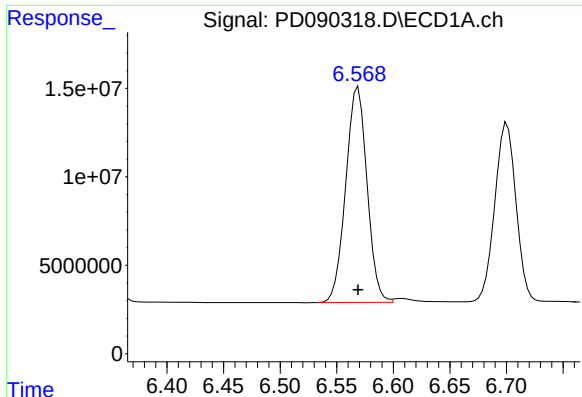

#14 Endrin


R.T.: 6.569 min
Delta R.T.: 0.000 min
Response: 159511993
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3089

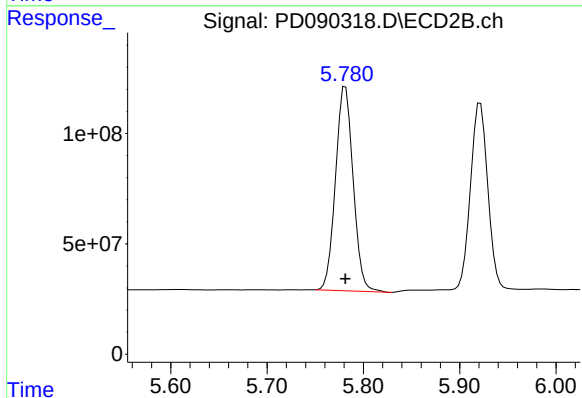


#14 Endrin

R.T.: 5.782 min
Delta R.T.: 0.000 min
Response: 1176342254
Conc: 40.00 ng/ml

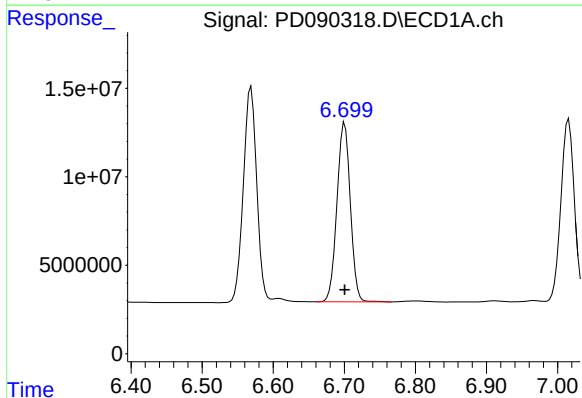


#16 4,4'-DDD

R.T.: 6.700 min
Delta R.T.: 0.000 min
Response: 132449004
Conc: 40.00 ng/ml

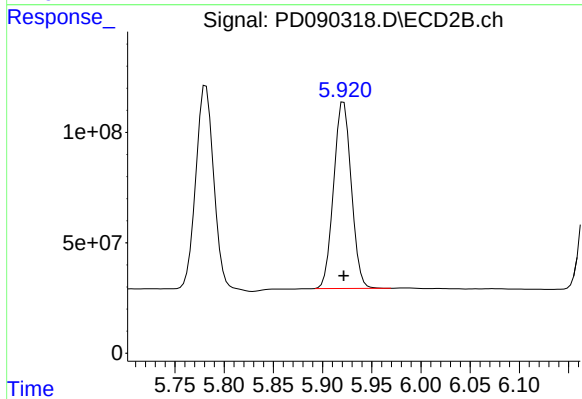

#16 4,4'-DDD


R.T.: 5.922 min
Delta R.T.: 0.000 min
Response: 1054081132
Conc: 40.00 ng/ml

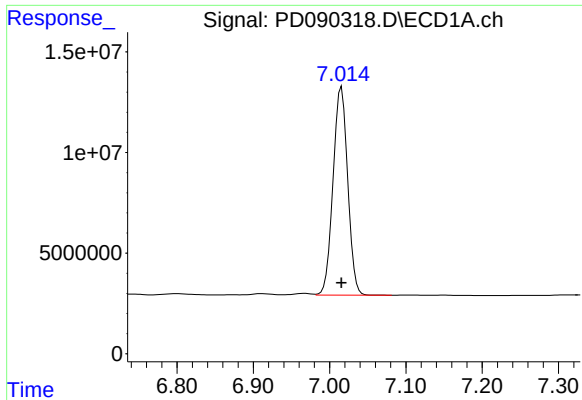

#17 4,4'-DDT


R.T.: 7.016 min
Delta R.T.: 0.000 min
Response: 137444337
Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3089

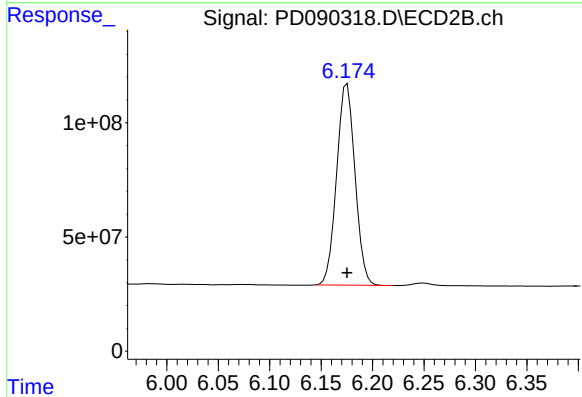


#17 4,4'-DDT

R.T.: 6.175 min
Delta R.T.: 0.000 min
Response: 1094597215
Conc: 40.00 ng/ml

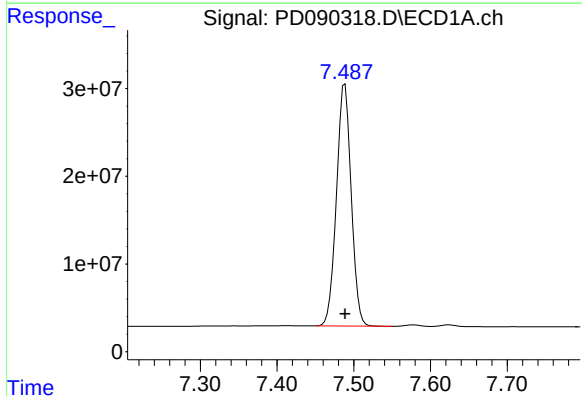


#20 Methoxychlor

R.T.: 7.488 min
Delta R.T.: 0.000 min
Response: 368063957
Conc: 200.00 ng/ml

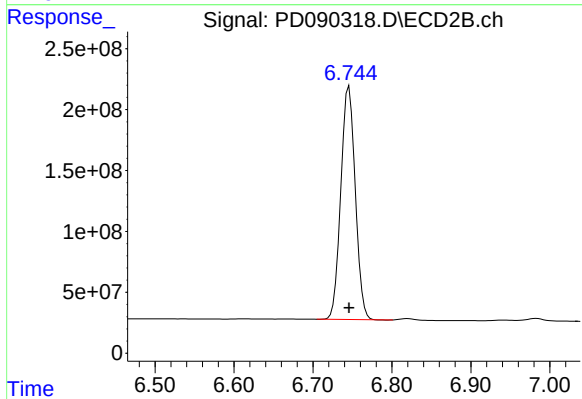

#20 Methoxychlor

R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 2433932049
Conc: 200.00 ng/ml

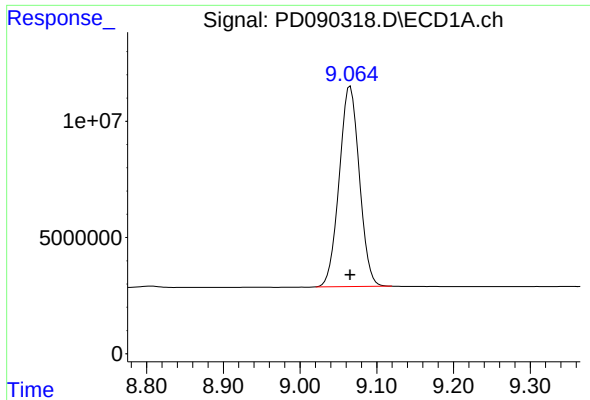

#27 Decachlorobiphenyl


R.T.: 9.065 min

Delta R.T.: 0.000 min

Response: 157689795

Conc: 40.00 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA3089

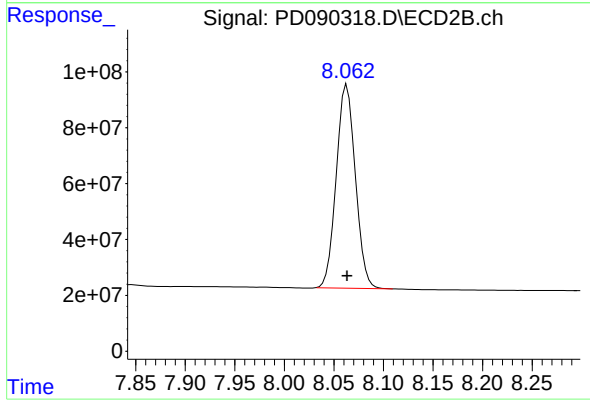

#27 Decachlorobiphenyl

R.T.: 8.063 min

Delta R.T.: 0.000 min

Response: 977602287

Conc: 40.00 ng/ml