

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091725\
 Data File : PD090320.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2025 14:09
 Operator : AR\AJ
 Sample : INDA401
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA4091

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 07:34:14 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091725CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 18 07:32:47 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.877	97847084	837.8E6	38.334	37.338
27)	SA Decachlor...	9.066	8.063	292.7E6	1849.8E6	74.236	75.686
Target Compounds							
2)	A alpha-BHC	3.995	3.388	219.3E6	1388.1E6	41.419	38.015
3)	MA gamma-BHC...	4.326	3.724	213.1E6	1272.2E6	41.060	38.068
4)	MA Heptachlor	4.924	4.076	197.9E6	1295.8E6	38.063	37.193
9)	A Endosulfan I	6.069	5.240	169.4E6	1070.2E6	38.202	36.199
13)	MA Dieldrin	6.342	5.505	377.2E6	2363.8E6	79.442	73.786
14)	MA Endrin	6.570	5.782	318.9E6	2210.4E6	79.965	75.161
16)	A 4,4'-DDD	6.701	5.922	264.9E6	1936.3E6	80.013	73.477
17)	MA 4,4'-DDT	7.016	6.175	277.3E6	2050.6E6	80.693	74.936
20)	A Methoxychlor	7.489	6.746	716.3E6	4250.8E6	389.250	349.296


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091725\
Data File : PD090320.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2025 14:09
Operator : AR\AJ
Sample : INDA401
Misc :
ALS Vial : 15 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 07:34:14 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091725CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 18 07:32:47 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

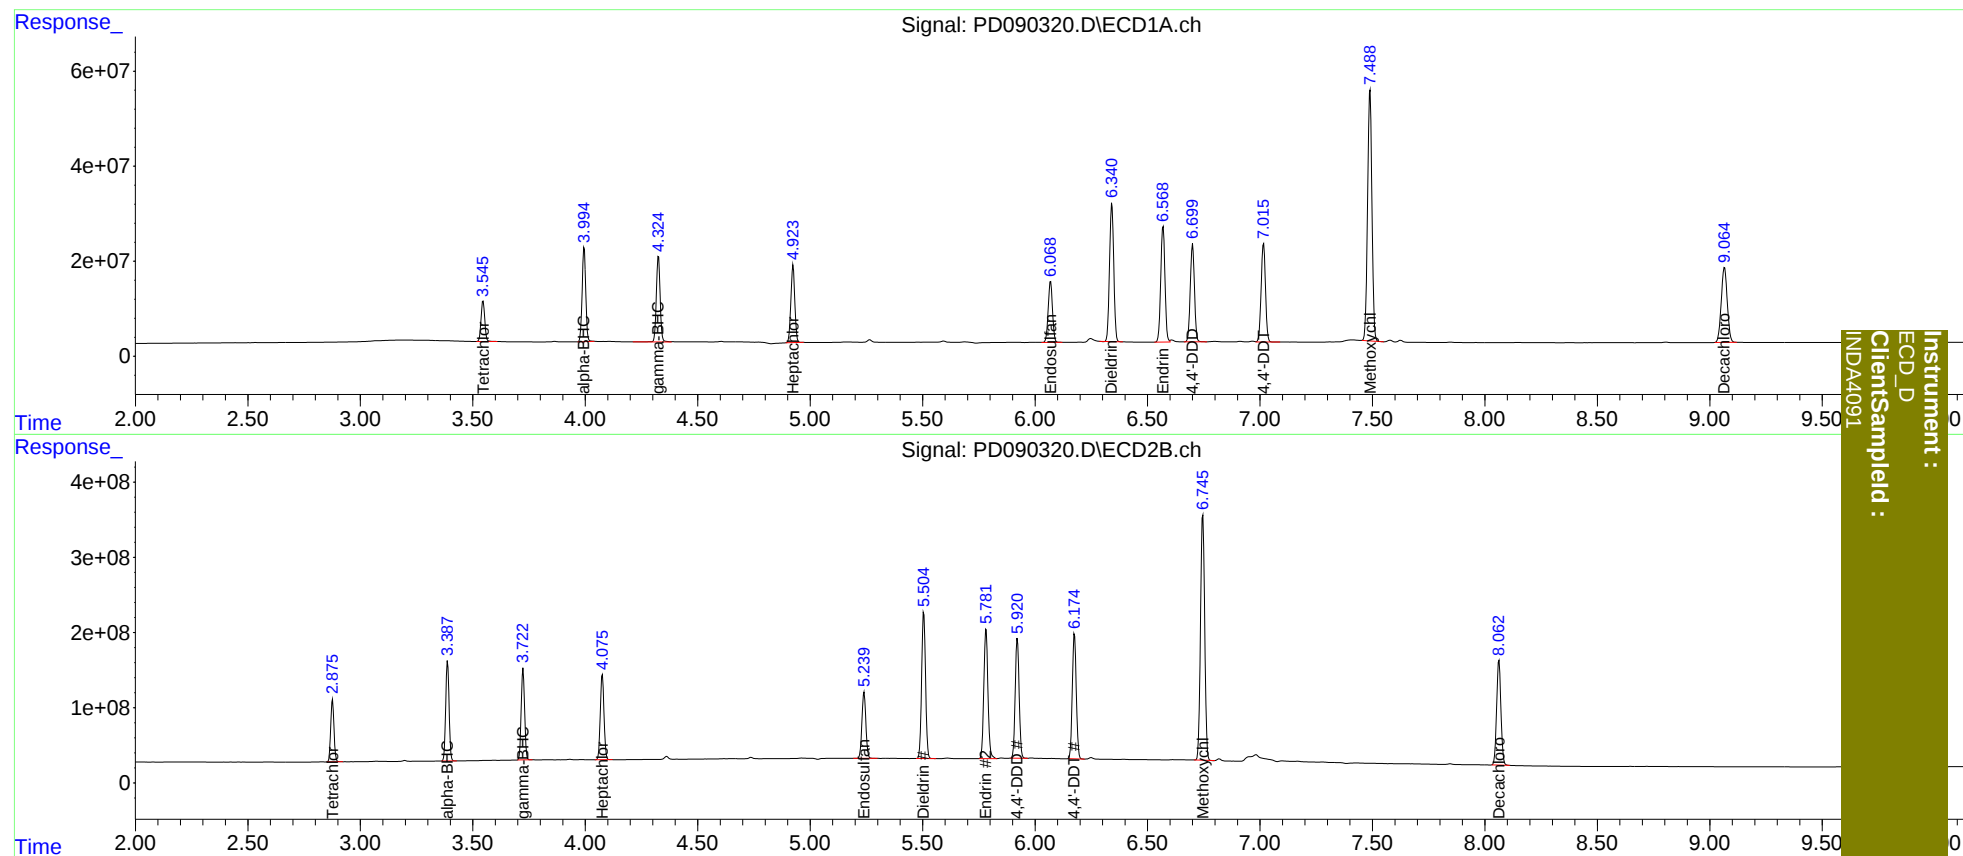


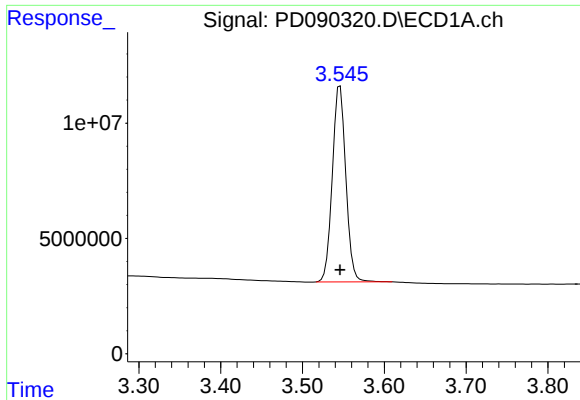

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 97847084
Conc: 38.33 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4091

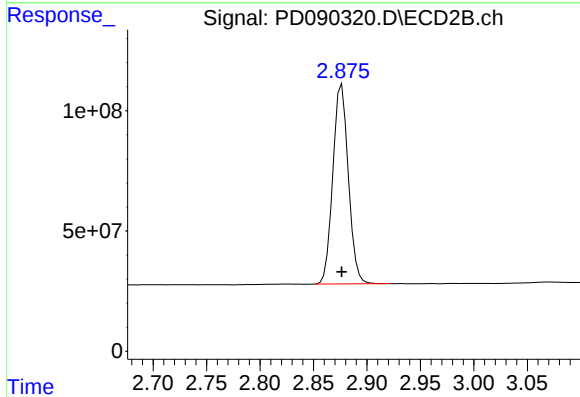


#1 Tetrachloro-m-xylene

R.T.: 2.877 min
Delta R.T.: 0.000 min
Response: 837766012
Conc: 37.34 ng/ml

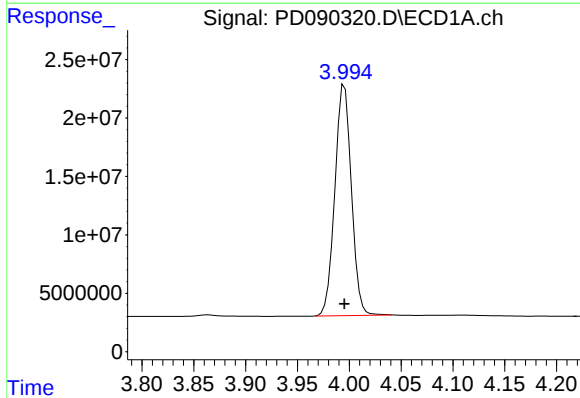


#2 alpha-BHC

R.T.: 3.995 min
Delta R.T.: 0.000 min
Response: 219348357
Conc: 41.42 ng/ml

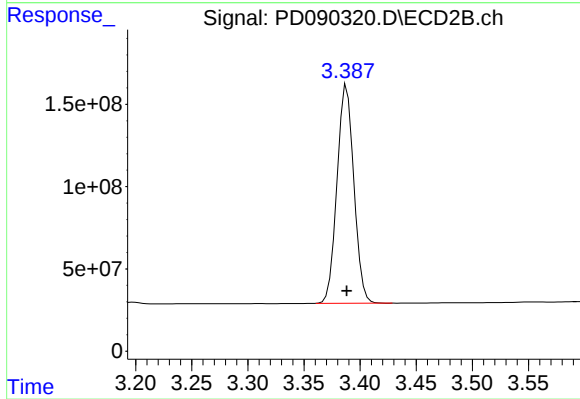

#2 alpha-BHC


R.T.: 3.388 min
Delta R.T.: 0.000 min
Response: 1388055888
Conc: 38.02 ng/ml

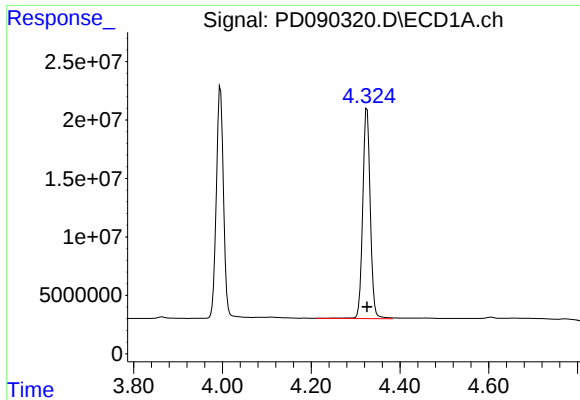

#3 gamma-BHC (Lindane)


R.T.: 4.326 min
Delta R.T.: 0.000 min
Response: 213064347
Conc: 41.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4091

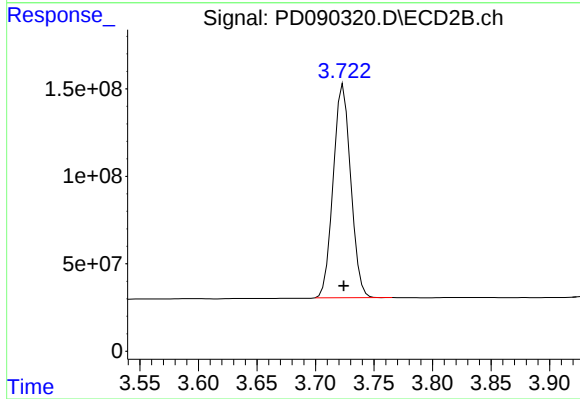


#3 gamma-BHC (Lindane)

R.T.: 3.724 min
Delta R.T.: 0.000 min
Response: 1272180409
Conc: 38.07 ng/ml

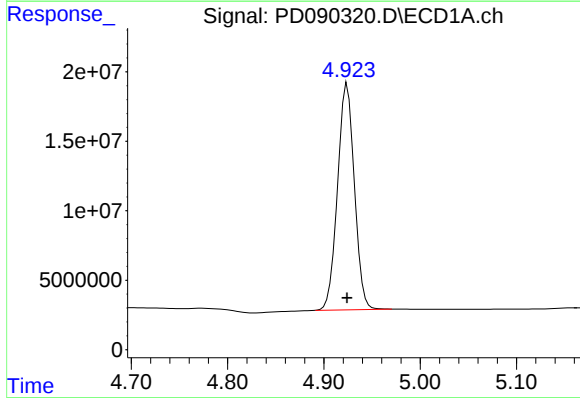


#4 Heptachlor

R.T.: 4.924 min
Delta R.T.: 0.000 min
Response: 197903901
Conc: 38.06 ng/ml

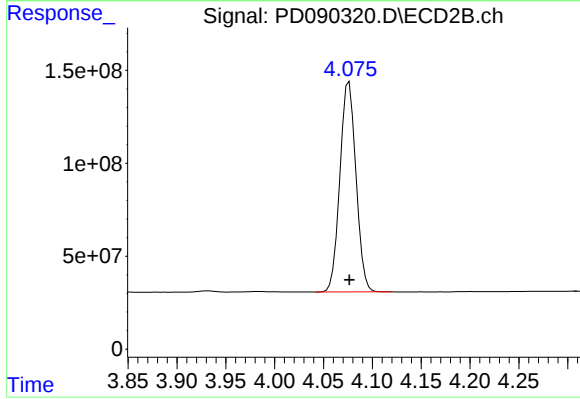

#4 Heptachlor


R.T.: 4.076 min
Delta R.T.: 0.000 min
Response: 1295786844
Conc: 37.19 ng/ml

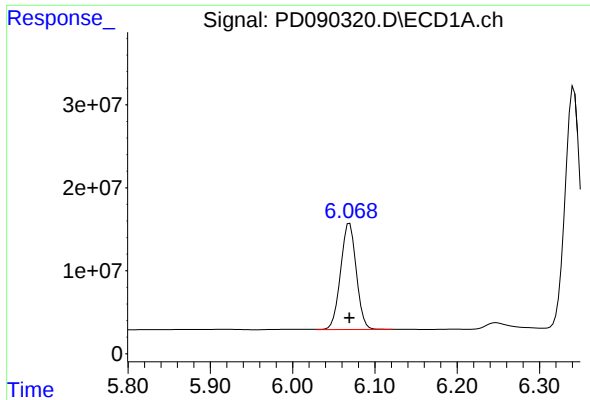

#9 Endosulfan I


R.T.: 6.069 min
Delta R.T.: 0.000 min
Response: 169418294
Conc: 38.20 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4091

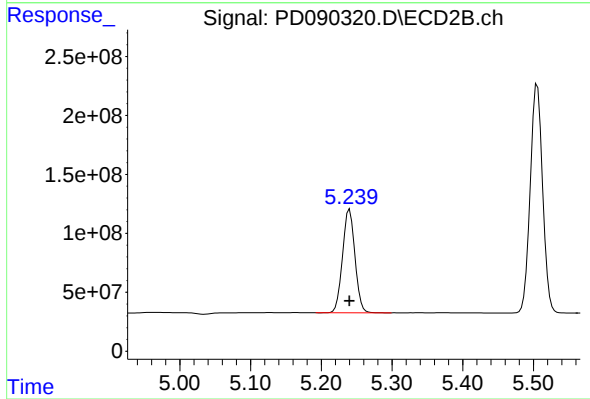


#9 Endosulfan I

R.T.: 5.240 min
Delta R.T.: 0.000 min
Response: 1070172105
Conc: 36.20 ng/ml

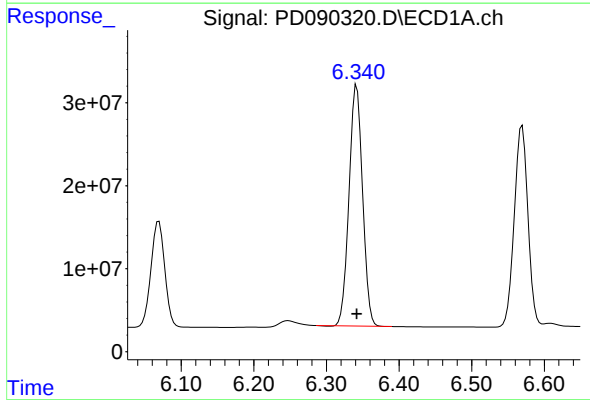


#13 Dieldrin

R.T.: 6.342 min
Delta R.T.: 0.000 min
Response: 377177131
Conc: 79.44 ng/ml

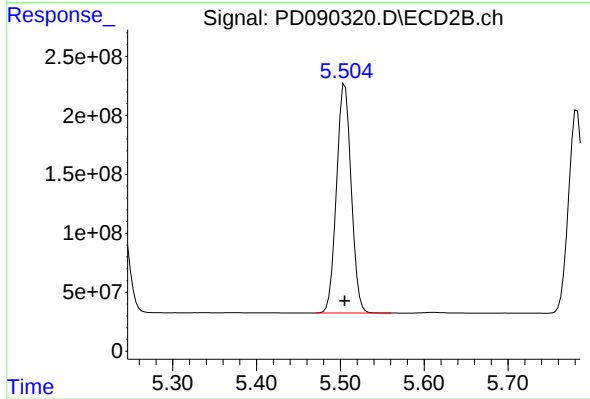

#13 Dieldrin


R.T.: 5.505 min
Delta R.T.: 0.000 min
Response: 2363789287
Conc: 73.79 ng/ml

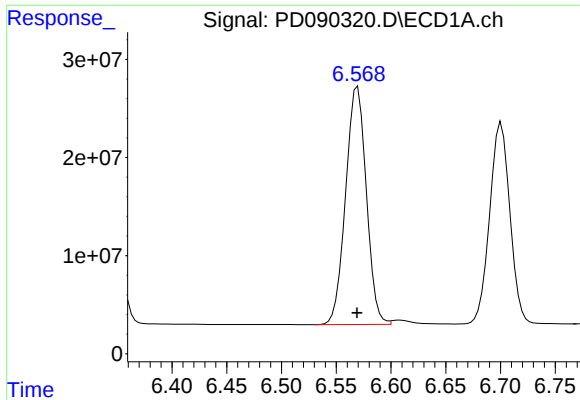

#14 Endrin


R.T.: 6.570 min
Delta R.T.: 0.000 min
Response: 318883166
Conc: 79.96 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4091

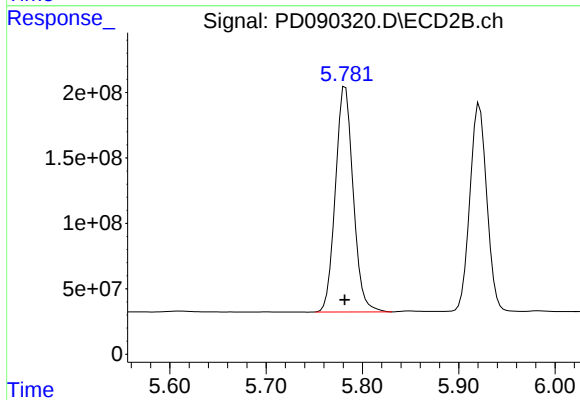


#14 Endrin

R.T.: 5.782 min
Delta R.T.: 0.000 min
Response: 2210366934
Conc: 75.16 ng/ml

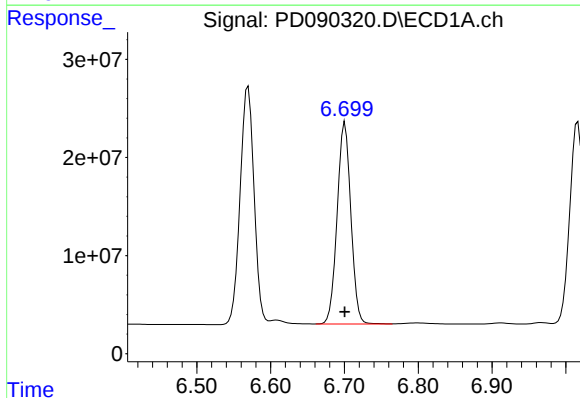


#16 4,4'-DDD

R.T.: 6.701 min
Delta R.T.: 0.000 min
Response: 264939930
Conc: 80.01 ng/ml

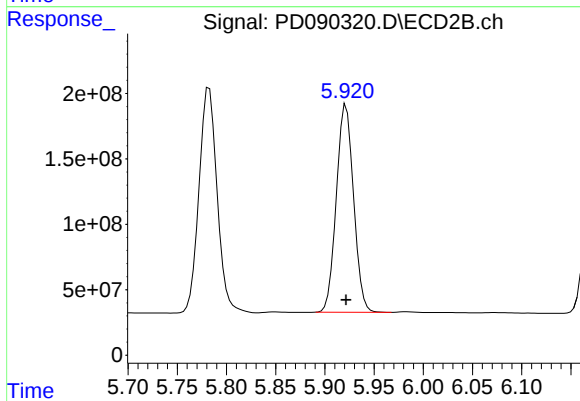

#16 4,4'-DDD


R.T.: 5.922 min
Delta R.T.: 0.000 min
Response: 1936261042
Conc: 73.48 ng/ml

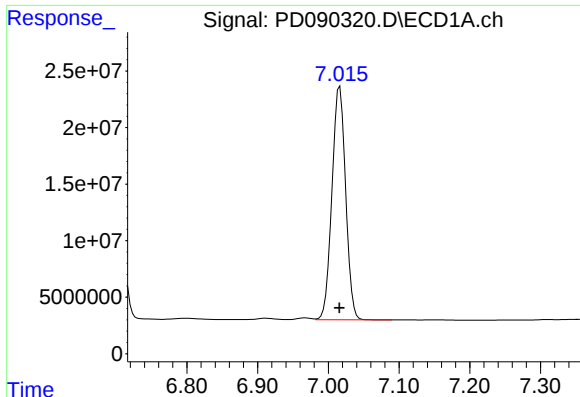

#17 4,4'-DDT


R.T.: 7.016 min
Delta R.T.: 0.000 min
Response: 277270090
Conc: 80.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4091

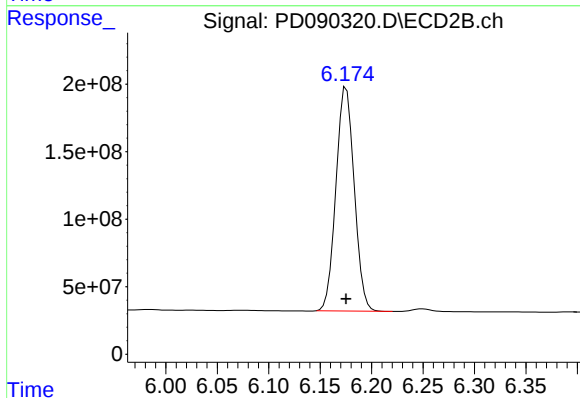


#17 4,4'-DDT

R.T.: 6.175 min
Delta R.T.: 0.000 min
Response: 2050605994
Conc: 74.94 ng/ml

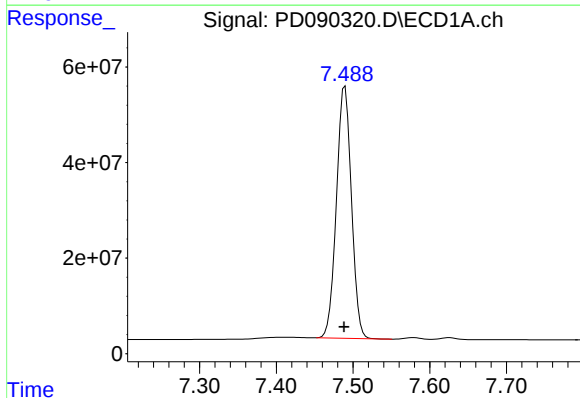


#20 Methoxychlor

R.T.: 7.489 min
Delta R.T.: 0.001 min
Response: 716344668
Conc: 389.25 ng/ml

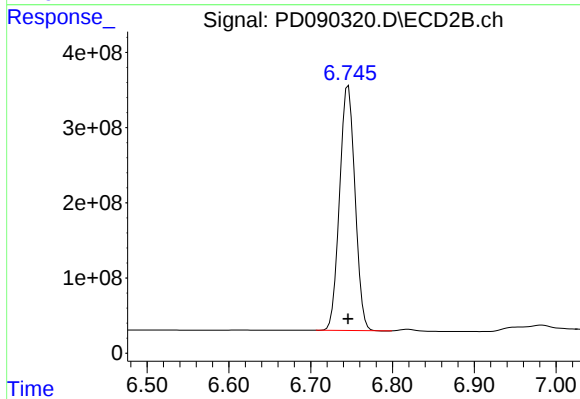

#20 Methoxychlor


R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 4250812910
Conc: 349.30 ng/ml

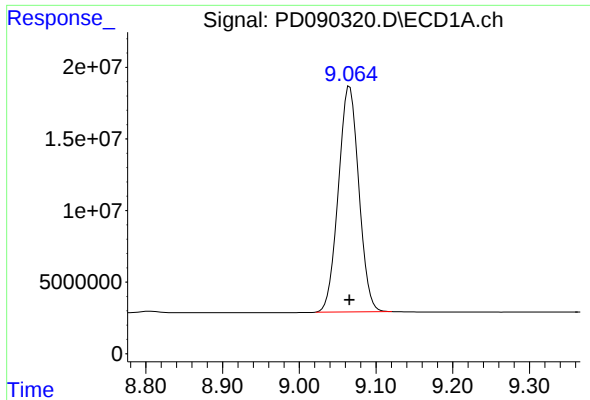

#27 Decachlorobiphenyl

R.T.: 9.066 min
Delta R.T.: 0.000 min
Response: 292658411
Conc: 74.24 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA4091

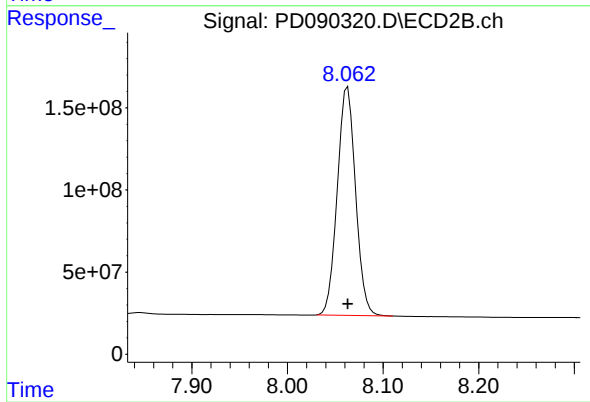

#27 Decachlorobiphenyl

R.T.: 8.063 min
Delta R.T.: 0.000 min
Response: 1849774875
Conc: 75.69 ng/ml