

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091725\
 Data File : PD090322.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2025 14:36
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA5093

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 07:34:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091725CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 18 07:32:47 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.876	194.7E6	1638.8E6	76.275	73.040
27)	SA Decachlor...	9.065	8.063	561.0E6	3725.6E6	142.306	152.440
Target Compounds							
2)	A alpha-BHC	3.995	3.388	468.9E6	2756.2E6	88.541	75.484
3)	MA gamma-BHC...	4.326	3.724	442.7E6	2517.4E6	85.305	75.331
4)	MA Heptachlor	4.924	4.076	431.8E6	2547.1E6	83.047	73.109
9)	A Endosulfan I	6.069	5.240	349.0E6	2111.5E6	78.702	71.423
13)	MA Dieldrin	6.342	5.505	795.8E6	4619.2E6	167.605	144.189
14)	MA Endrin	6.569	5.782	669.4E6	4191.4E6	167.852	142.523
16)	A 4,4'-DDD	6.701	5.921	561.0E6	3826.8E6	169.428	145.219
17)	MA 4,4'-DDT	7.016	6.175	584.6E6	4093.0E6	170.148	149.570
20)	A Methoxychlor	7.488	6.746	1435.7E6	7481.8E6	780.163	614.788


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091725\
Data File : PD090322.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2025 14:36
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 07:34:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091725CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 18 07:32:47 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

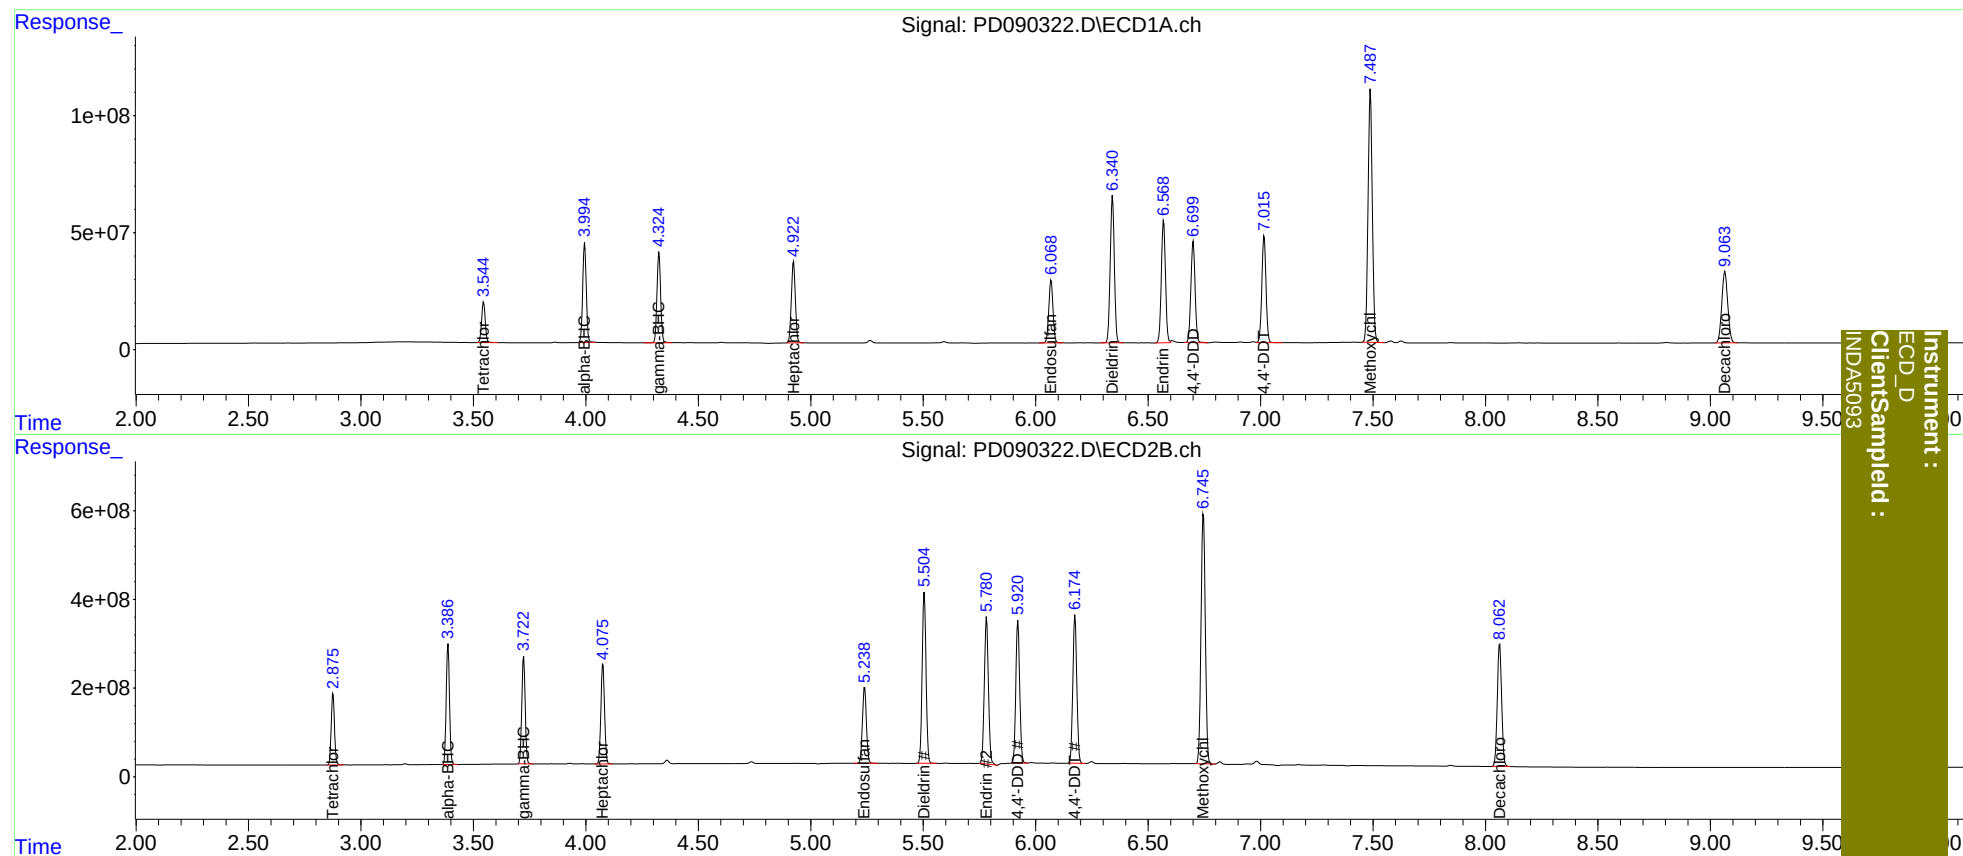


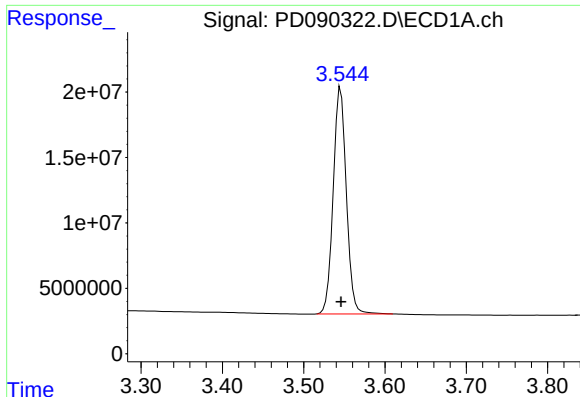

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 194689881
Conc: 76.27 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5093

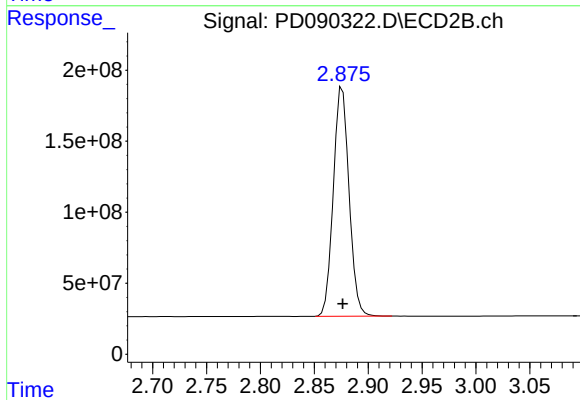


#1 Tetrachloro-m-xylene

R.T.: 2.876 min
Delta R.T.: 0.000 min
Response: 1638817617
Conc: 73.04 ng/ml

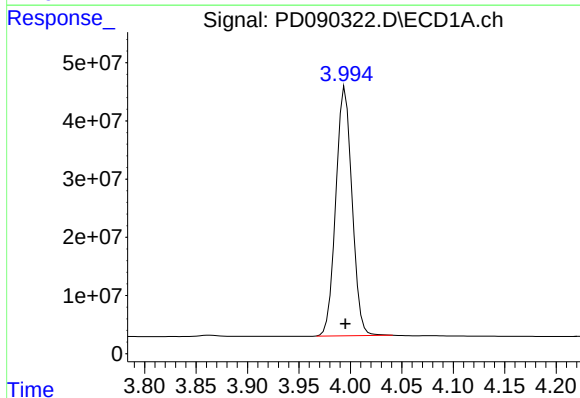


#2 alpha-BHC

R.T.: 3.995 min
Delta R.T.: 0.000 min
Response: 468898910
Conc: 88.54 ng/ml

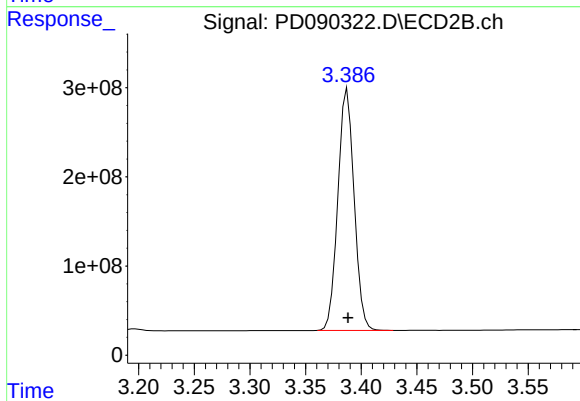

#2 alpha-BHC


R.T.: 3.388 min
Delta R.T.: 0.000 min
Response: 2756167428
Conc: 75.48 ng/ml

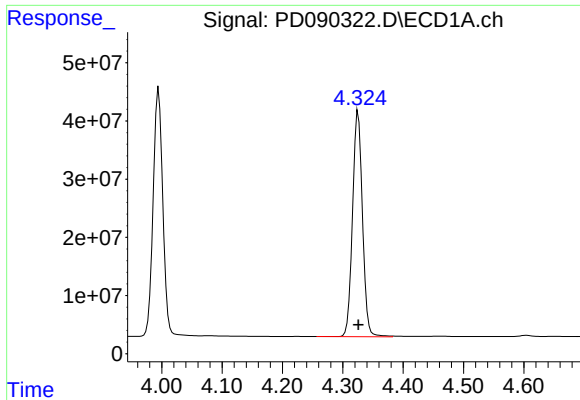

#3 gamma-BHC (Lindane)


R.T.: 4.326 min
Delta R.T.: 0.000 min
Response: 442654970
Conc: 85.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5093

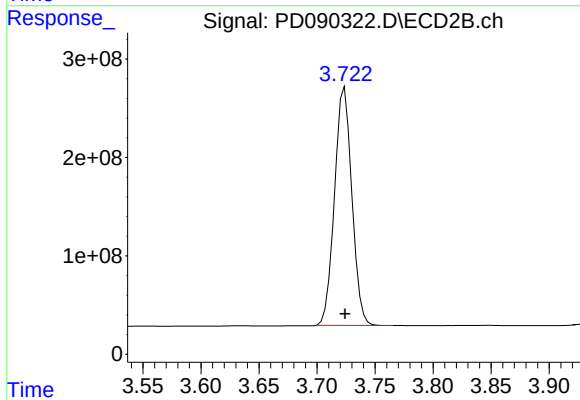


#3 gamma-BHC (Lindane)

R.T.: 3.724 min
Delta R.T.: 0.000 min
Response: 2517443703
Conc: 75.33 ng/ml

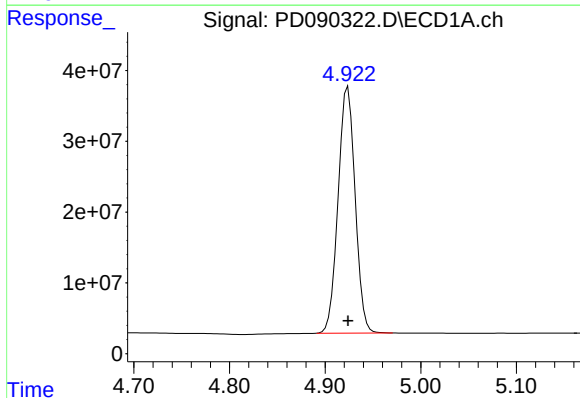


#4 Heptachlor

R.T.: 4.924 min
Delta R.T.: 0.000 min
Response: 431793663
Conc: 83.05 ng/ml

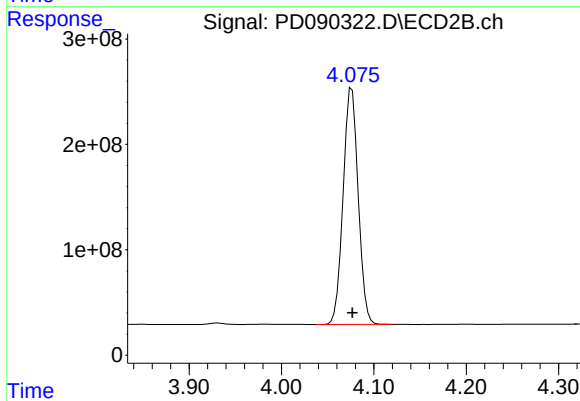

#4 Heptachlor


R.T.: 4.076 min
Delta R.T.: 0.000 min
Response: 2547086207
Conc: 73.11 ng/ml

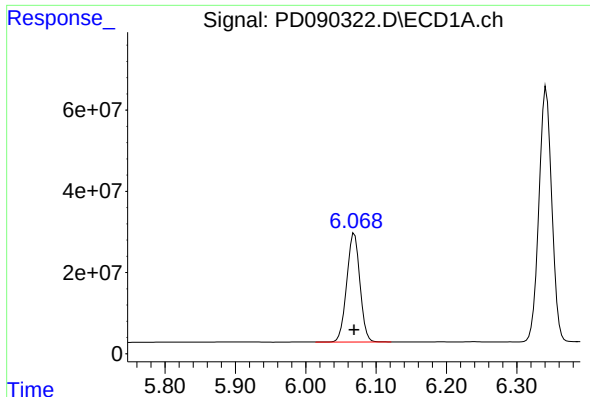

#9 Endosulfan I


R.T.: 6.069 min
Delta R.T.: 0.000 min
Response: 349023224
Conc: 78.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5093

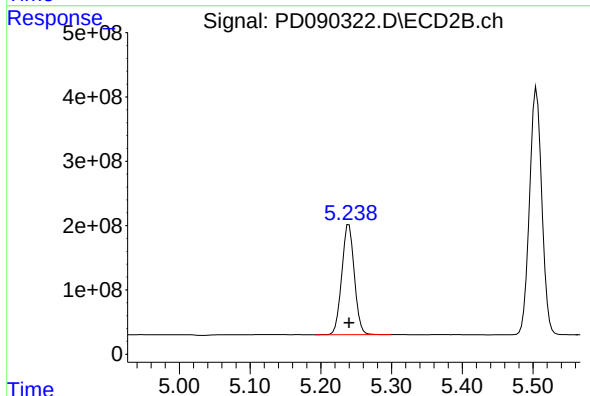


#9 Endosulfan I

R.T.: 5.240 min
Delta R.T.: 0.000 min
Response: 2111511520
Conc: 71.42 ng/ml

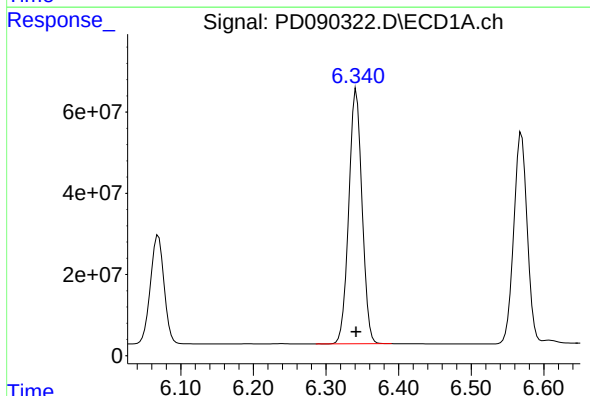


#13 Dieldrin

R.T.: 6.342 min
Delta R.T.: 0.000 min
Response: 795757137
Conc: 167.61 ng/ml

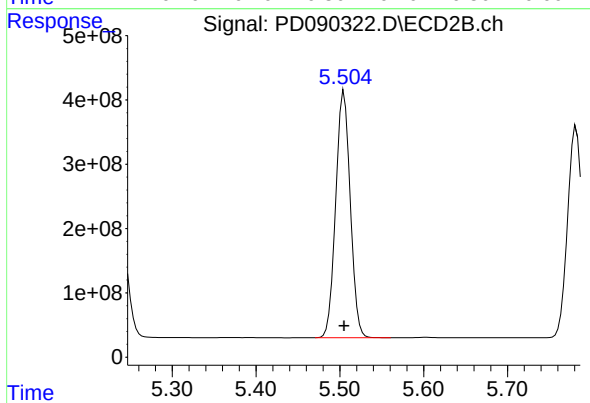

#13 Dieldrin


R.T.: 5.505 min
Delta R.T.: 0.000 min
Response: 4619219865
Conc: 144.19 ng/ml

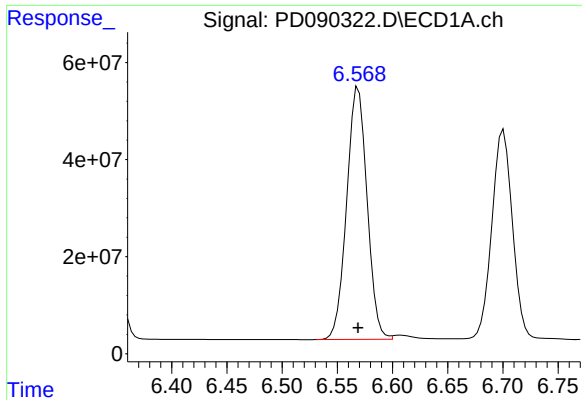

#14 Endrin


R.T.: 6.569 min
Delta R.T.: 0.000 min
Response: 669360873
Conc: 167.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5093

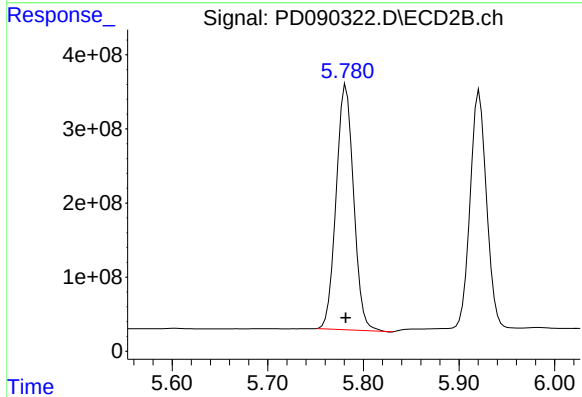


#14 Endrin

R.T.: 5.782 min
Delta R.T.: 0.000 min
Response: 4191405757
Conc: 142.52 ng/ml

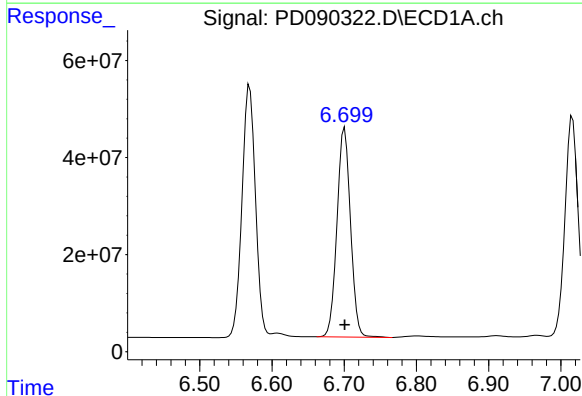


#16 4,4'-DDD

R.T.: 6.701 min
Delta R.T.: 0.000 min
Response: 561013489
Conc: 169.43 ng/ml

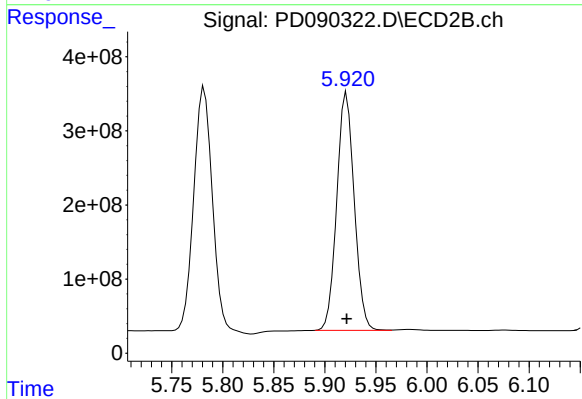

#16 4,4'-DDD


R.T.: 5.921 min
Delta R.T.: 0.000 min
Response: 3826802637
Conc: 145.22 ng/ml

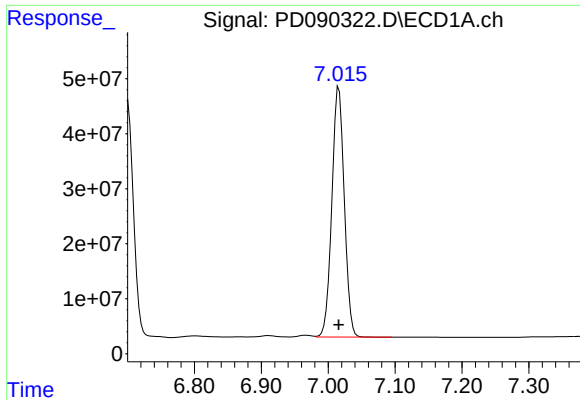

#17 4,4'-DDT


R.T.: 7.016 min
Delta R.T.: 0.000 min
Response: 584646348
Conc: 170.15 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5093

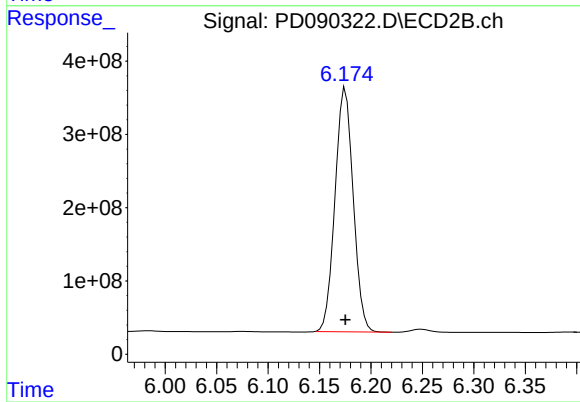


#17 4,4'-DDT

R.T.: 6.175 min
Delta R.T.: 0.000 min
Response: 4092974179
Conc: 149.57 ng/ml

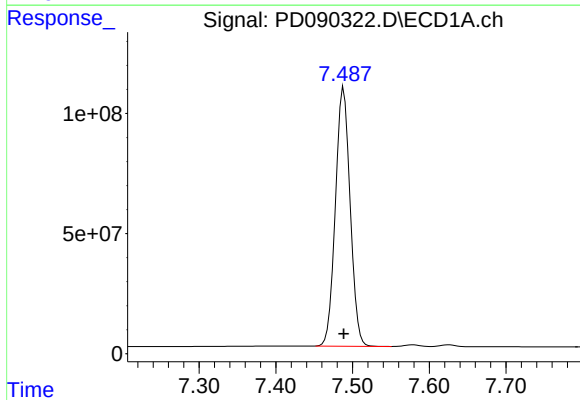


#20 Methoxychlor

R.T.: 7.488 min
Delta R.T.: 0.000 min
Response: 1435748890
Conc: 780.16 ng/ml

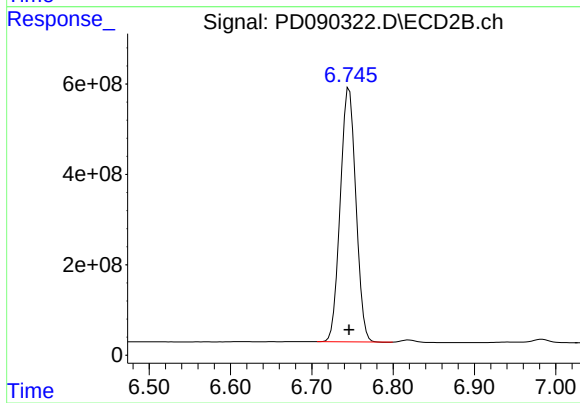

#20 Methoxychlor


R.T.: 6.746 min
Delta R.T.: 0.000 min
Response: 7481766120
Conc: 614.79 ng/ml

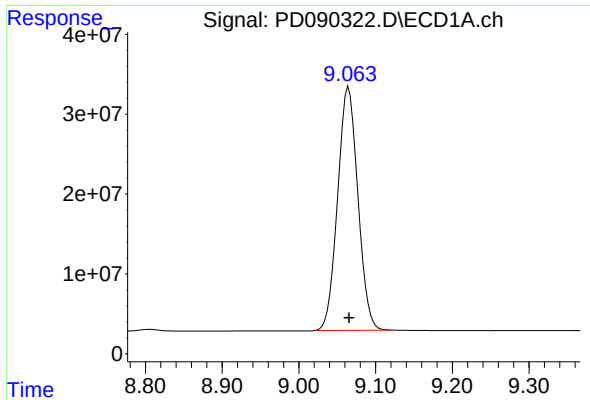

#27 Decachlorobiphenyl

R.T.: 9.065 min
Delta R.T.: 0.000 min
Response: 561005610
Conc: 142.31 ng/ml

Instrument :
ECD_D
ClientSampleId :
INDA5093

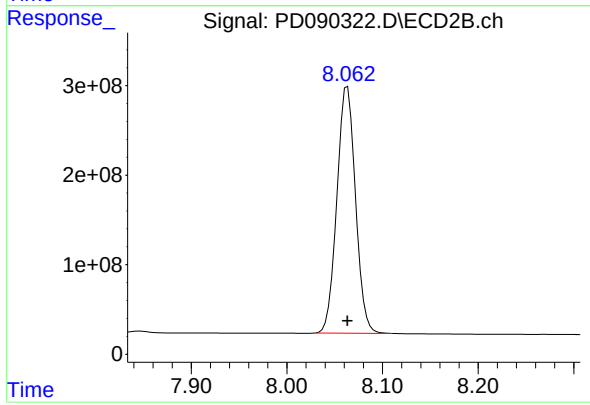

#27 Decachlorobiphenyl

R.T.: 8.063 min
Delta R.T.: 0.000 min
Response: 3725643637
Conc: 152.44 ng/ml