

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091725\
 Data File : PD090316.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2025 13:14
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 INDA2087

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 07:33:58 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091725CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 18 07:32:47 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.876	27483773	241.5E6	10.767	10.762
27)	SA Decachlor...	9.065	8.063	84790632	508.2E6	21.508	20.792
Target Compounds							
2)	A alpha-BHC	3.995	3.388	53443749	389.8E6	10.092	10.677
3)	MA gamma-BHC...	4.326	3.724	52380939	359.8E6	10.094	10.766
4)	MA Heptachlor	4.924	4.076	53762109	373.8E6	10.340	10.730
9)	A Endosulfan I	6.069	5.240	46363267	311.4E6	10.454	10.532
13)	MA Dieldrin	6.341	5.505	95772231	678.9E6	20.172	21.193
14)	MA Endrin	6.569	5.782	80607348	641.4E6	20.213	21.810
16)	A 4,4'-DDD	6.700	5.922	66757699	556.4E6	20.161	21.112
17)	MA 4,4'-DDT	7.016	6.176	68209193	565.8E6	19.851	20.675
20)	A Methoxychlor	7.488	6.746	188.6E6	1322.8E6	102.466	108.698

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091725\
Data File : PD090316.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2025 13:14
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 07:33:58 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091725CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 18 07:32:47 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

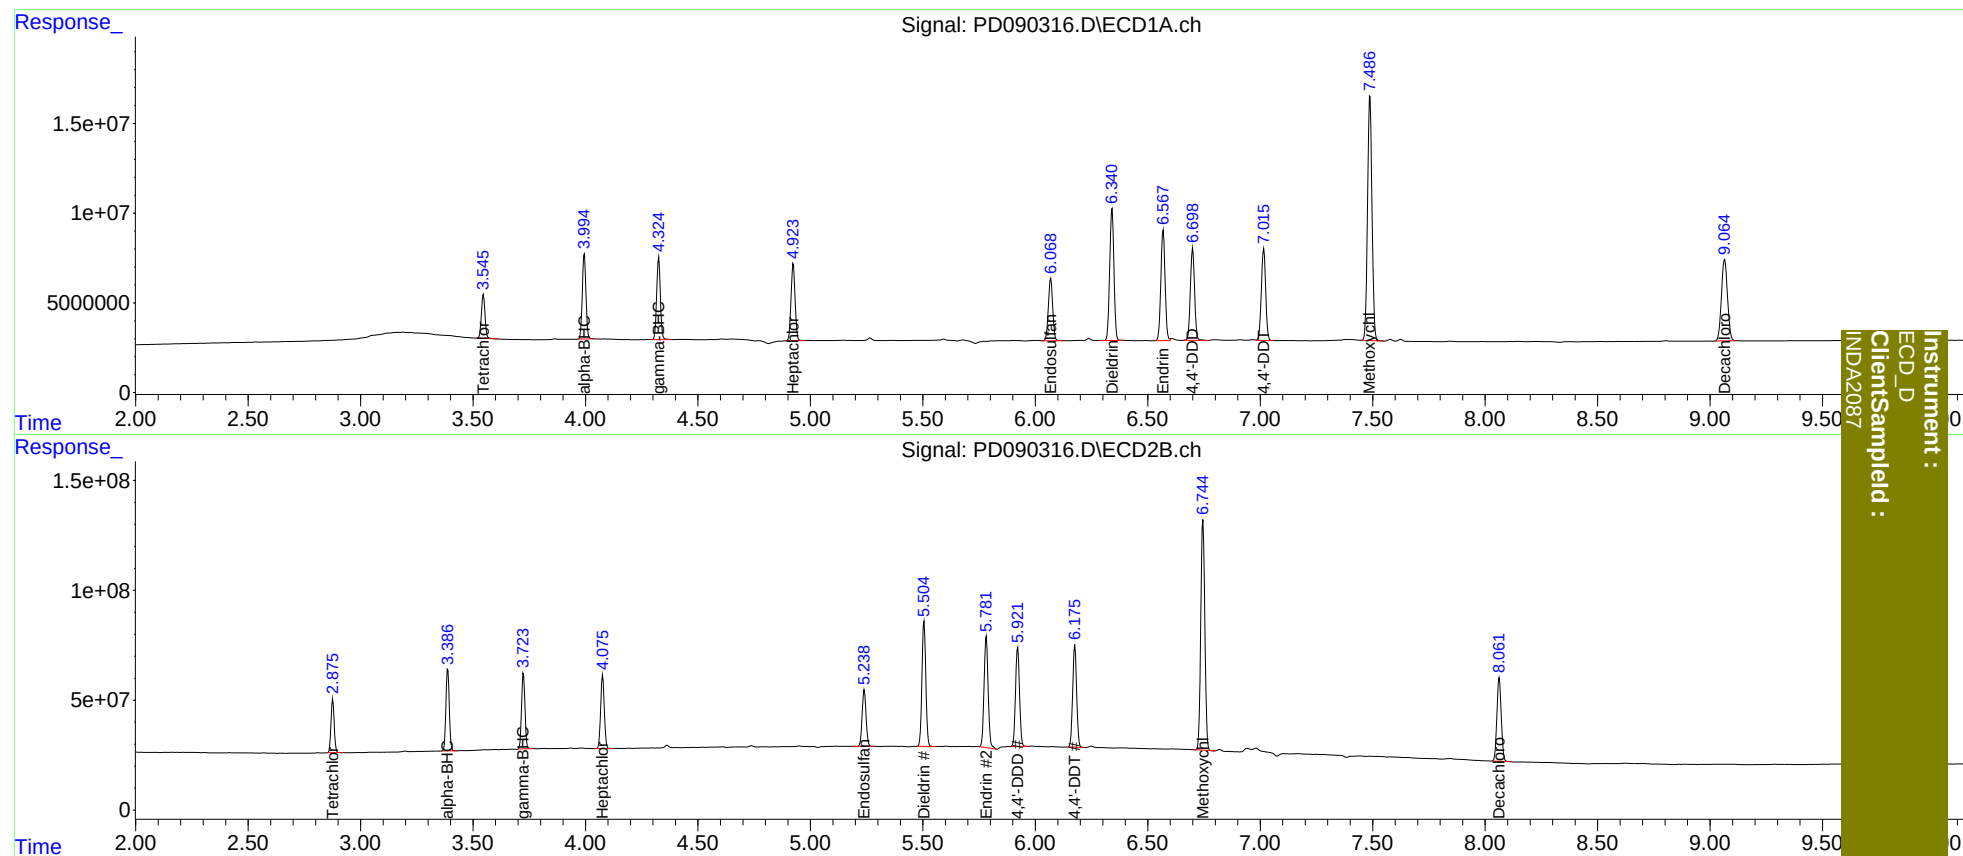

Instrument :
ECD_D
ClientSampled :
INDA2087