

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091819\
 Data File : PD054681.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Sep 2019 18:32
 Operator : SG\AJ
 Sample : PB123123BS
 Misc :
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PLCS23

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 04:22:29 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091819CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 18 17:43:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.295	3.966	13307789	17128960	19.701	20.998
27)	SA Decachlor...	7.974	9.001	33448162	40432515	37.954	39.321
Target Compounds							
3)	MA gamma-BHC...	3.998	4.635	45406932	56745835	47.534	52.200
8)	B Heptachlo...	4.961	5.829	45792268	60632794	54.691	56.984
10)	B trans-Chl...	5.183	6.062	48411650	62807366	54.919	56.783
11)	B cis-Chlor...	5.183f	0.000	48411650	0	56.597	N.D. #
12)	B 4,4'-DDE	5.409	6.291	100.7E6	129.8E6	113.882	119.928
13)	MA Dieldrin	5.532	6.439	103.8E6	132.1E6	107.082	114.933
14)	MA Endrin	5.785	6.656	93671404	107.0E6	118.013	124.027
19)	B Endosulfa...	6.438	7.209	72622281	91940755	89.099	92.014
21)	B Endrin ke...	0.000	7.678	0	3273346	N.D.	2.920
22)	Toxaphene-1	5.532	6.291	103.8E6	129.8E6	18477.578	22939.930
23)	Toxaphene-2	0.000	6.656	0	107.0E6	N.D.	14720.668


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091819\
Data File : PD054681.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Sep 2019 18:32
Operator : SG\AJ
Sample : PB123123BS
Misc :
ALS Vial : 22 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 04:22:29 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091819CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 18 17:43:20 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

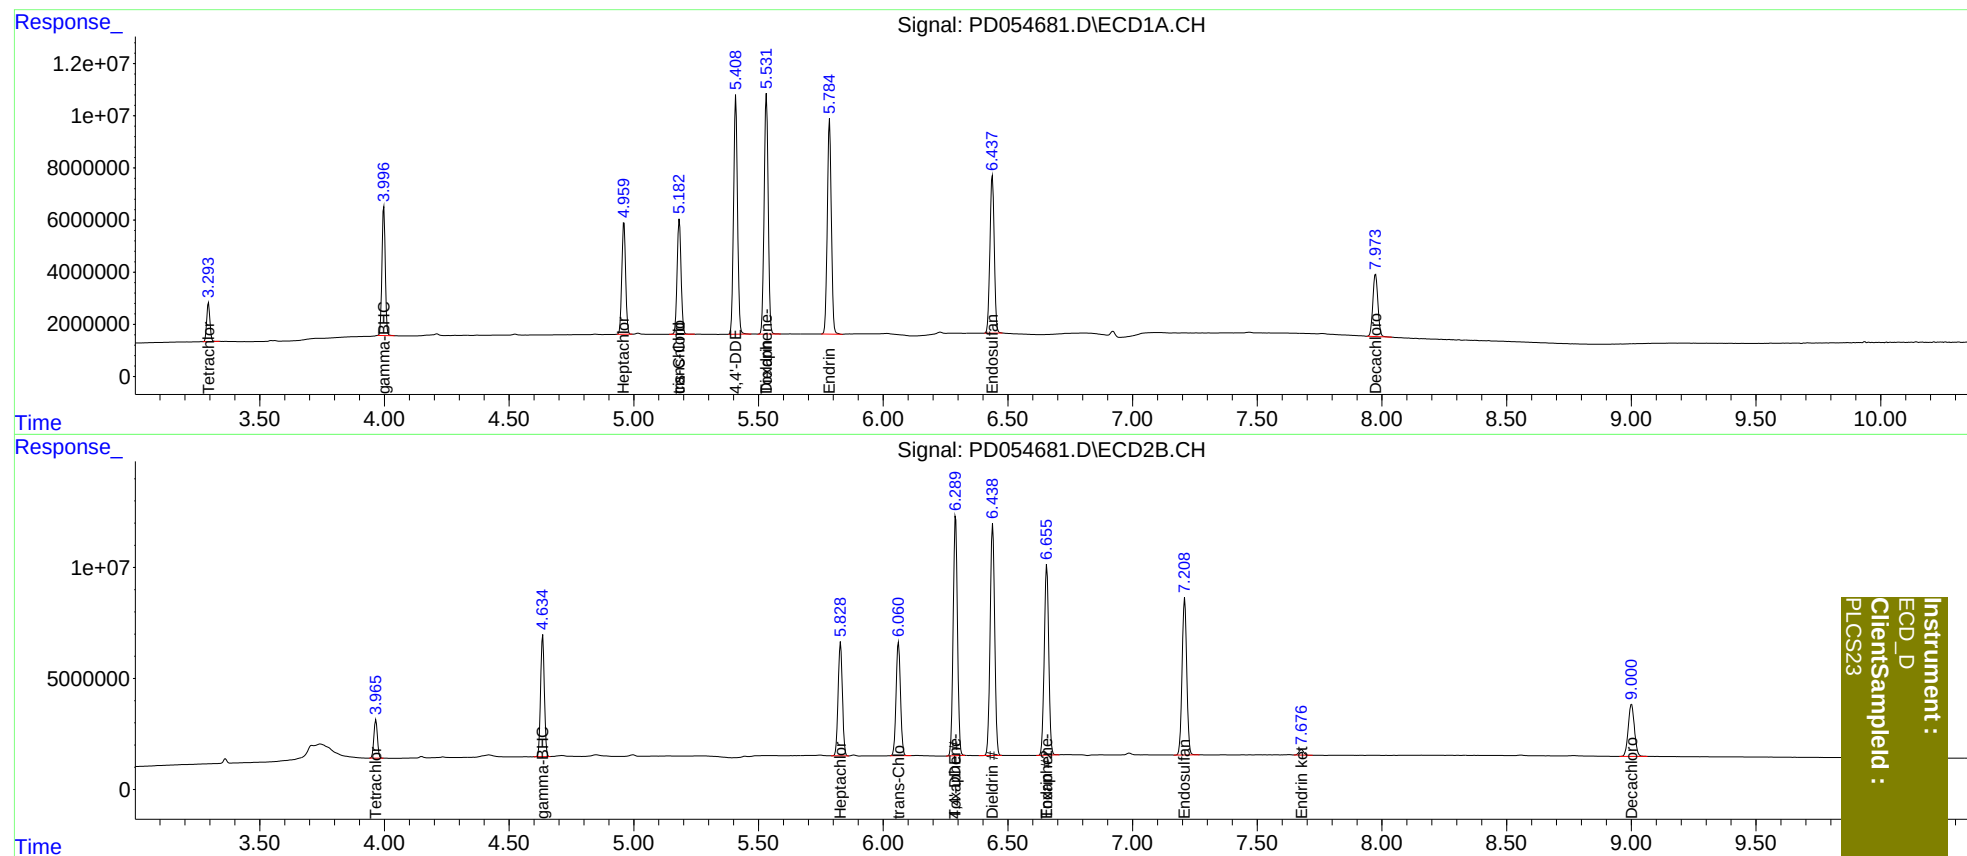


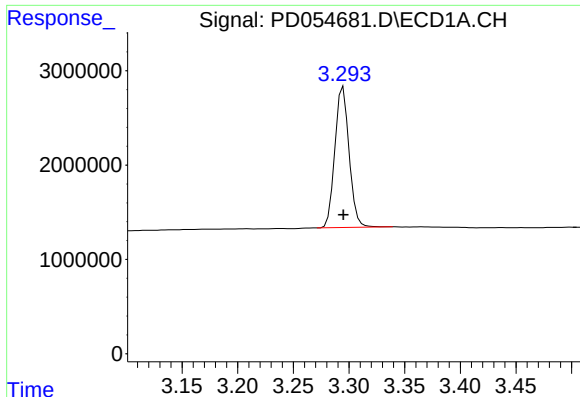

#1 Tetrachloro-m-xylene


R.T.: 3.295 min
Delta R.T.: 0.000 min
Response: 13307789
Conc: 19.70 ng/ml

Instrument :
ECD_D
ClientSampleId :
PLCS23

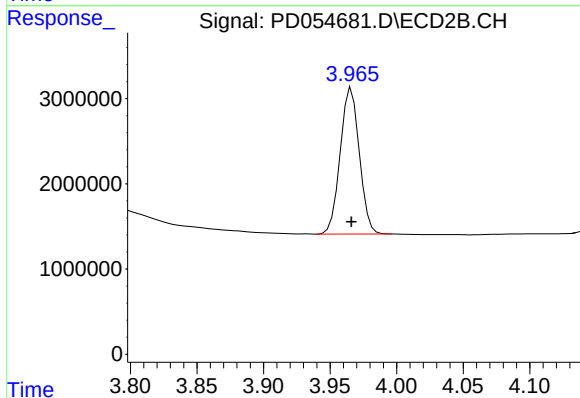


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: 0.000 min
Response: 17128960
Conc: 21.00 ng/ml

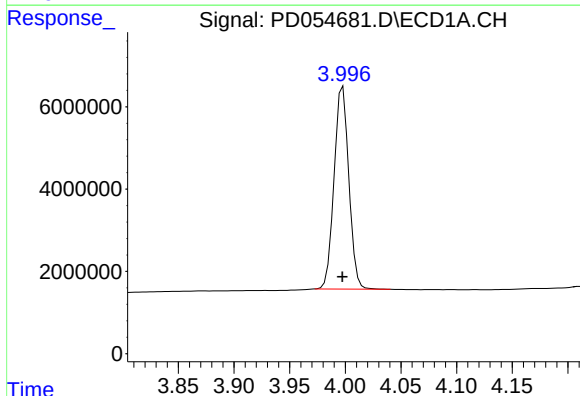


#3 gamma-BHC (Lindane)

R.T.: 3.998 min
Delta R.T.: 0.000 min
Response: 45406932
Conc: 47.53 ng/ml

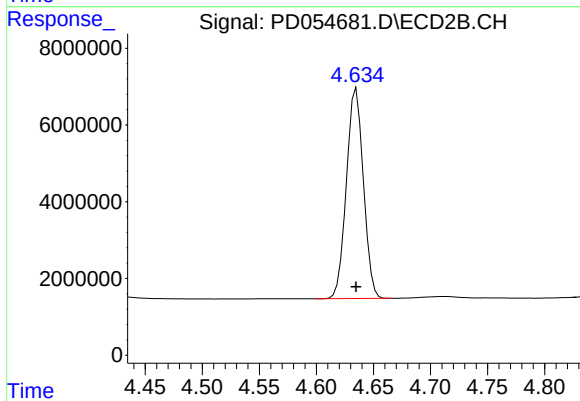

#3 gamma-BHC (Lindane)


R.T.: 4.635 min
Delta R.T.: 0.000 min
Response: 56745835
Conc: 52.20 ng/ml

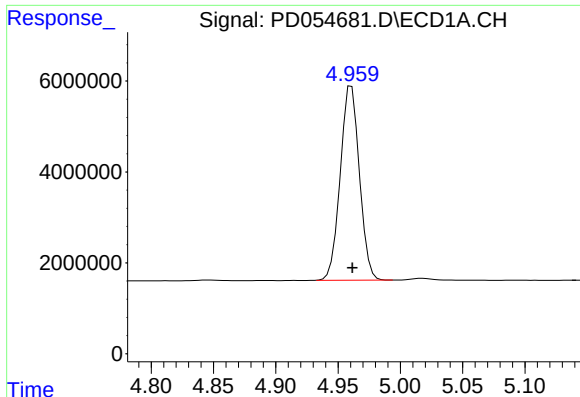

#8 Heptachlor epoxide


R.T.: 4.961 min
Delta R.T.: 0.000 min
Response: 45792268
Conc: 54.69 ng/ml

Instrument :
ECD_D
ClientSampleId :
PLCS23

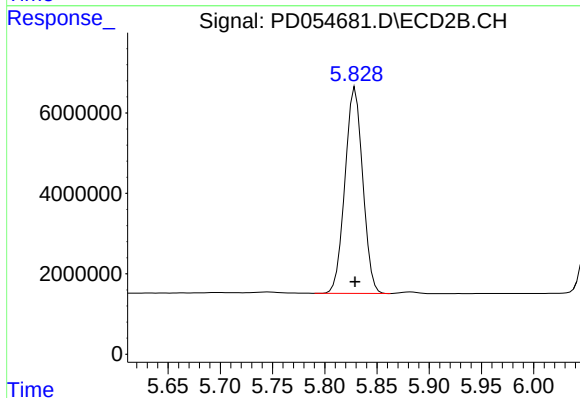


#8 Heptachlor epoxide

R.T.: 5.829 min
Delta R.T.: 0.000 min
Response: 60632794
Conc: 56.98 ng/ml

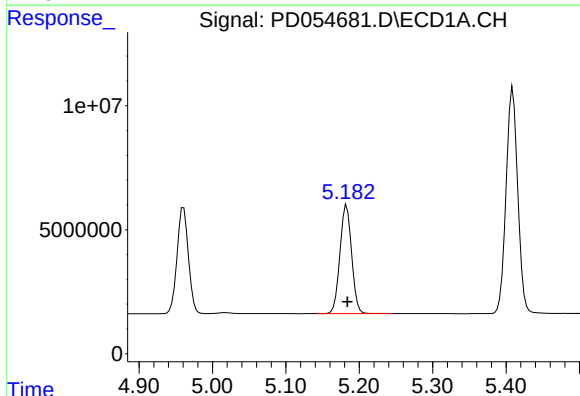


#10 trans-Chlordane

R.T.: 5.183 min
Delta R.T.: 0.000 min
Response: 48411650
Conc: 54.92 ng/ml

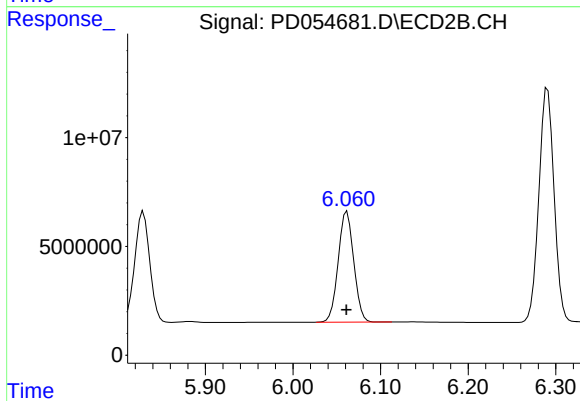

#10 trans-Chlordane


R.T.: 6.062 min
Delta R.T.: 0.000 min
Response: 62807366
Conc: 56.78 ng/ml

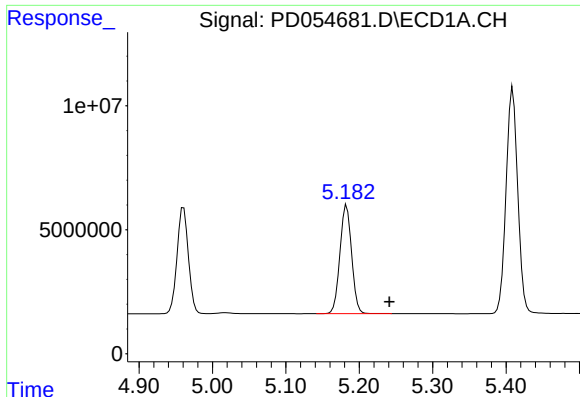

#11 cis-Chlordane


R.T.: 5.183 min
Delta R.T.: -0.058 min
Response: 48411650
Conc: 56.60 ng/ml

Instrument :
ECD_D
ClientSampleId :
PLCS23

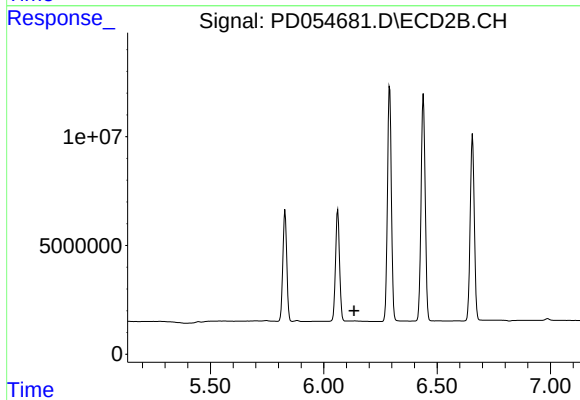


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T.: 6.134 min
Response: 0
Conc: N.D.

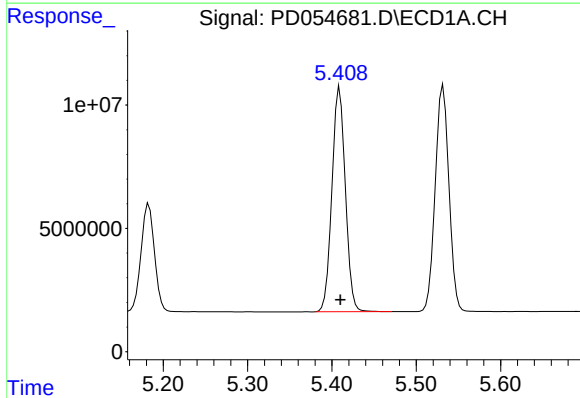


#12 4,4'-DDE

R.T.: 5.409 min
Delta R.T.: 0.000 min
Response: 100680813
Conc: 113.88 ng/ml

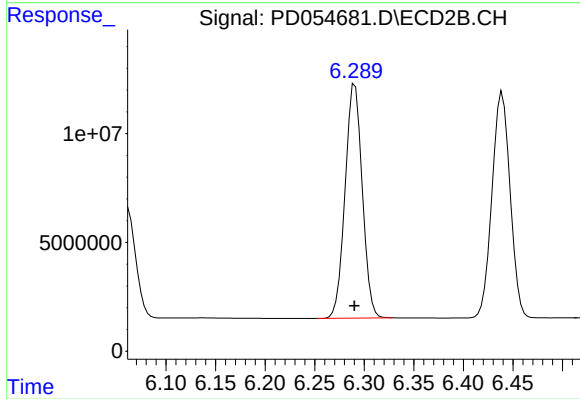

#12 4,4'-DDE


R.T.: 6.291 min
Delta R.T.: 0.000 min
Response: 129761908
Conc: 119.93 ng/ml

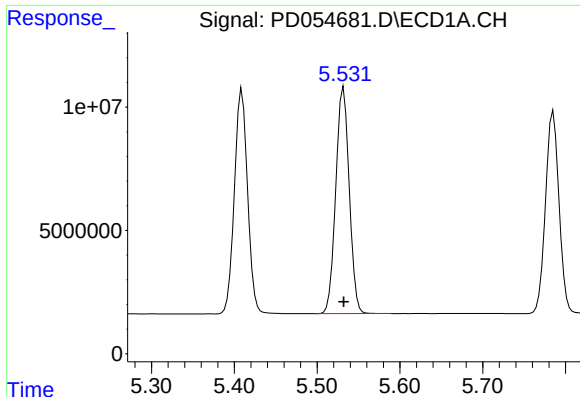

#13 Dieldrin


R.T.: 5.532 min
Delta R.T.: 0.000 min
Response: 103803631
Conc: 107.08 ng/ml

Instrument :
ECD_D
ClientSampleId :
PLCS23

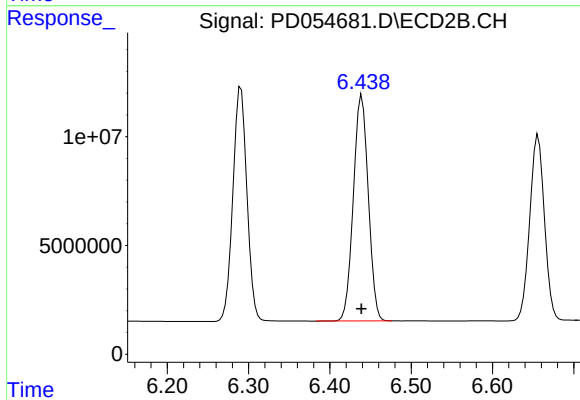


#13 Dieldrin

R.T.: 6.439 min
Delta R.T.: 0.000 min
Response: 132095743
Conc: 114.93 ng/ml

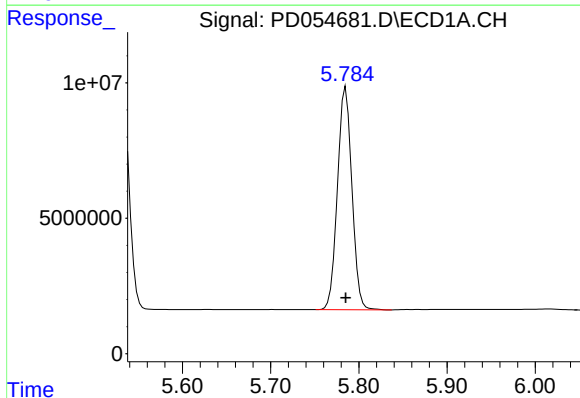


#14 Endrin

R.T.: 5.785 min
Delta R.T.: 0.000 min
Response: 93671404
Conc: 118.01 ng/ml

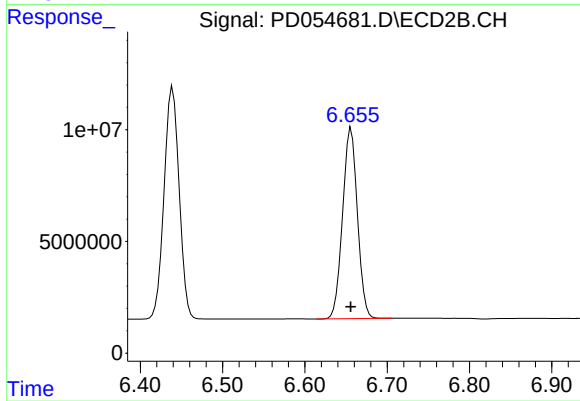

#14 Endrin


R.T.: 6.656 min
Delta R.T.: 0.000 min
Response: 106951916
Conc: 124.03 ng/ml

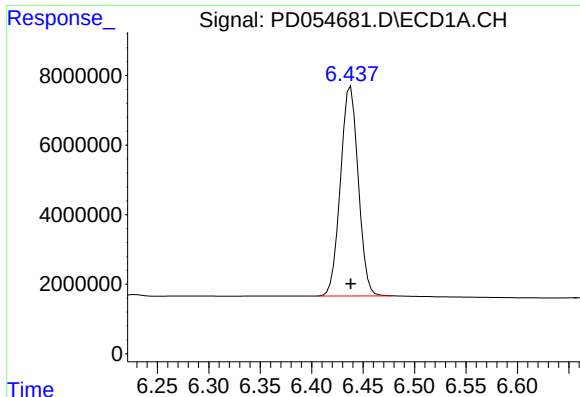

#19 Endosulfan Sulfate


R.T.: 6.438 min
Delta R.T.: 0.000 min
Response: 72622281
Conc: 89.10 ng/ml

Instrument :
ECD_D
ClientSampleId :
PLCS23

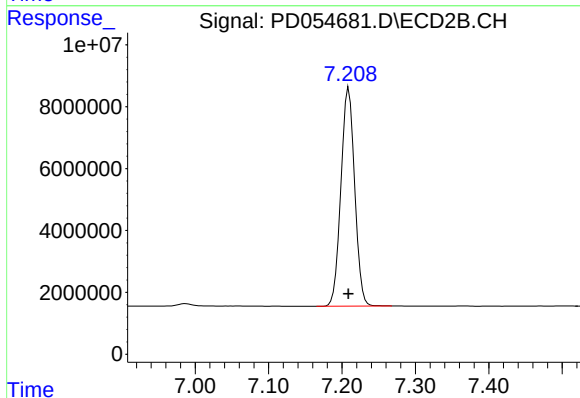


#19 Endosulfan Sulfate

R.T.: 7.209 min
Delta R.T.: 0.000 min
Response: 91940755
Conc: 92.01 ng/ml

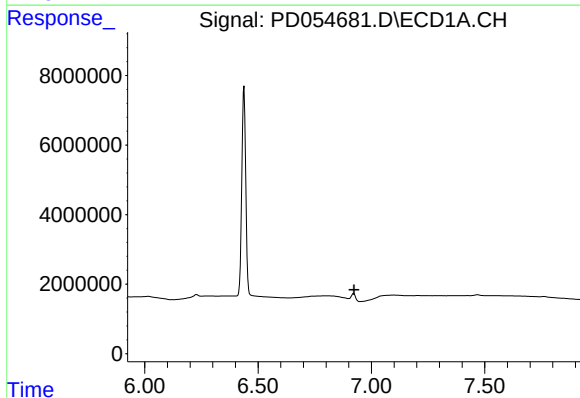


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.924 min
Response: 0
Conc: N.D.

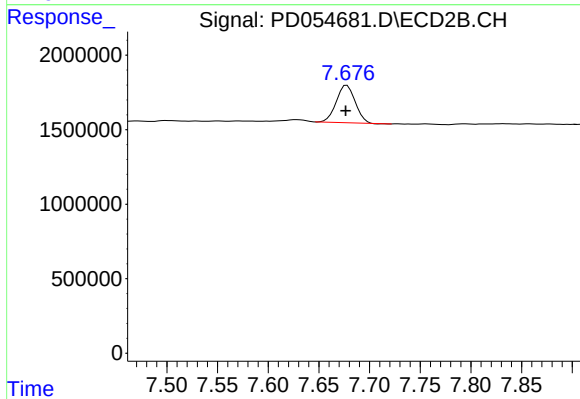

#21 Endrin ketone


R.T.: 7.678 min
Delta R.T.: 0.001 min
Response: 3273346
Conc: 2.92 ng/ml

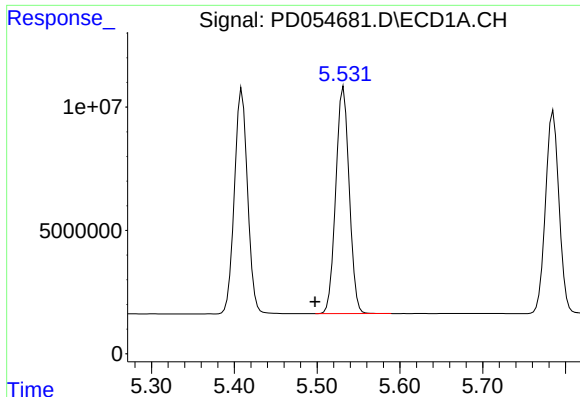

#22 Toxaphene-1


R.T.: 5.532 min
Delta R.T.: 0.034 min
Response: 103803631
Conc: 18477.58 ng/ml

Instrument :
ECD_D
ClientSampleId :
PLCS23

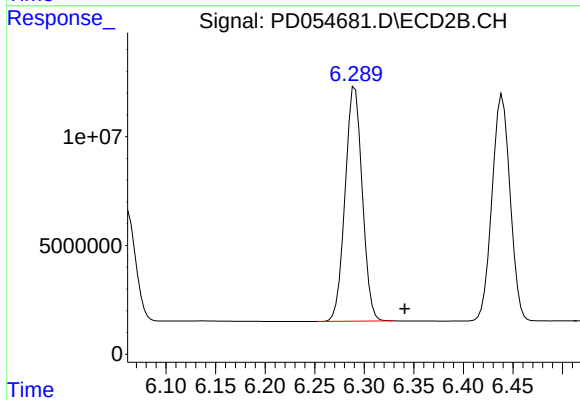


#22 Toxaphene-1

R.T.: 6.291 min
Delta R.T.: -0.050 min
Response: 129761908
Conc: 22939.93 ng/ml

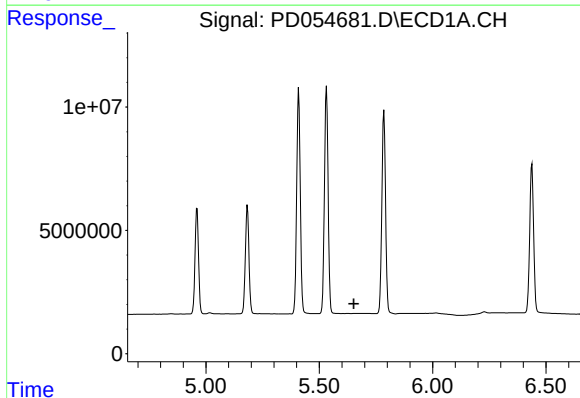


#23 Toxaphene-2

R.T.: 0.000 min
Exp R.T. : 5.653 min
Response: 0
Conc: N.D.

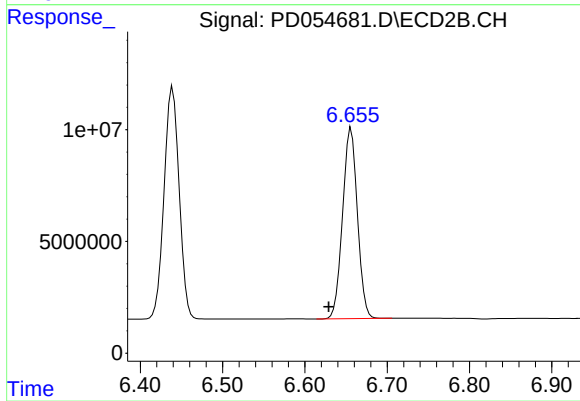

#23 Toxaphene-2


R.T.: 6.656 min
Delta R.T.: 0.027 min
Response: 106951916
Conc: 14720.67 ng/ml

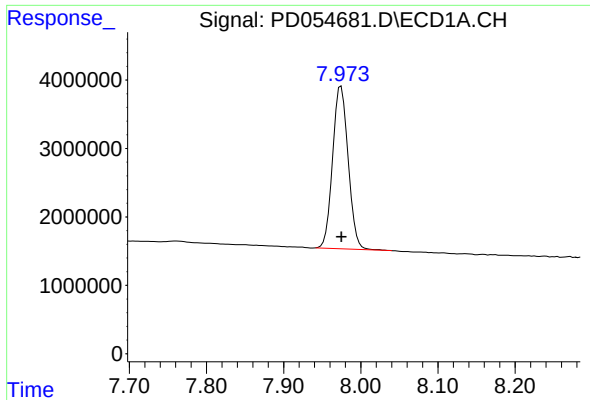

#27 Decachlorobiphenyl

R.T.: 7.974 min
Delta R.T.: 0.000 min
Response: 33448162
Conc: 37.95 ng/ml

Instrument :
ECD_D
ClientSampleId :
PLCS23

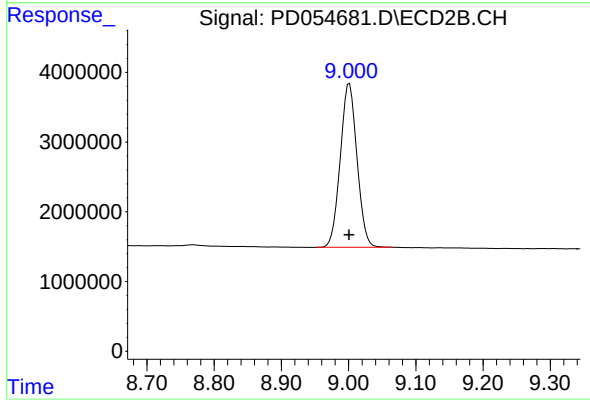

#27 Decachlorobiphenyl

R.T.: 9.001 min
Delta R.T.: 0.000 min
Response: 40432515
Conc: 39.32 ng/ml