

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091819\
 Data File : PD054683.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 18 Sep 2019 19:00
 Operator : SG\AJ
 Sample : K4845-02
 Misc :
 ALS Vial : 24 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AA1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 04:22:51 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091819CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 18 17:43:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.295	3.966	8013997	9938412	11.864	12.183
2)	SA Decachlor...	7.975	9.001	18825320	21871309	21.361	21.270
Target Compounds							
10)	B trans-Chl...	0.000	6.046	0	2534997	N.D.	2.292

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091819\
Data File : PD054683.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Sep 2019 19:00
Operator : SG\AJ
Sample : K4845-02
Misc :
ALS Vial : 24 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 04:22:51 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091819CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 18 17:43:20 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

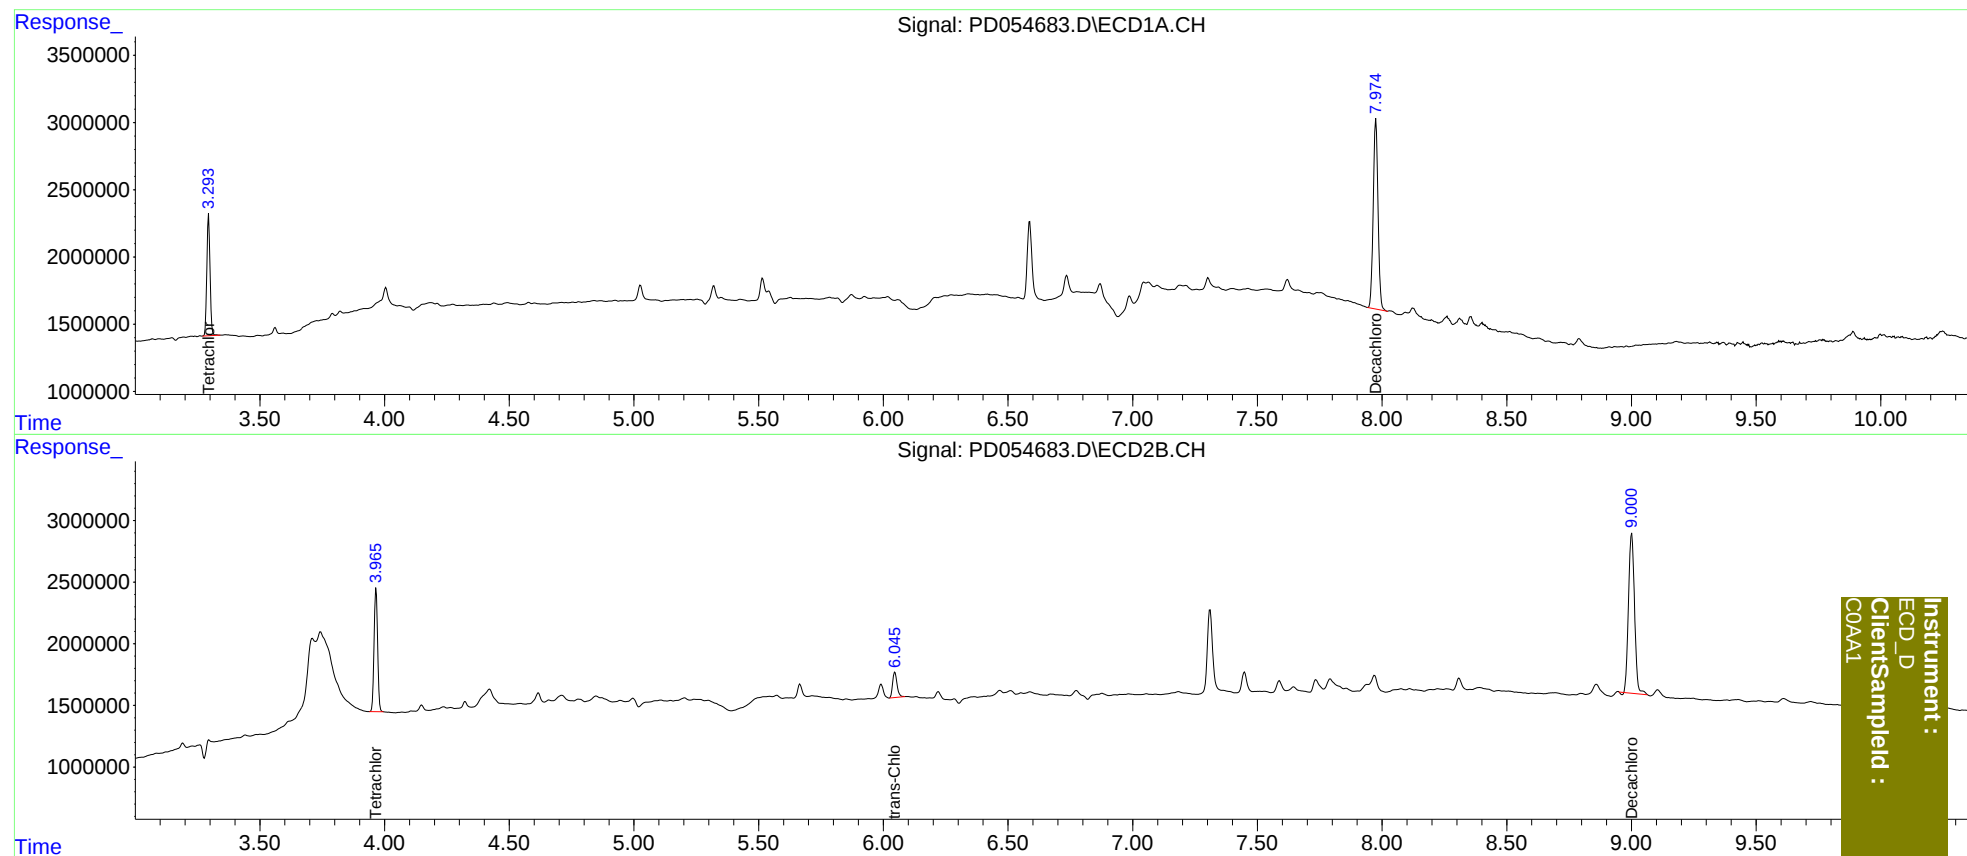


Instrument :
ECD_D
ClientSampleId :
C00A1

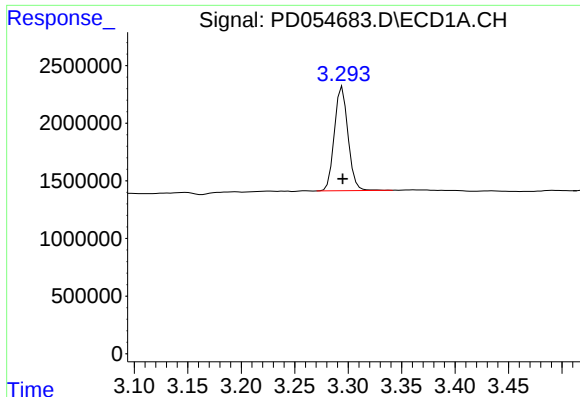

#1 Tetrachloro-m-xylene


R.T.: 3.295 min
Delta R.T.: 0.000 min
Response: 8013997
Conc: 11.86 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AA1

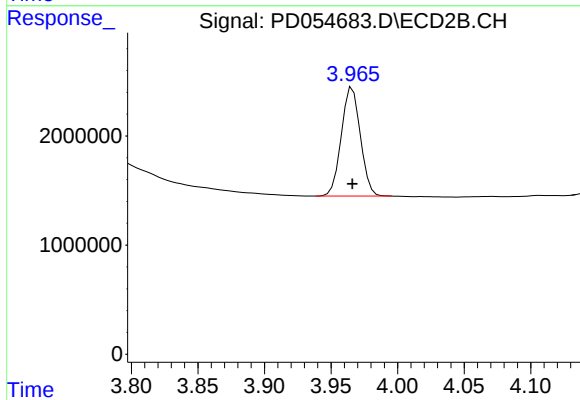


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: 0.000 min
Response: 9938412
Conc: 12.18 ng/ml

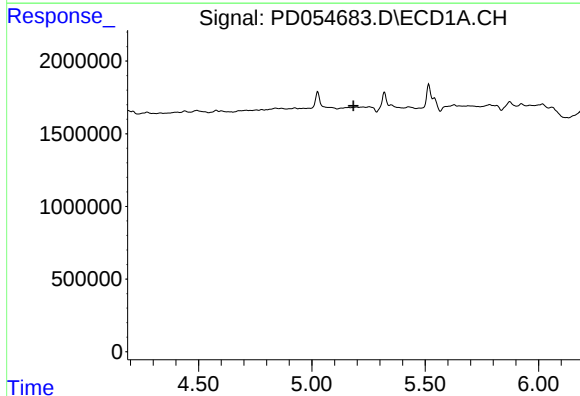


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.184 min
Response: 0
Conc: N.D.

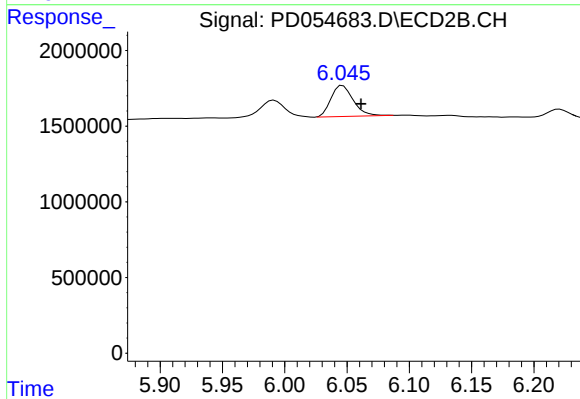

#10 trans-Chlordane


R.T.: 6.046 min
Delta R.T.: -0.015 min
Response: 2534997
Conc: 2.29 ng/ml

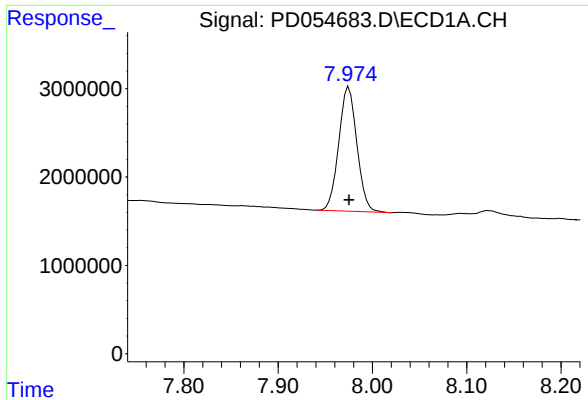

#27 Decachlorobiphenyl

R.T.: 7.975 min
Delta R.T.: 0.000 min
Response: 18825320
Conc: 21.36 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AA1

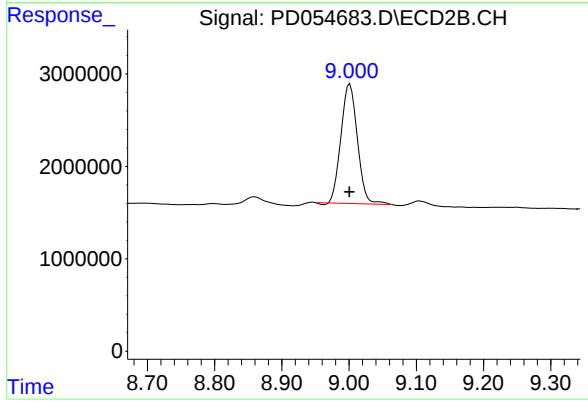

#27 Decachlorobiphenyl

R.T.: 9.001 min
Delta R.T.: 0.000 min
Response: 21871309
Conc: 21.27 ng/ml