

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091819\
Data File : PD054684.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Sep 2019 19:14
Operator : SG\AJ
Sample : K4845-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0AM5

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 04:22:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091819CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 18 17:43:20 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.295	3.966	12198855	15061013	18.059	18.463
27)	SA Decachlor...	7.974	9.002	28290983	33595292	32.102	32.671


Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091819\
Data File : PD054684.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 18 Sep 2019 19:14
Operator : SG\AJ
Sample : K4845-03
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 04:22:59 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091819CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 18 17:43:20 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

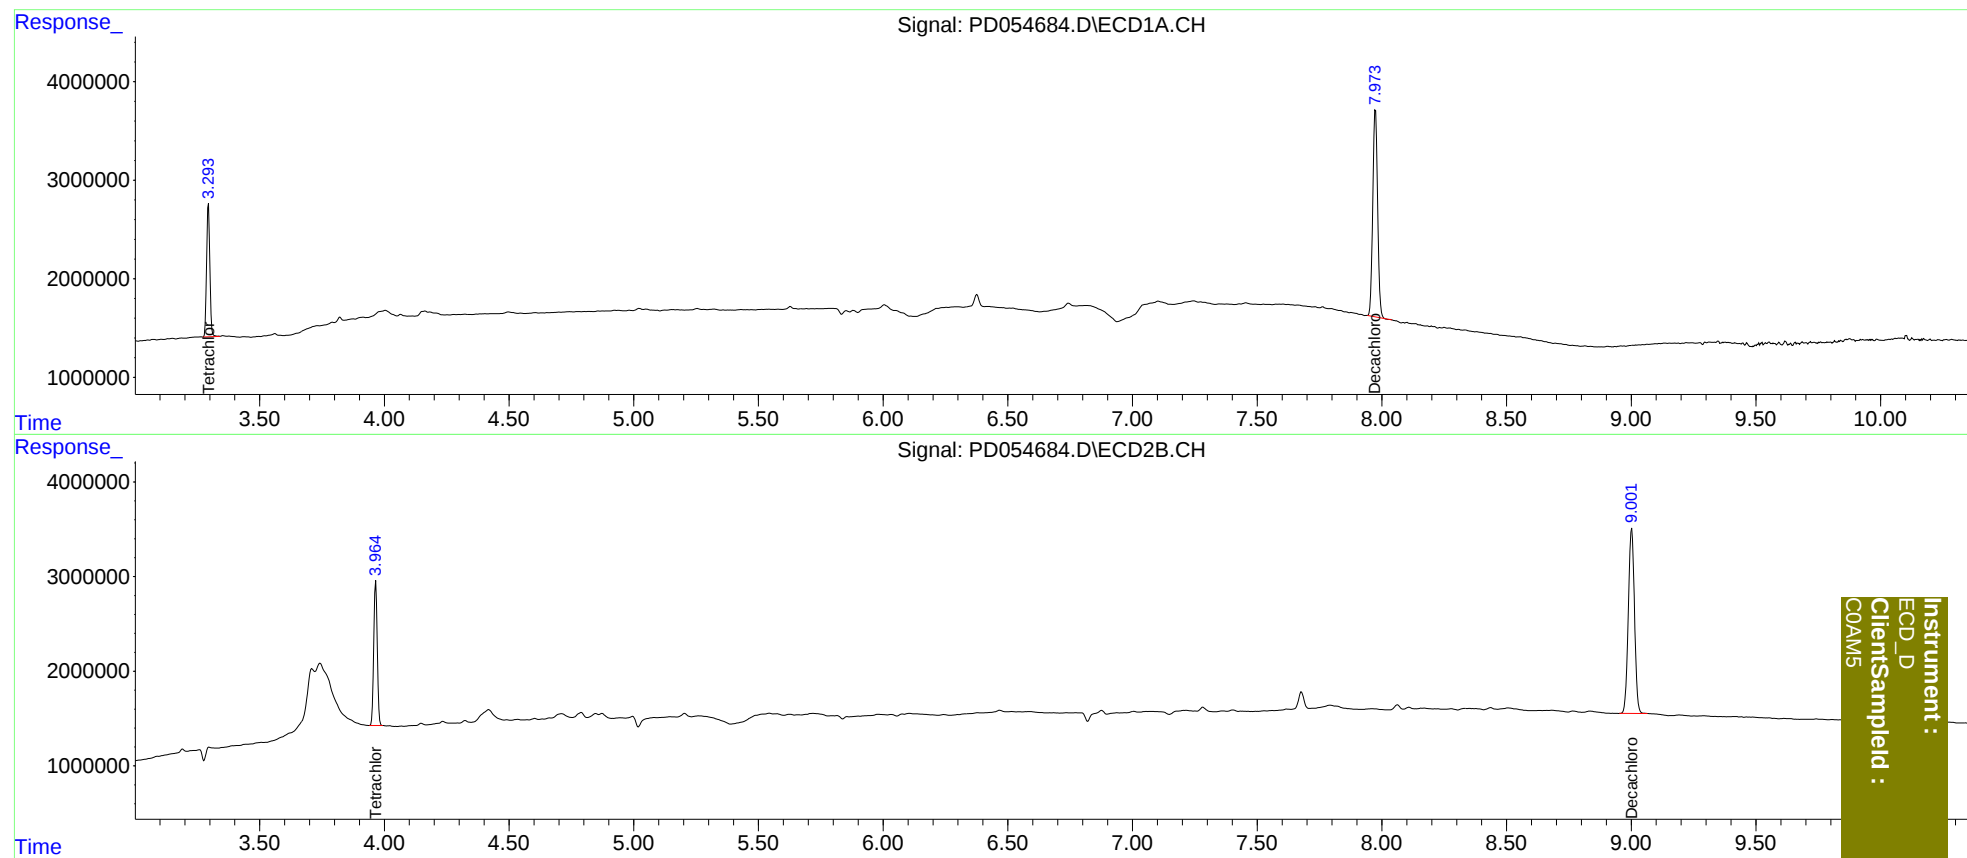


Instrument :
ECD_D
ClientSampled :
COAM5

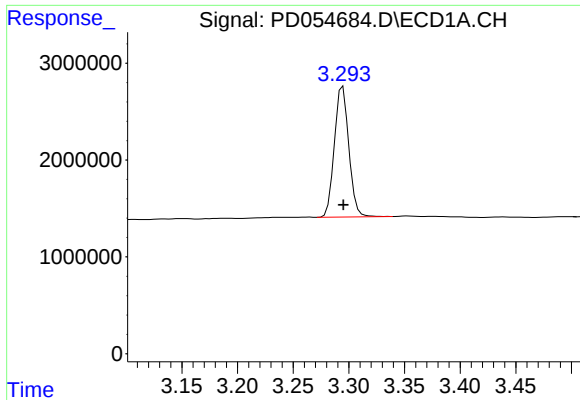

#1 Tetrachloro-m-xylene


R.T.: 3.295 min
Delta R.T.: 0.000 min
Response: 12198855
Conc: 18.06 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AM5

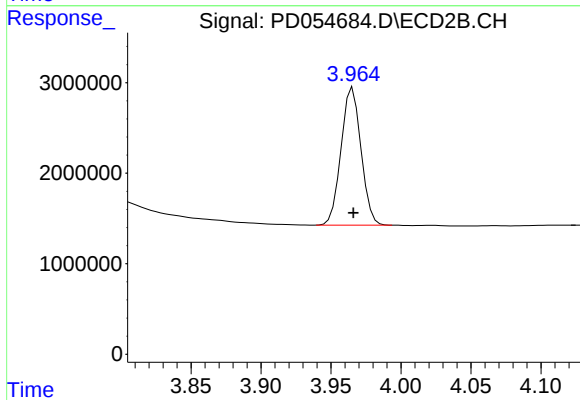


#1 Tetrachloro-m-xylene

R.T.: 3.966 min
Delta R.T.: 0.000 min
Response: 15061013
Conc: 18.46 ng/ml

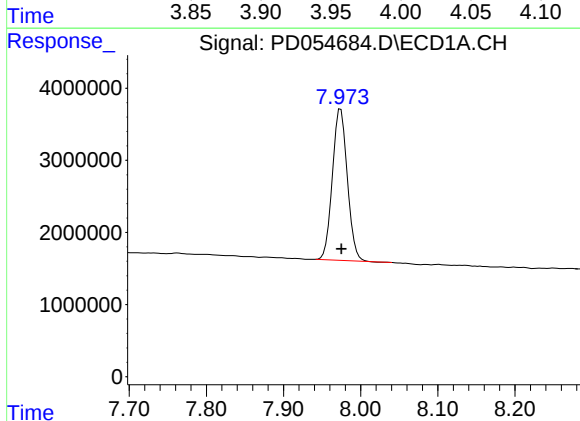

#27 Decachlorobiphenyl

R.T.: 7.974 min
Delta R.T.: -0.001 min
Response: 28290983
Conc: 32.10 ng/ml

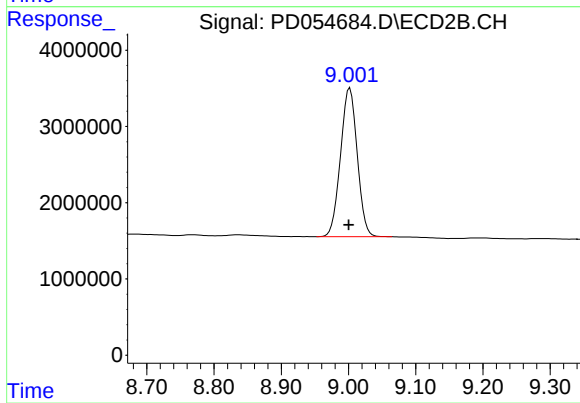

#27 Decachlorobiphenyl

R.T.: 9.002 min
Delta R.T.: 0.002 min
Response: 33595292
Conc: 32.67 ng/ml