

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091820\
 Data File : PD059262.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2020 09:33
 Operator : DD\AJ
 Sample : PB131672BL
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK72

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 06:53:37 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090420CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 05 02:06:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.208	3.865	20824230	40813973	20.659	24.905
27) SA Decachlor...	7.841	8.860	41074244	64376548	41.911	47.866
Target Compounds						
8) B Heptachlo...	0.000	5.762f	0	1314101	N.D.	0.655


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091820\
Data File : PD059262.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2020 09:33
Operator : DD\AJ
Sample : PB131672BL
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PBLK72

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 06:53:37 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090420CLP.M
Quant Title : GC Extractables
QLast Update : Sat Sep 05 02:06:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

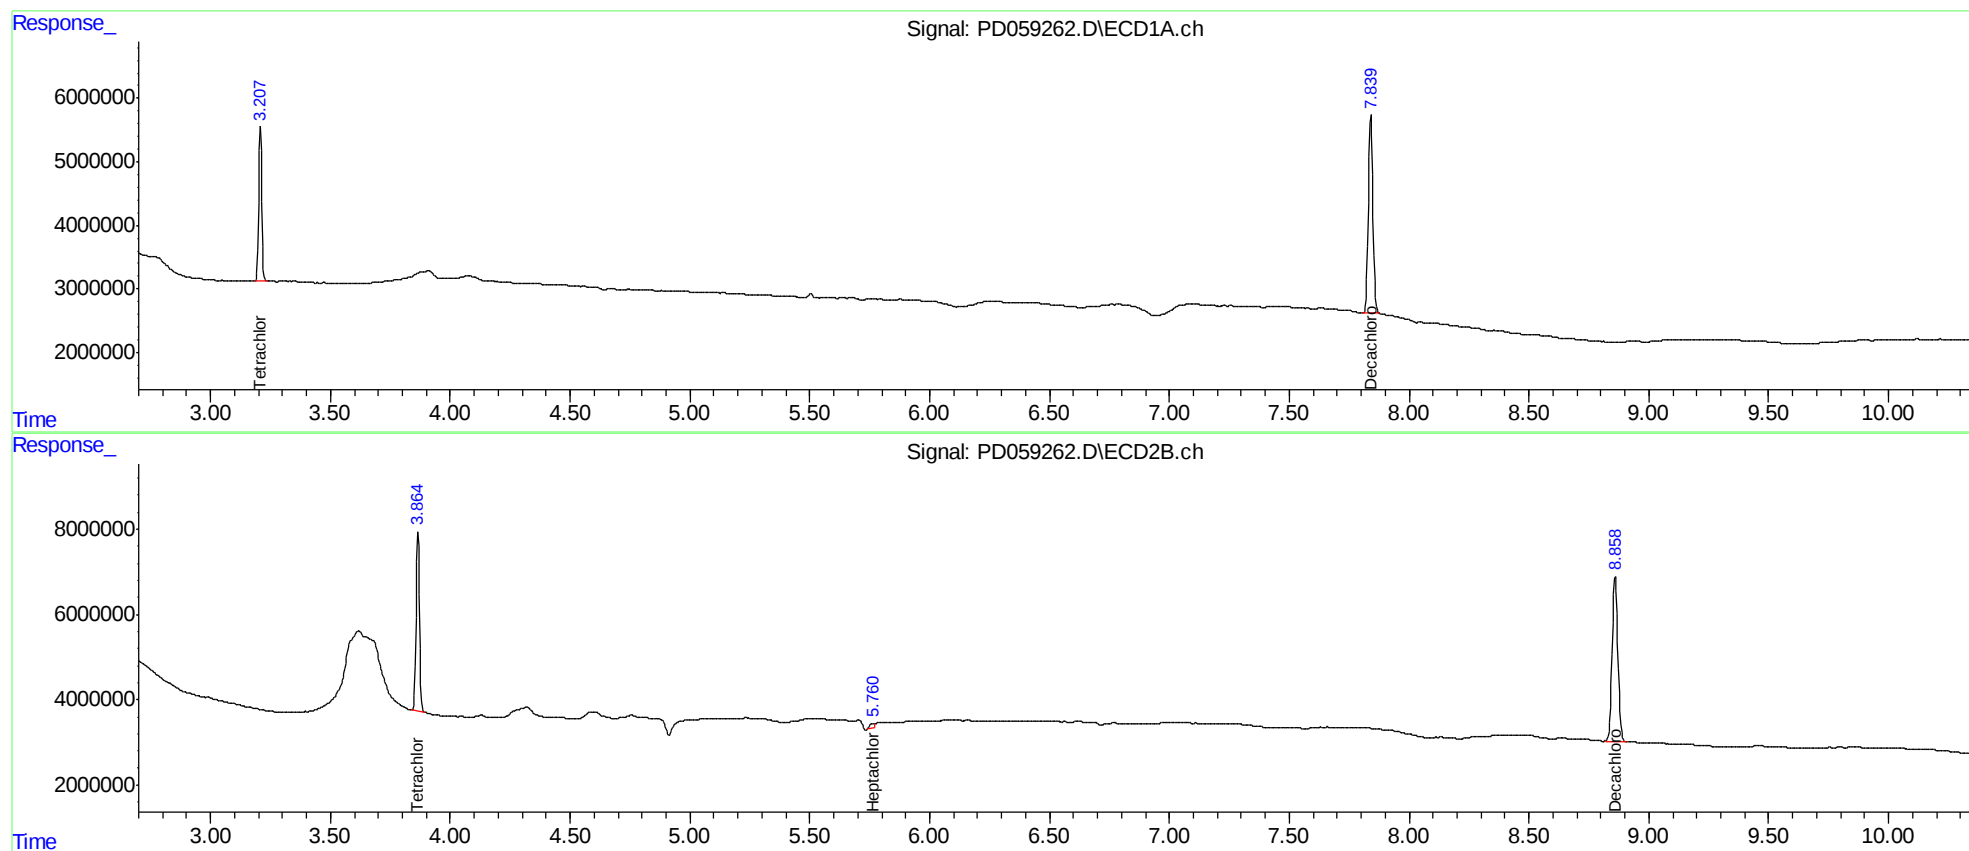


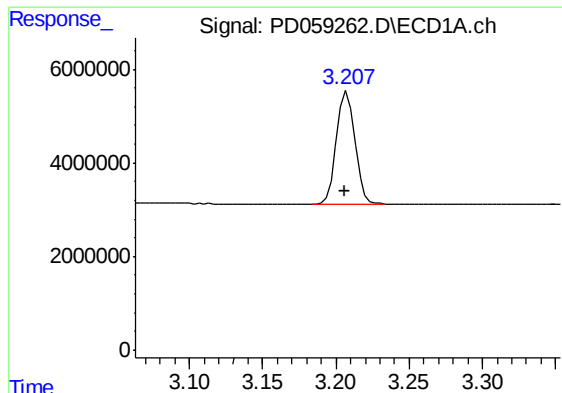

#1 Tetrachloro-m-xylene


R.T.: 3.208 min
Delta R.T.: 0.002 min
Response: 20824230
Conc: 20.66 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK72

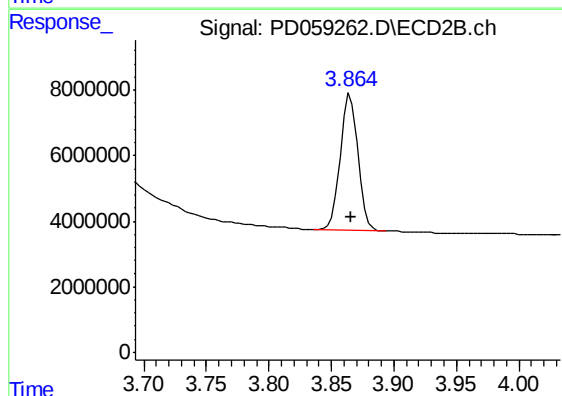


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 40813973
Conc: 24.91 ng/ml

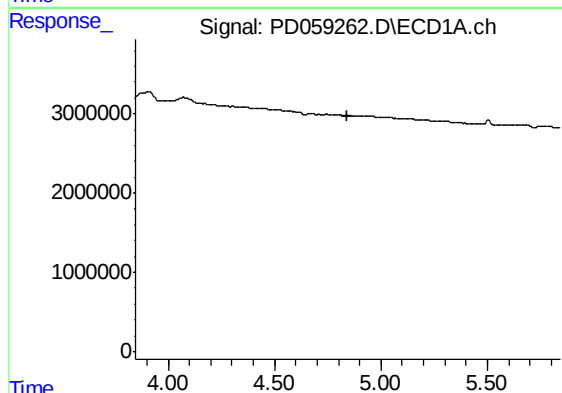


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.845 min
Response: 0
Conc: N.D.

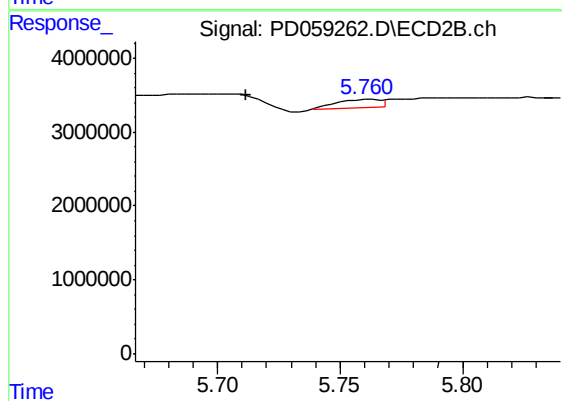

#8 Heptachlor epoxide


R.T.: 5.762 min
Delta R.T.: 0.050 min
Response: 1314101
Conc: 0.65 ng/ml

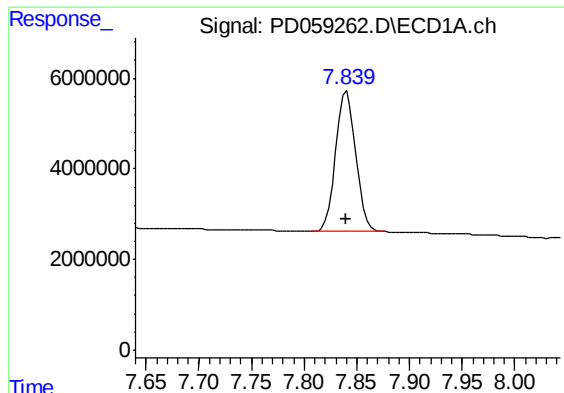

#27 Decachlorobiphenyl

R.T.: 7.841 min
Delta R.T.: 0.000 min
Response: 41074244
Conc: 41.91 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK72

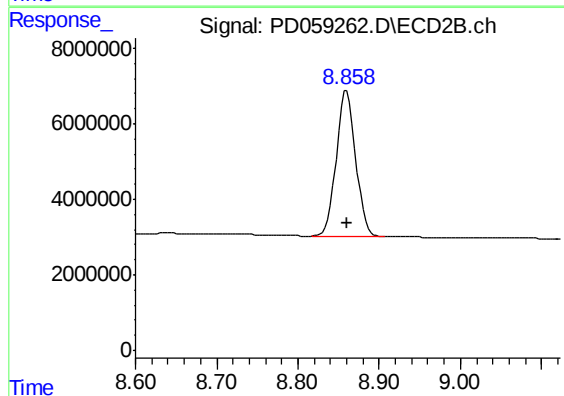

#27 Decachlorobiphenyl

R.T.: 8.860 min
Delta R.T.: 0.000 min
Response: 64376548
Conc: 47.87 ng/ml