

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091820\
 Data File : PD059272.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 17 Sep 2020 12:03
 Operator : DD\AJ
 Sample : PIBLK14
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PIBLK15

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 06:56:45 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090420CLP.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 05 02:06:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.206	3.865	19769042	38880151	19.612	23.725
27) SA Decachlor...	7.839	8.859	37532955	58025430	38.298	43.144
Target Compounds						
8) B Heptachlo...	0.000	5.757f	0	665197	N.D.	0.331


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091820\
Data File : PD059272.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 17 Sep 2020 12:03
Operator : DD\AJ
Sample : PIBLK14
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PIBLK15

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 06:56:45 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD090420CLP.M
Quant Title : GC Extractables
QLast Update : Sat Sep 05 02:06:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

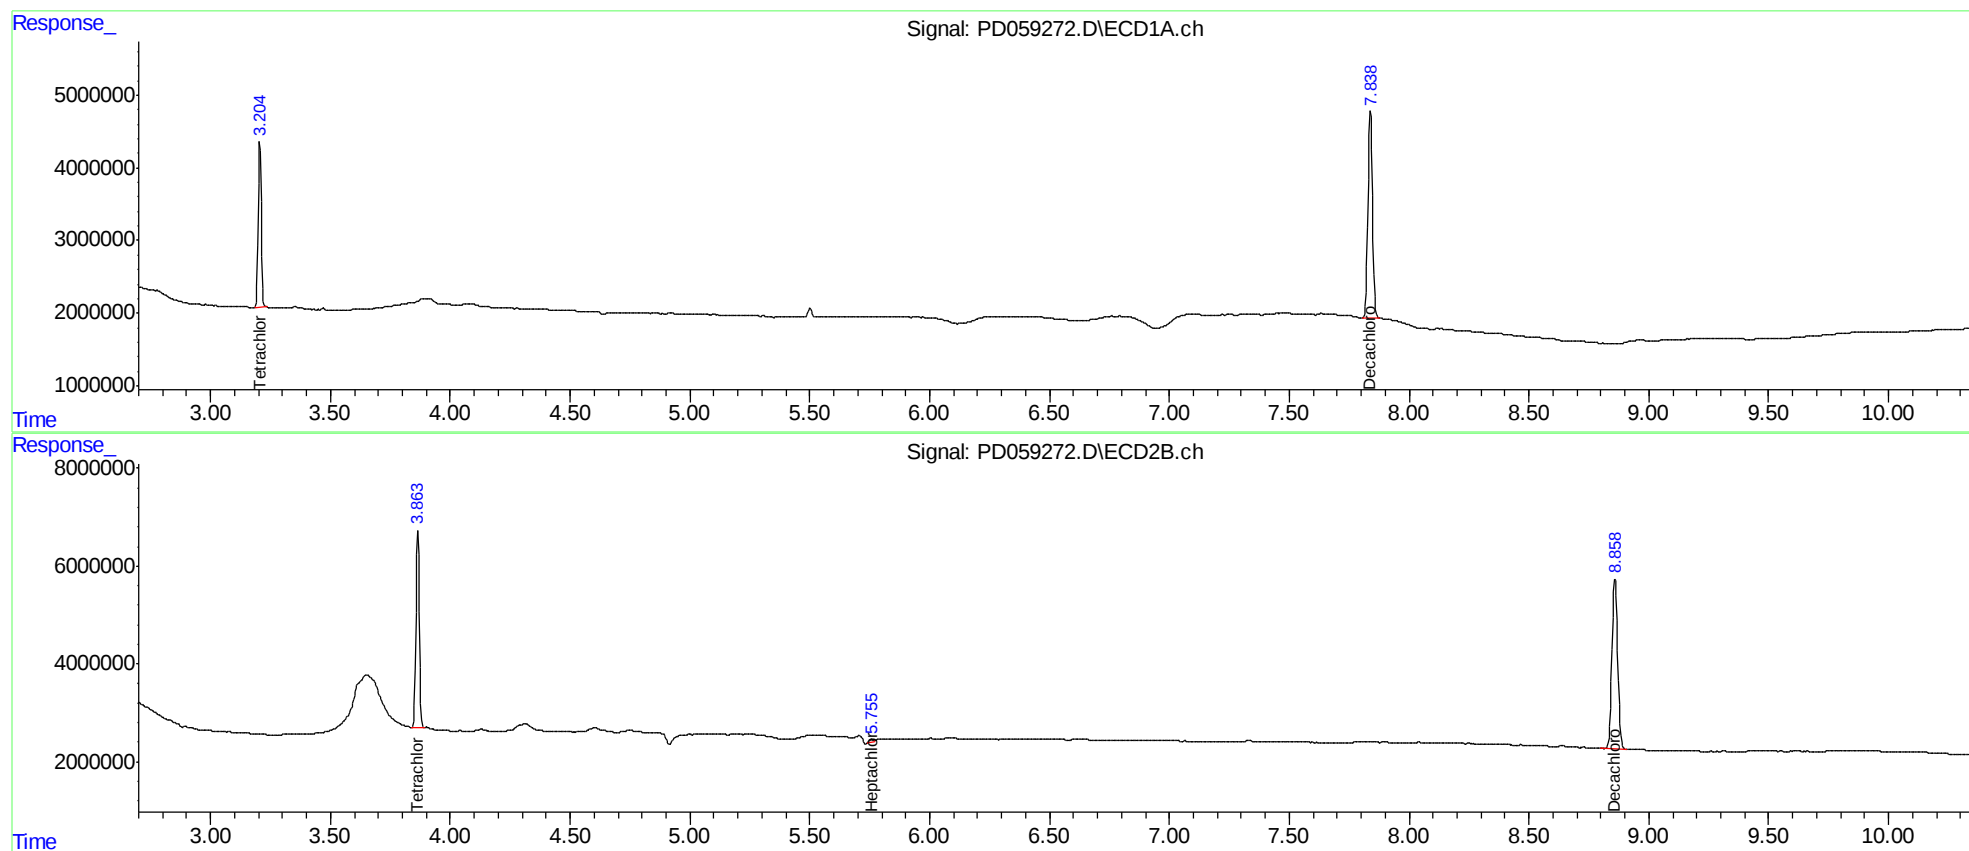


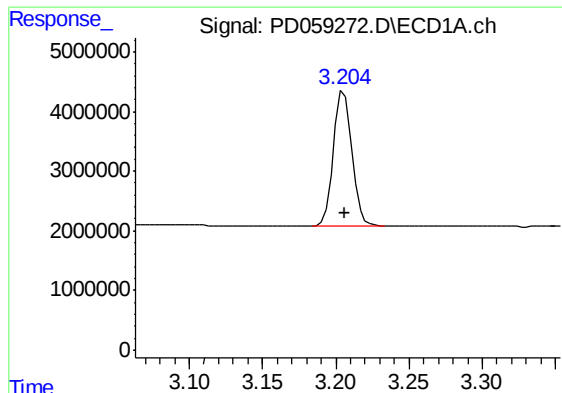

#1 Tetrachloro-m-xylene


R.T.: 3.206 min
Delta R.T.: 0.000 min
Response: 19769042
Conc: 19.61 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK15

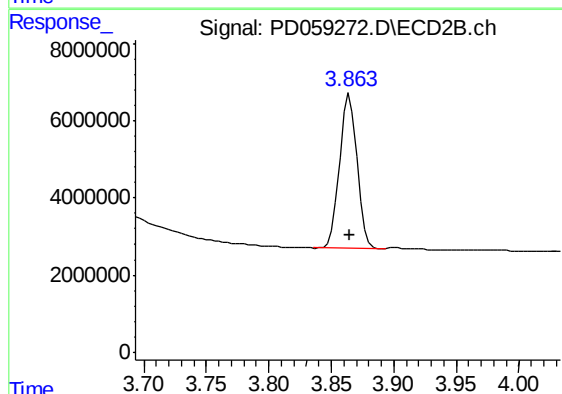


#1 Tetrachloro-m-xylene

R.T.: 3.865 min
Delta R.T.: 0.000 min
Response: 38880151
Conc: 23.73 ng/ml

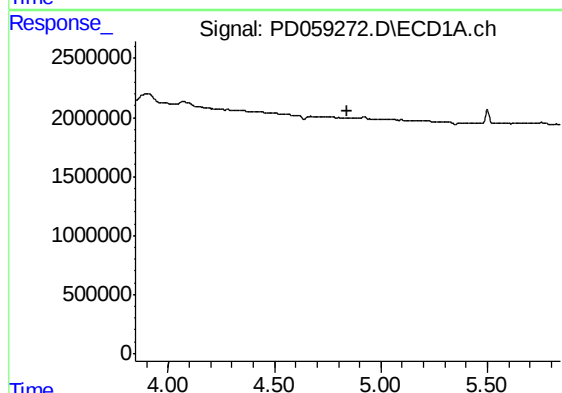


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.845 min
Response: 0
Conc: N.D.

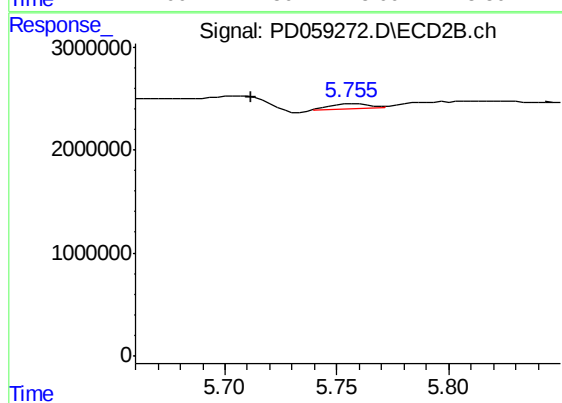

#8 Heptachlor epoxide


R.T.: 5.757 min
Delta R.T.: 0.045 min
Response: 665197
Conc: 0.33 ng/ml

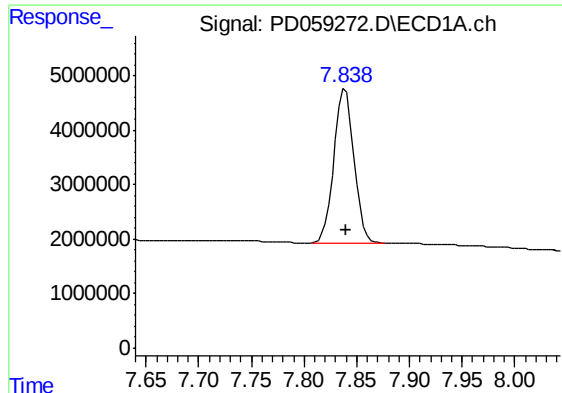

#27 Decachlorobiphenyl

R.T.: 7.839 min
Delta R.T.: 0.000 min
Response: 37532955
Conc: 38.30 ng/ml

Instrument :
ECD_D
ClientSampleId :
PIBLK15

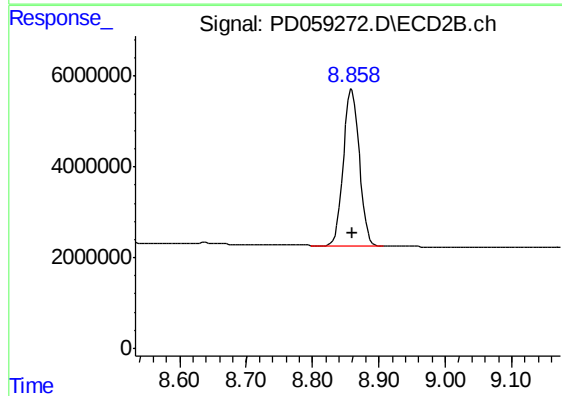

#27 Decachlorobiphenyl

R.T.: 8.859 min
Delta R.T.: 0.000 min
Response: 58025430
Conc: 43.14 ng/ml