

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091824\
 Data File : PD085313.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2024 14:45
 Operator : AR\AJ
 Sample : HEXANE
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 22:29:06 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds


Target Compounds							
8) B	Heptachlo...	5.659	0.000	2527649	0	1.695	N.D. #
9) A	Endosulfan I	0.000	5.255	0	1677937	N.D.	0.438
10) B	trans-Chl...	0.000	5.221f	0	17730184	N.D.	4.311
11) B	cis-Chlor...	0.000	5.221	0	17730184	N.D.	4.226
17) MA	4,4'-DDT	7.054f	0.000	739110	0	0.826	N.D. #
19) B	Endosulfa...	7.054f	0.000	739110	0	0.642	N.D. #
22)	Toxaphene-1	0.000	5.221f	0	17730184	N.D.	699.312
24)	Toxaphene-3	7.054	0.000	739110	0	21.573	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091824\
Data File : PD085313.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2024 14:45
Operator : AR\AJ
Sample : HEXANE
Misc :
ALS Vial : 1 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 22:29:06 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

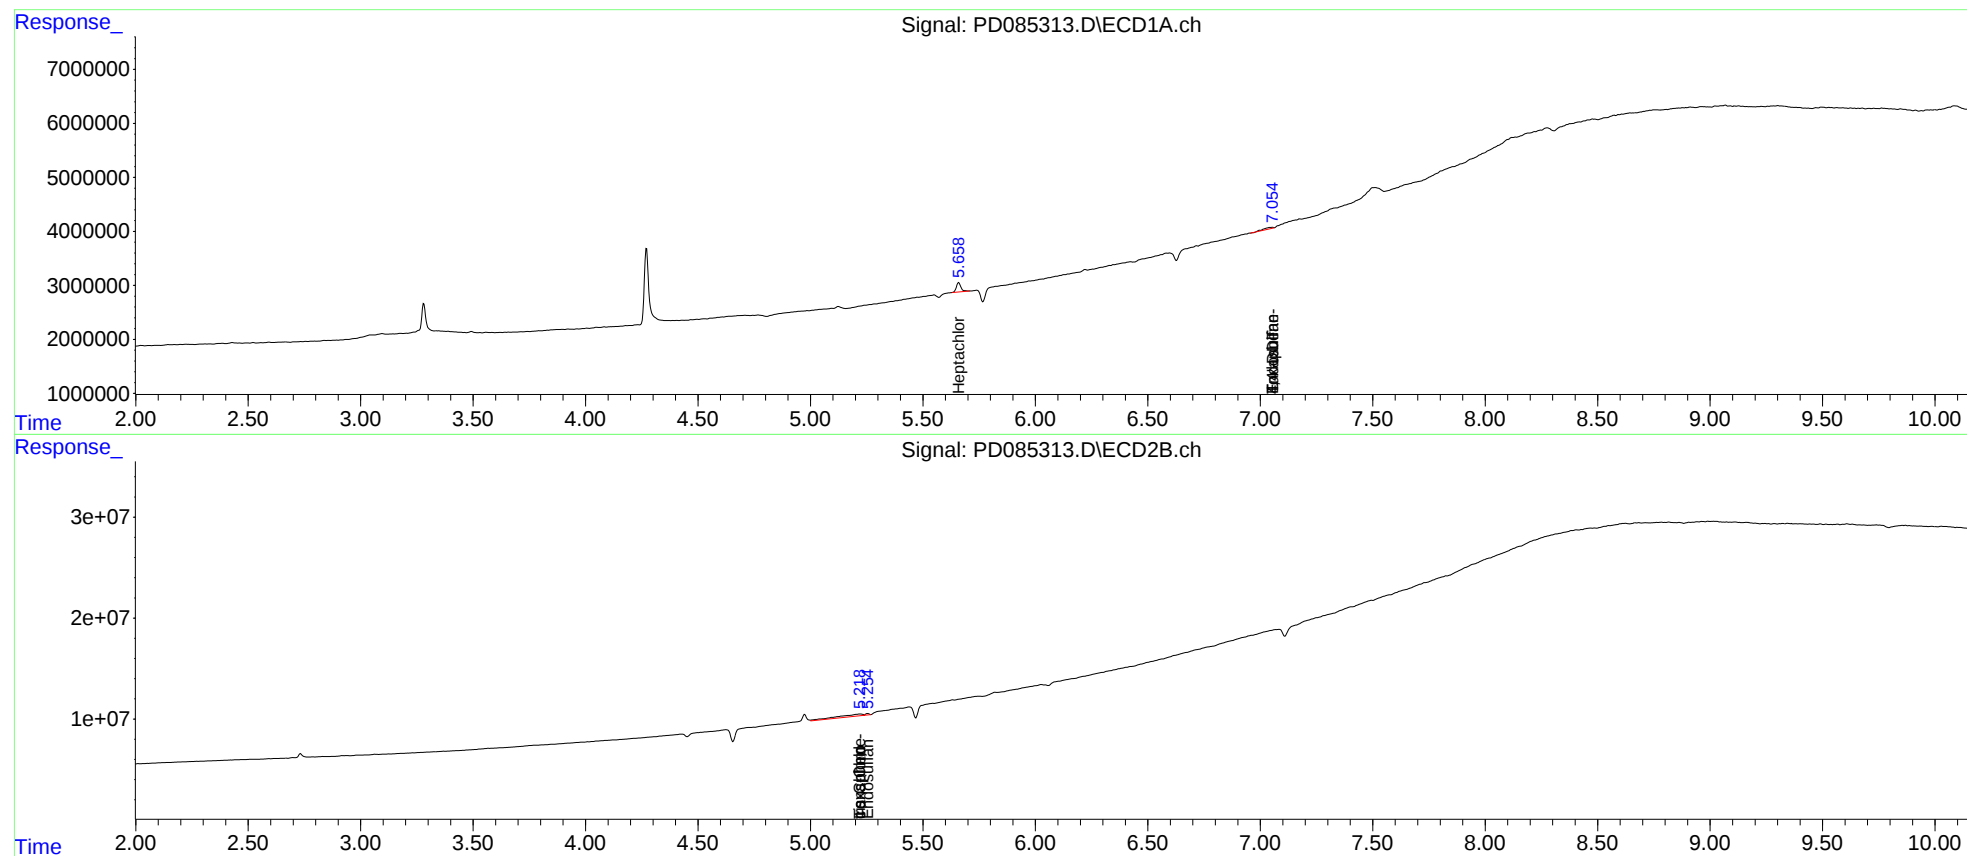

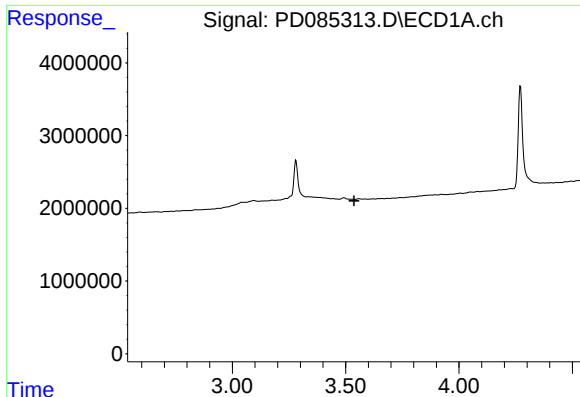


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 3.537 min
Response: 0
Conc: N.D.

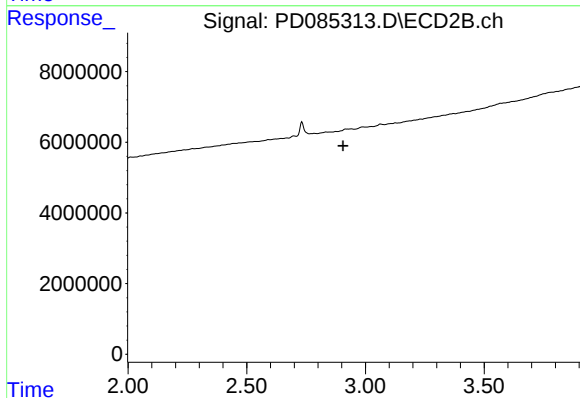


#1 Tetrachloro-m-xylene

R.T.: 0.000 min
Exp R.T. : 2.906 min
Response: 0
Conc: N.D.

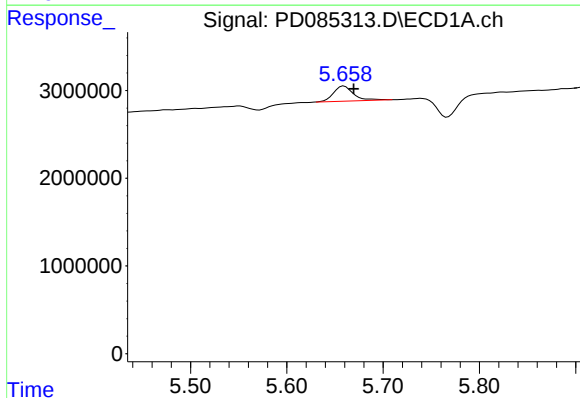


#8 Heptachlor epoxide

R.T.: 5.659 min
Delta R.T.: -0.010 min
Response: 2527649
Conc: 1.69 ng/ml

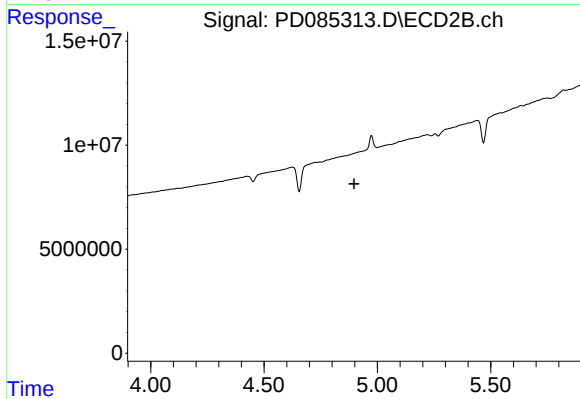


#8 Heptachlor epoxide

R.T.: 0.000 min
Exp R.T. : 4.898 min
Response: 0
Conc: N.D.

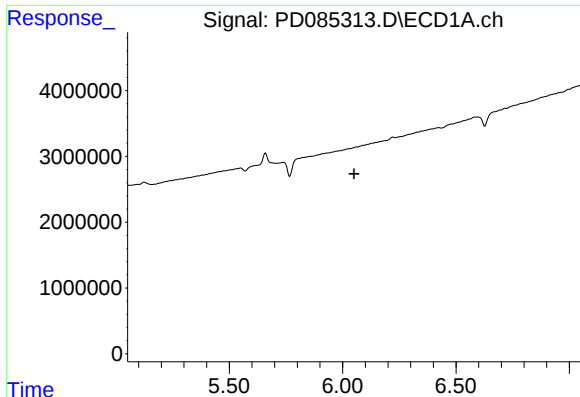


#9 Endosulfan I

R.T.: 0.000 min
Exp R.T. : 6.051 min
Response: 0
Conc: N.D.

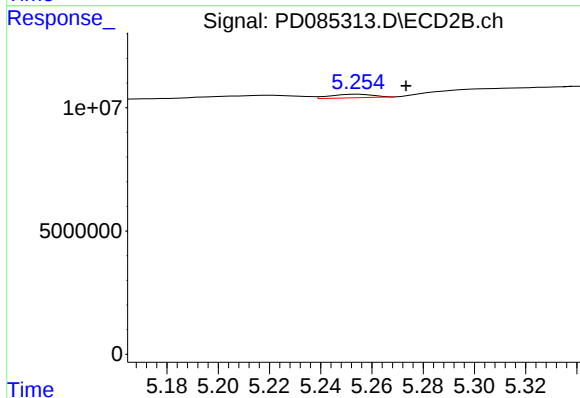


#9 Endosulfan I

R.T.: 5.255 min
Delta R.T.: -0.019 min
Response: 1677937
Conc: 0.44 ng/ml

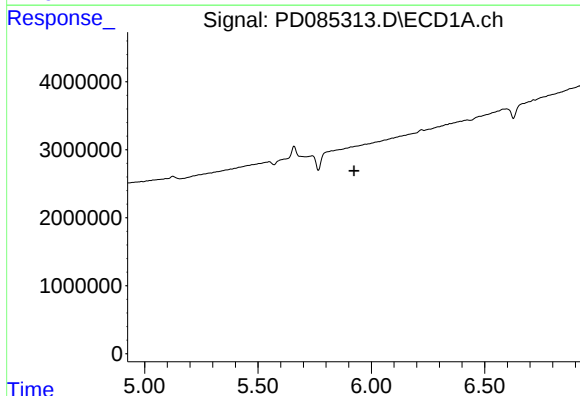


#10 trans-Chlordane

R.T.: 0.000 min
Exp R.T. : 5.924 min
Response: 0
Conc: N.D.

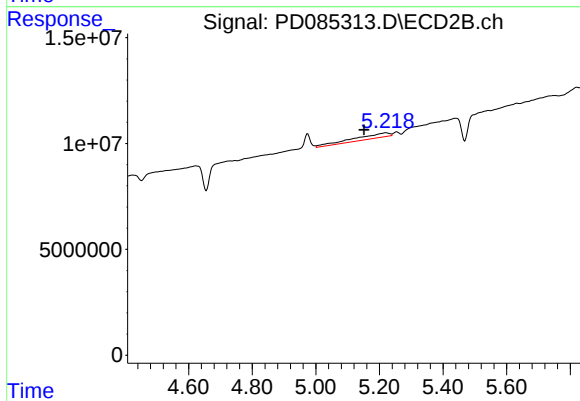


#10 trans-Chlordane

R.T.: 5.221 min
Delta R.T.: 0.069 min
Response: 17730184
Conc: 4.31 ng/ml

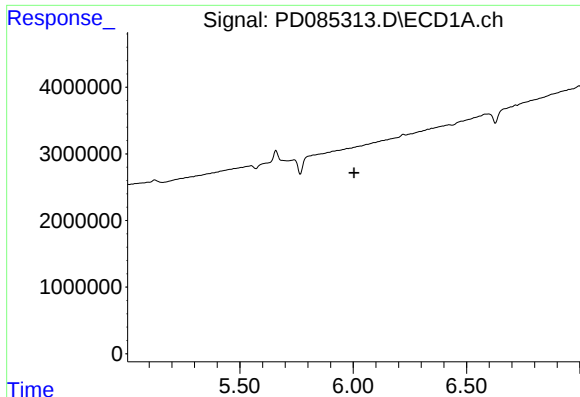


#11 cis-Chlordane

R.T.: 0.000 min
Exp R.T. : 6.004 min
Response: 0
Conc: N.D.

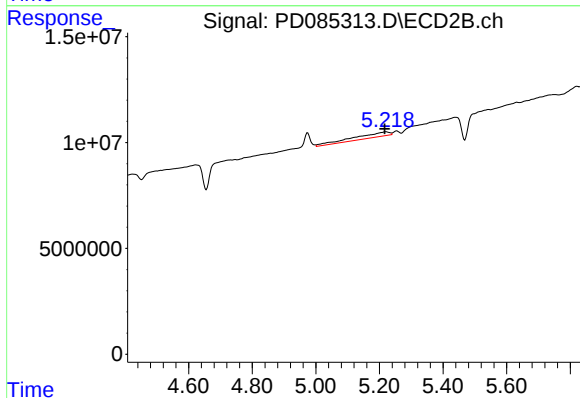


#11 cis-Chlordane

R.T.: 5.221 min
Delta R.T.: 0.004 min
Response: 17730184
Conc: 4.23 ng/ml

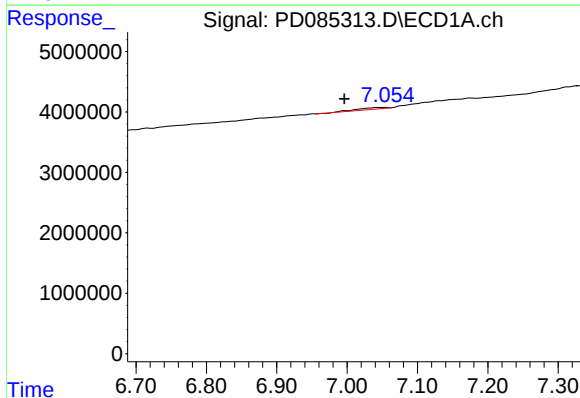


#17 4,4'-DDT

R.T.: 7.054 min
Delta R.T.: 0.058 min
Response: 739110
Conc: 0.83 ng/ml

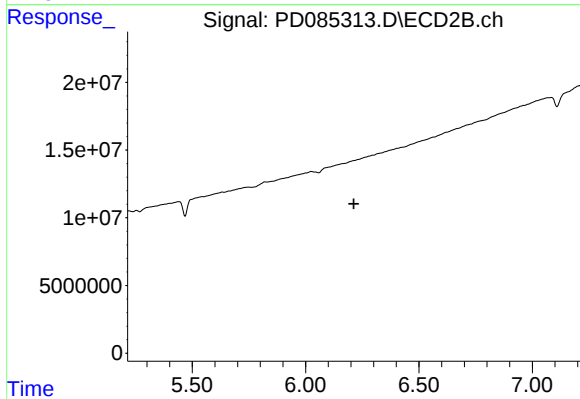


#17 4,4'-DDT

R.T.: 0.000 min
Exp R.T. : 6.213 min
Response: 0
Conc: N.D.

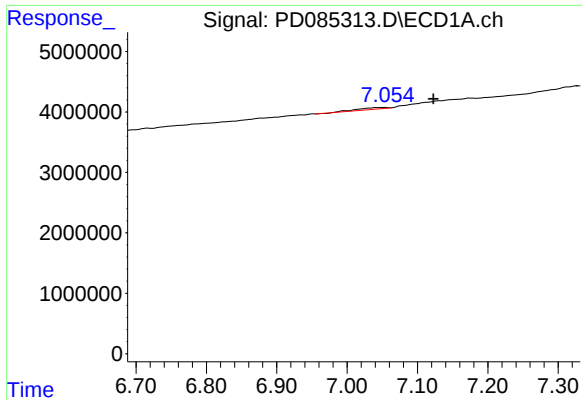


#19 Endosulfan Sulfate

R.T.: 7.054 min
Delta R.T.: -0.069 min
Response: 739110
Conc: 0.64 ng/ml

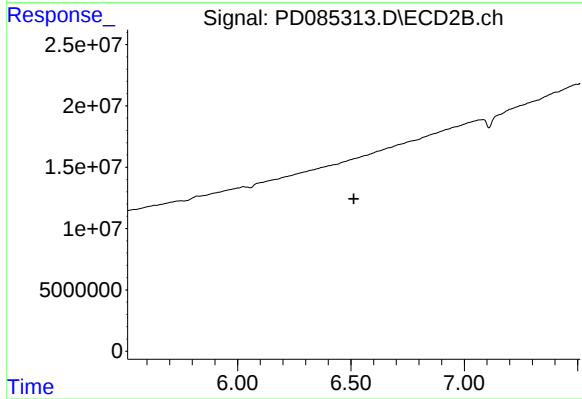


#19 Endosulfan Sulfate

R.T.: 0.000 min
Exp R.T. : 6.513 min
Response: 0
Conc: N.D.

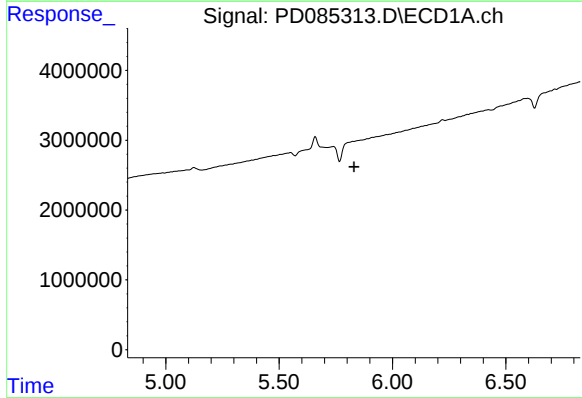


#22 Toxaphene-1

R.T.: 0.000 min
Exp R.T. : 5.831 min
Response: 0
Conc: N.D.

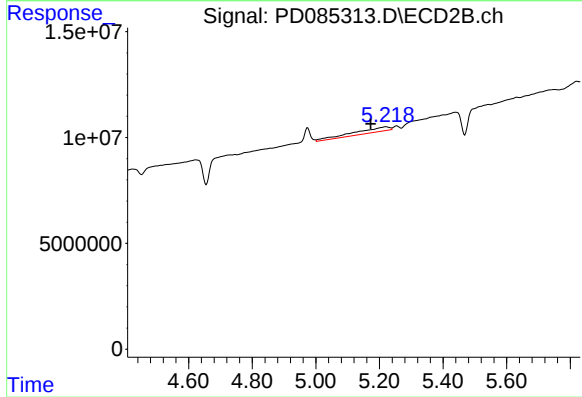


#22 Toxaphene-1

R.T.: 5.221 min
Delta R.T.: 0.048 min
Response: 17730184
Conc: 699.31 ng/ml

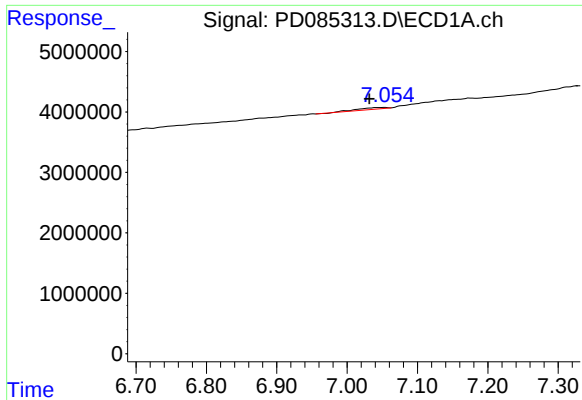


#24 Toxaphene-3

R.T.: 7.054 min
Delta R.T.: 0.022 min
Response: 739110
Conc: 21.57 ng/ml

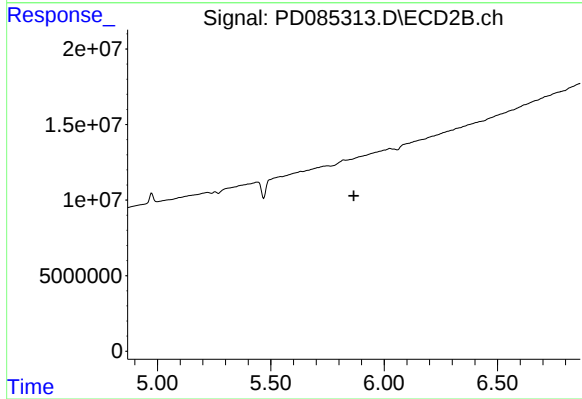


#24 Toxaphene-3

R.T.: 0.000 min
Exp R.T. : 5.866 min
Response: 0
Conc: N.D.

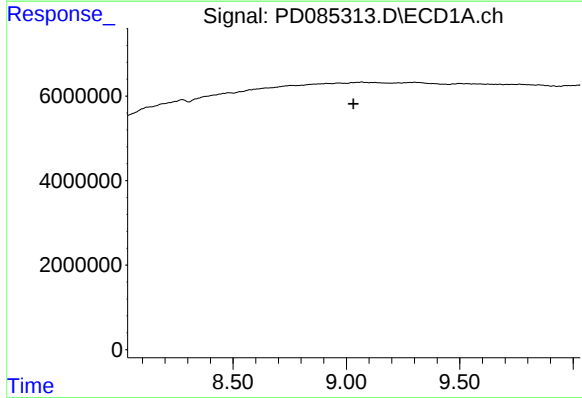

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 9.031 min
Response: 0
Conc: N.D.

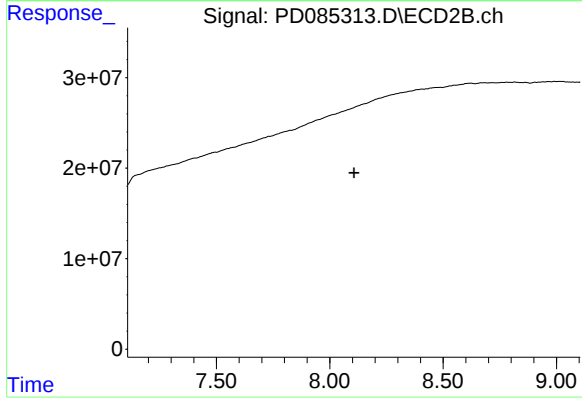

#27 Decachlorobiphenyl

R.T.: 0.000 min
Exp R.T. : 8.107 min
Response: 0
Conc: N.D.