

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091824\
 Data File : PD085369.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2024 03:51
 Operator : AR\AJ
 Sample : P4016-19MS
 Misc :
 ALS Vial : 52 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDC23MS

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/19/2024
 Supervised By :Ankita Jodhani 09/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 05:21:03 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.531	2.912	91997048	11339.4E6	90.960m	3204.304m#
27)	SA Decachlor...	9.030	8.094	18838810	25800155	14.424m	7.420m#
Target Compounds							
2)	A alpha-BHC	3.982	3.412	399.7E6	793.8E6	235.109	156.566 #
3)	MA gamma-BHC...	4.249f	3.744	98111.9E6	3065.7E6	60643.183m	632.645m#
4)	MA Heptachlor	4.908	4.096	90783002	311.5E6	59.004m	73.172m
5)	MB Aldrin	5.249	4.416	65373169	60457344	40.875m	13.613m#
6)	B beta-BHC	4.494	4.037	70389640	79447865	96.906m	36.647m#
7)	B delta-BHC	4.742	4.277	488.5E6	957.5E6	297.859	192.885m#
8)	B Heptachlo...	5.665	4.886	54951322	736.3E6	36.844m	173.859m#
9)	A Endosulfan I	6.052	5.269	129.3E6	232.0E6	93.949m	60.534 #
10)	B trans-Chl...	5.922	5.143	72002807	247.3E6	51.052m	60.130m
11)	B cis-Chlor...	6.002	5.212	136.6E6	313.4E6	92.359m	74.698
12)	B 4,4'-DDE	6.171	5.393	222.8E6	386.0E6	178.573m	98.402m#
13)	MA Dieldrin	6.324	5.534	133.1E6	326.2E6	90.258	75.918
14)	MA Endrin	6.549	5.810	109.6E6	358.0E6	97.102m	96.700m
15)	B Endosulfa...	6.761	6.102	110.8E6	381.3E6	83.949m	102.826m
16)	A 4,4'-DDD	6.681	5.952	137.1E6	256.9E6	138.846	75.703 #
17)	MA 4,4'-DDT	6.995	6.206	101.5E6	350.6E6	113.351m	109.599
18)	B Endrin al...	6.891	6.282	99568858	202.9E6	110.252	71.068 #
19)	B Endosulfa...	7.125	6.507	913.8E6	234.0E6	793.221m	65.528 #
20)	A Methoxychlor	7.476	6.776	1826.4E6	680.4E6	3506.186m	411.330m#
21)	B Endrin ke...	7.601	7.018	196.9E6	322.9E6	161.011	73.330 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091824\
Data File : PD085369.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2024 03:51
Operator : AR\AJ
Sample : P4016-19MS
Misc :
ALS Vial : 52 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 05:21:03 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

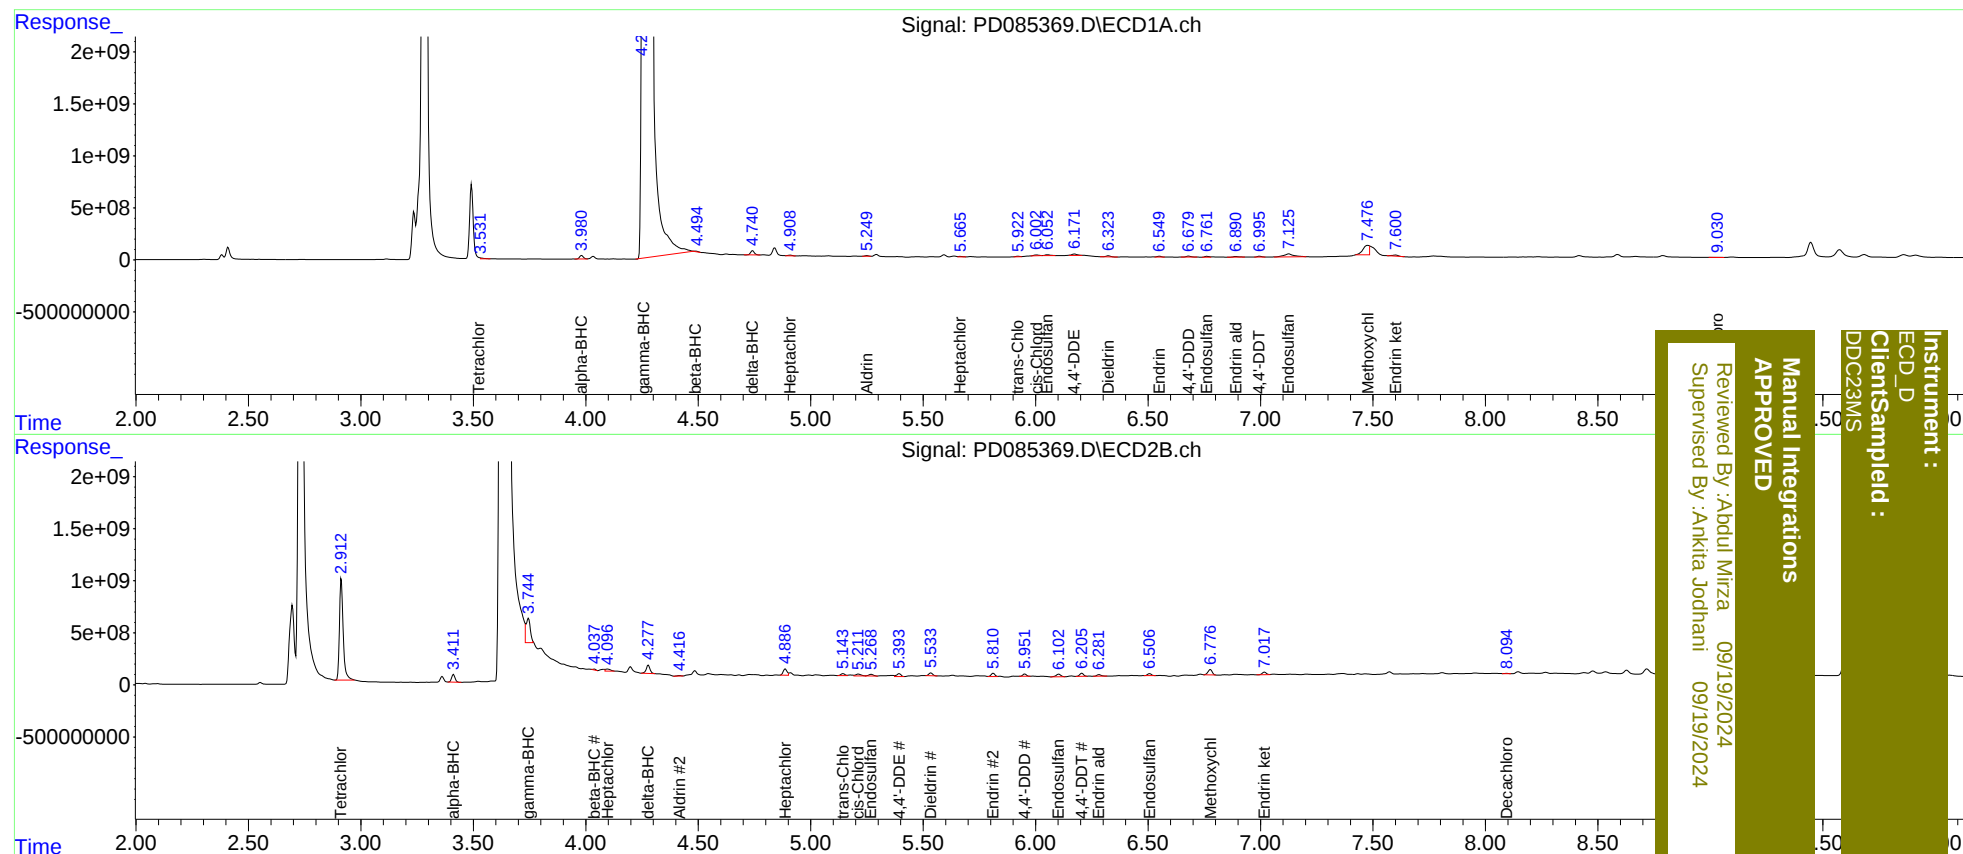

Reviewed By: Abdul Mirza 09/19/2024
Supervised By: Ankita Jodhani 09/19/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
DDC23MS