

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091824\
 Data File : PD085333.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2024 19:50
 Operator : AR\AJ
 Sample : P3910-05RE
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDC07RE

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/19/2024
 Supervised By : Ankita Jodhani 09/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 22:34:01 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.533	2.901	20627726	63410419	20.395m	17.919m
2)	SA Decachlor...	9.033	8.100	16659698	43365785	12.756m	12.471m
Target Compounds							
2)	A alpha-BHC	3.981	3.411	5574802	27476877	3.279	5.419 #
9)	A Endosulfan I	6.063	5.276	2641458	9507457	1.920m	2.480m#
10)	B trans-Chl...	5.912	5.142	4746662	18941435	3.366m	4.605m#
11)	B cis-Chlor...	5.995	5.217	3145145	21010451	2.127m	5.008m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091824\
Data File : PD085333.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2024 19:50
Operator : AR\AJ
Sample : P3910-05RE
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 22:34:01 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

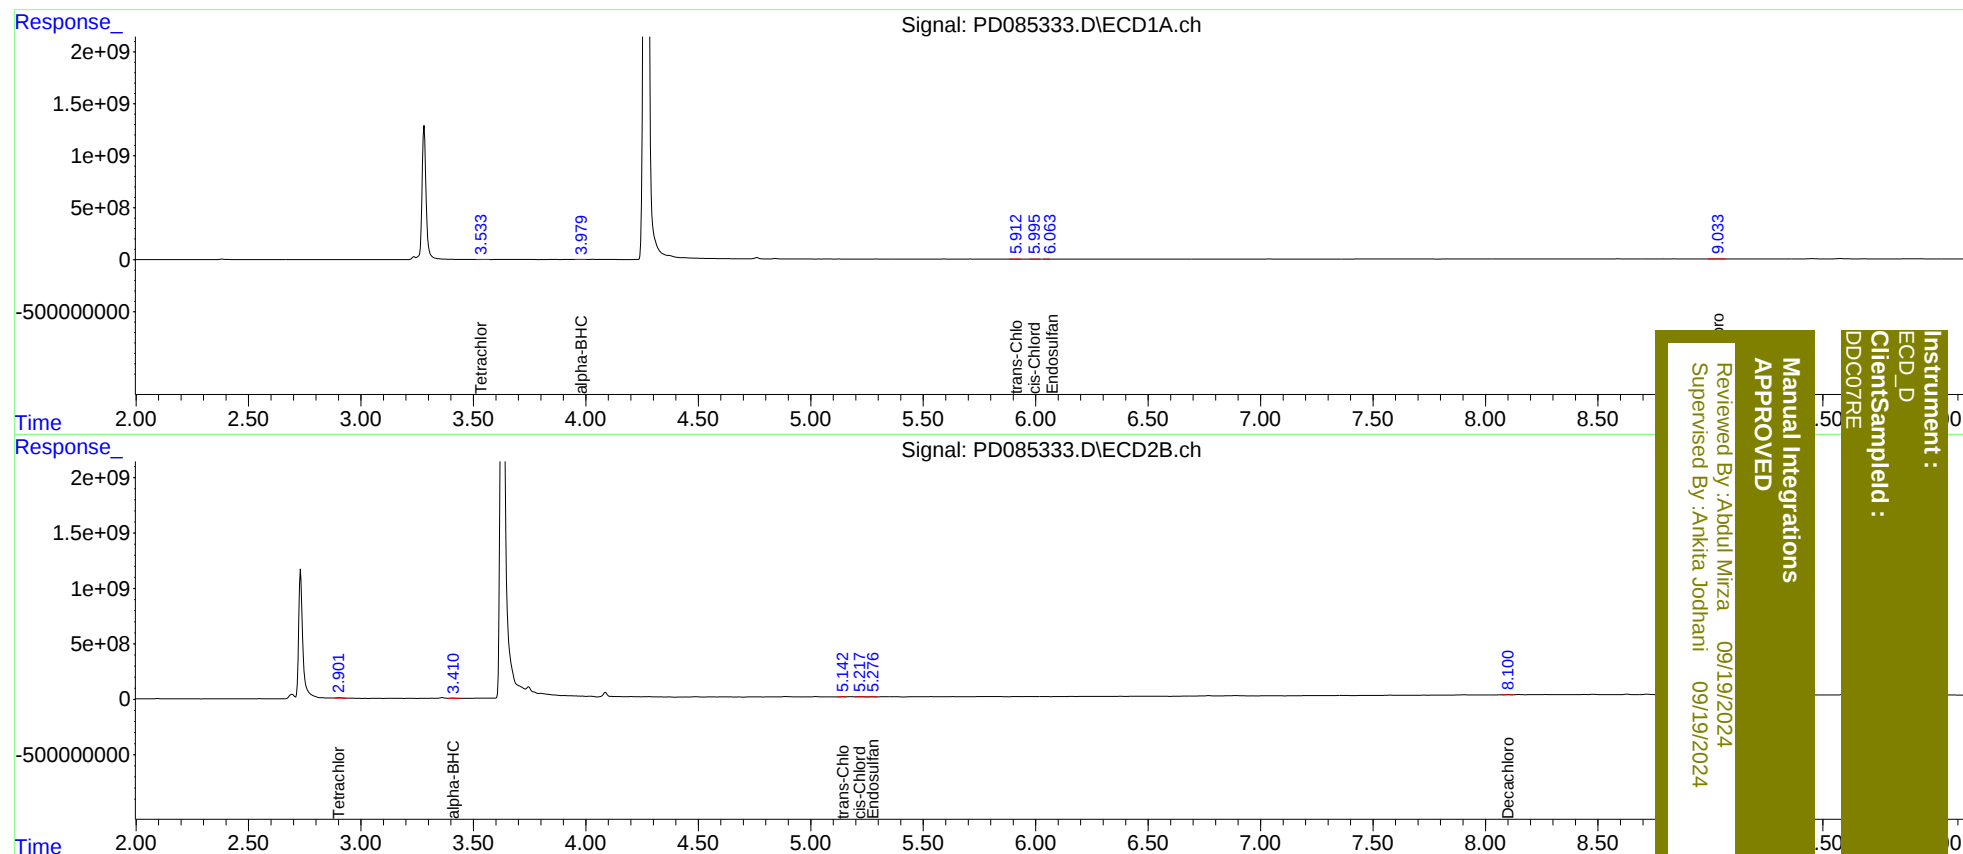

Reviewed By: Abdul Mirza 09/19/2024
Supervised By: Ankita Jodhani 09/19/2024

Manual Integrations
APPROVED

Instrument :
ECD_D
Client Sampled :
DDC07RE