

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091824\
 Data File : PD085334.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2024 20:03
 Operator : AR\AJ
 Sample : P3910-06RE
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDC08RE

Manual Integrations
 APPROVED

Reviewed By :Abdul Mirza 09/19/2024
 Supervised By :Ankita Jodhani 09/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 22:34:21 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.534	2.900	18328260	71501856	18.122m	20.205m
2) SA Decachlor...	9.031	8.100	17984204	34115031	13.770m	9.811 #
Target Compounds						
9) A Endosulfan I	6.053	5.271	12750716	35752182	9.268m	9.327m
10) B trans-Chl...	5.910	5.140	5898854	25723054	4.182m	6.254m#
11) B cis-Chlor...	5.993	5.216	14923219	67956755	10.093m	16.197m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091824\
Data File : PD085334.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2024 20:03
Operator : AR\AJ
Sample : P3910-06RE
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 22:34:21 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

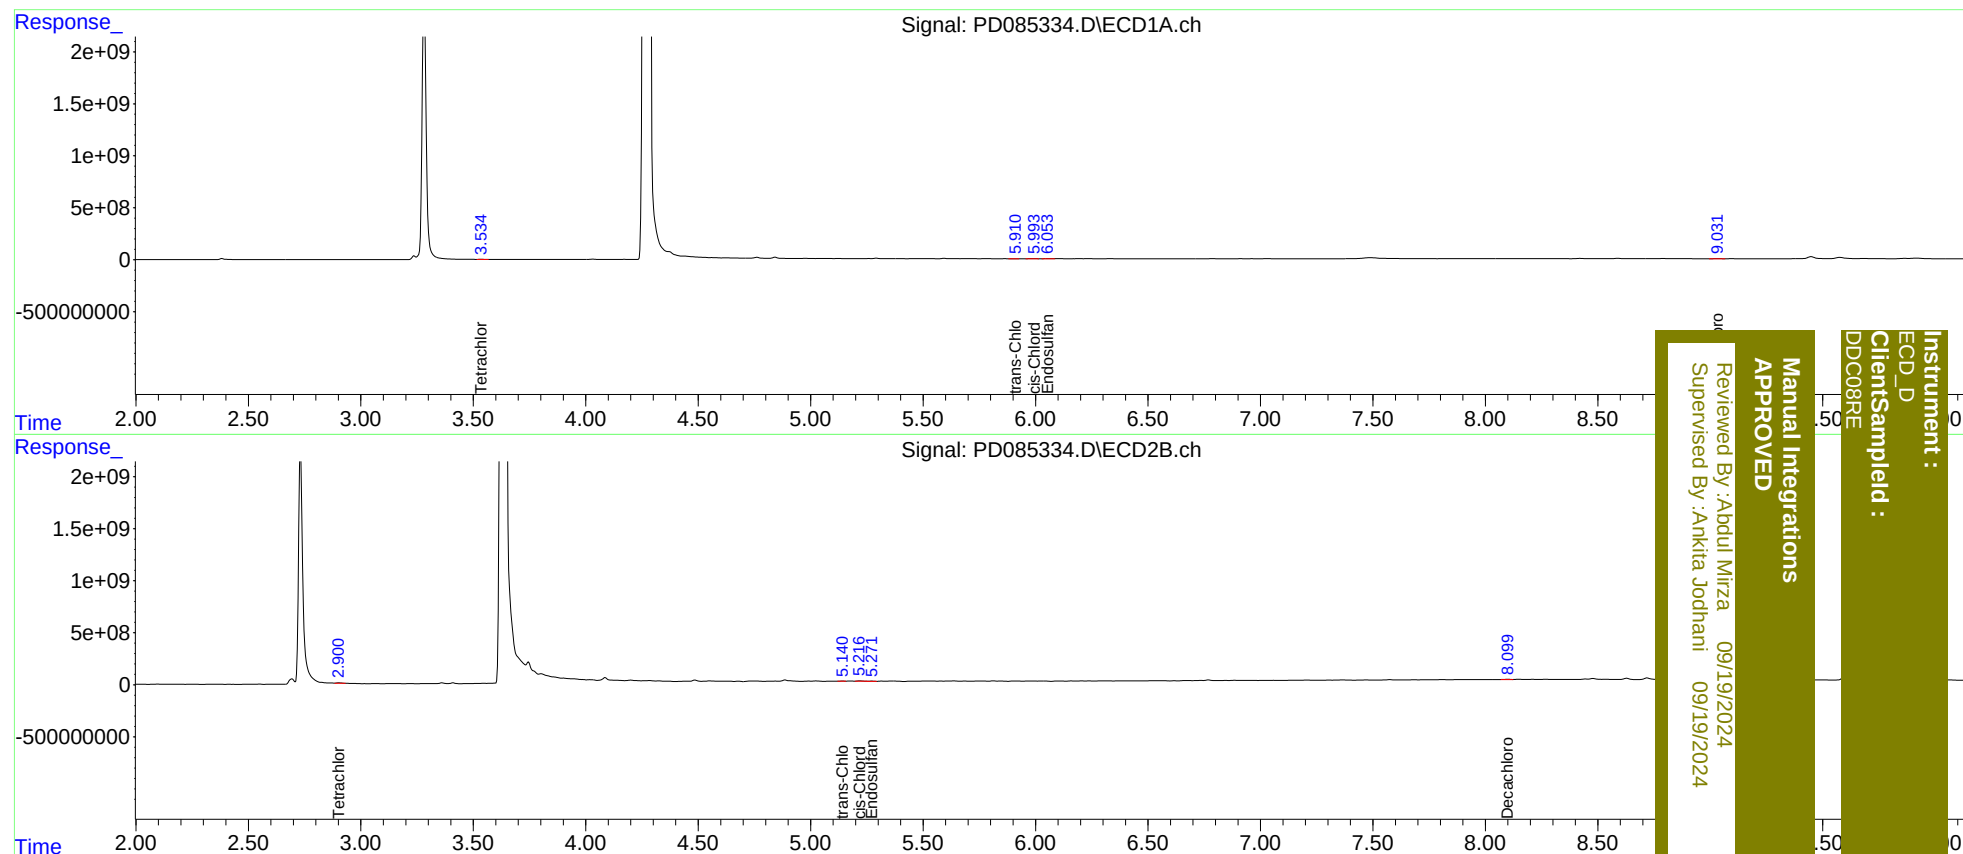

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 09/19/2024
Supervised By: Ankita Jodhani 09/19/2024

Instrument :
ECD_D
Client Sampled :
DDC08RE