

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091824\
 Data File : PD085343.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2024 22:03
 Operator : AR\AJ
 Sample : P3910-15RE
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDC35RE

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/19/2024
 Supervised By : Ankita Jodhani 09/19/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 18 22:37:05 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
 Quant Title : GC Extractables
 QLast Update : Tue Aug 27 02:47:48 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.535	2.907	21115959	89120365	20.878m	25.184m
2) SA Decachlor...	9.033	8.097	16654531	21211894	12.752m	6.100m#
Target Compounds						
6) B beta-BHC	4.491	4.039	11299345	11003807	15.556m	5.076 #
9) A Endosulfan I	6.058	5.277	2827727	3400730	2.055m	0.887m#
10) B trans-Chl...	5.902	5.147	6638989	11744023	4.707m	2.855m#
16) A 4,4'-DDD	6.681	5.957	10262256	11958573	10.394m	3.524m#

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091824\
Data File : PD085343.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2024 22:03
Operator : AR\AJ
Sample : P3910-15RE
Misc :
ALS Vial : 26 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 18 22:37:05 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD082524CLP.M
Quant Title : GC Extractables
QLast Update : Tue Aug 27 02:47:48 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

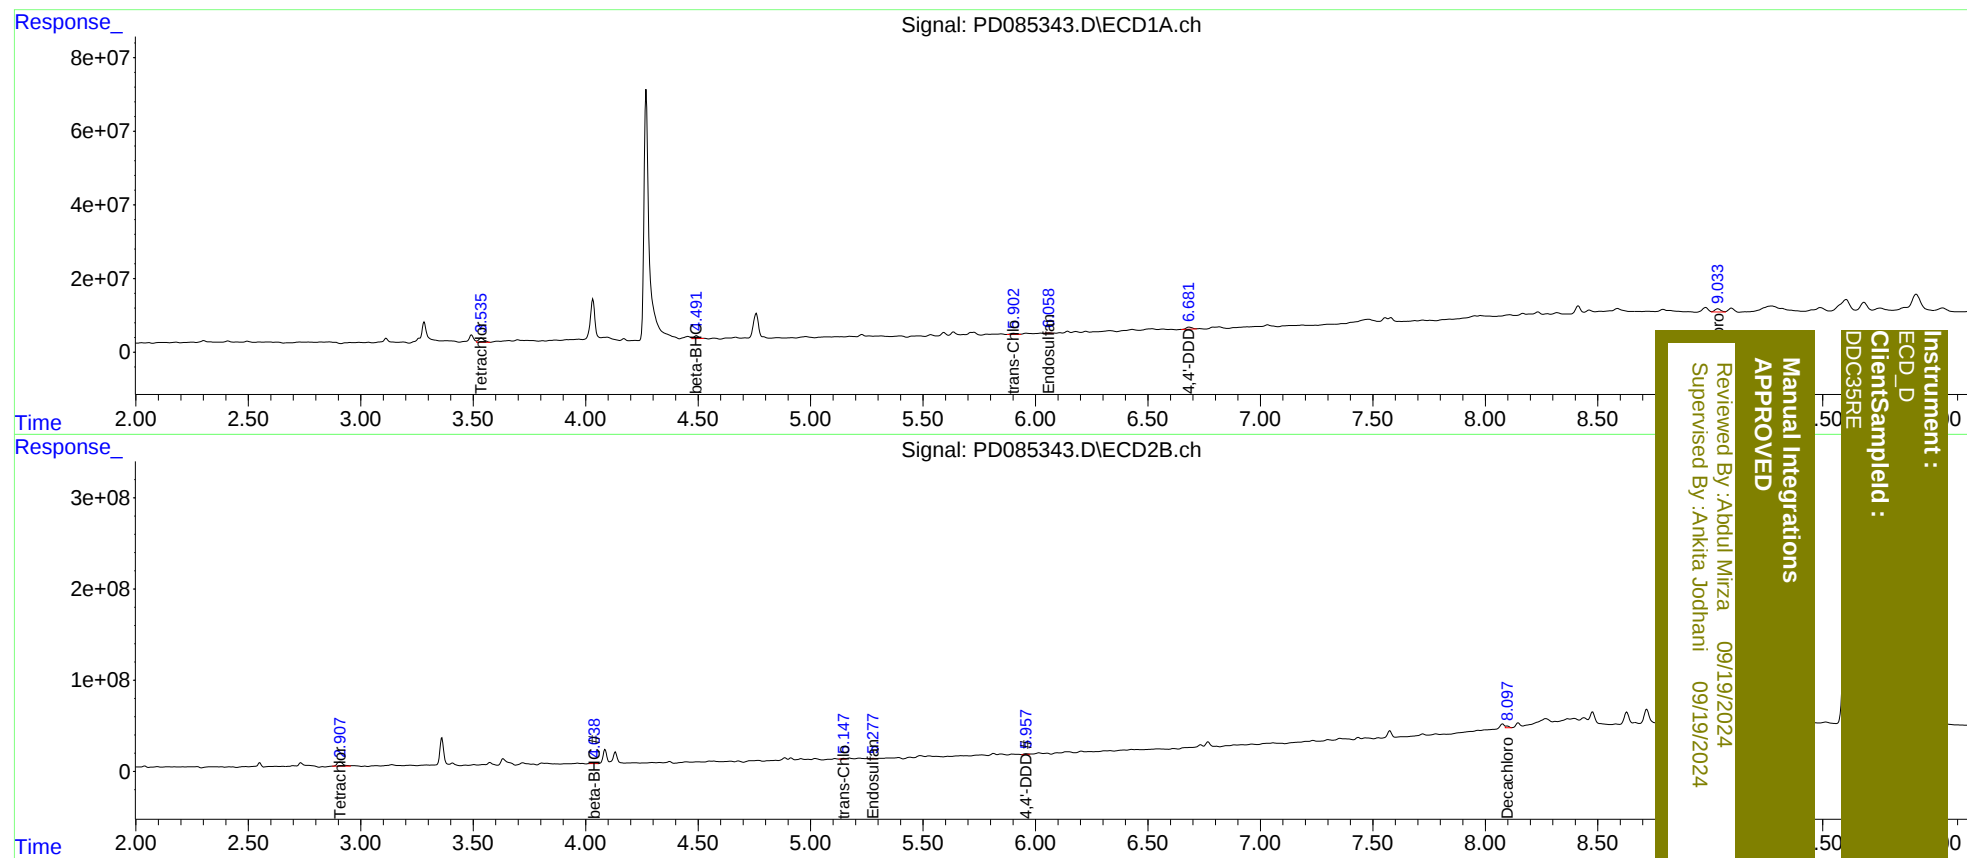

Manual Integrations
APPROVED
Reviewed By: Abdul Mirza 09/19/2024
Supervised By: Ankita Jodhani 09/19/2024

Instrument :
ECD_D
Client Sampled :
DDC35RE