

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091825\
 Data File : PD090336.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2025 11:51
 Operator : AR\AJ
 Sample : PCHLORICC750
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 05:32:01 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091825.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:30:47 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.875	190.9E6	2062.1E6	72.553	72.446
28)	SA Decachlor...	9.067	8.064	281.8E6	1917.4E6	71.115	71.360
Target Compounds							
23)	Chlordane-1	4.710	3.899	151.2E6	841.1E6	738.946	717.733
24)	Chlordane-2	5.237	4.481	147.9E6	860.6E6	720.193	710.551
25)	Chlordane-3	5.942	5.119	619.7E6	2640.8E6	751.215	721.020
26)	Chlordane-4	6.027	5.183	742.3E6	2240.8E6	744.193	714.115
27)	Chlordane-5	6.867	6.083	129.7E6	1067.8E6	742.141	715.431



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091825\
Data File : PD090336.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2025 11:51
Operator : AR\AJ
Sample : PCHLORICC750
Misc :
ALS Vial : 11 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 05:32:01 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091825.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:30:47 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

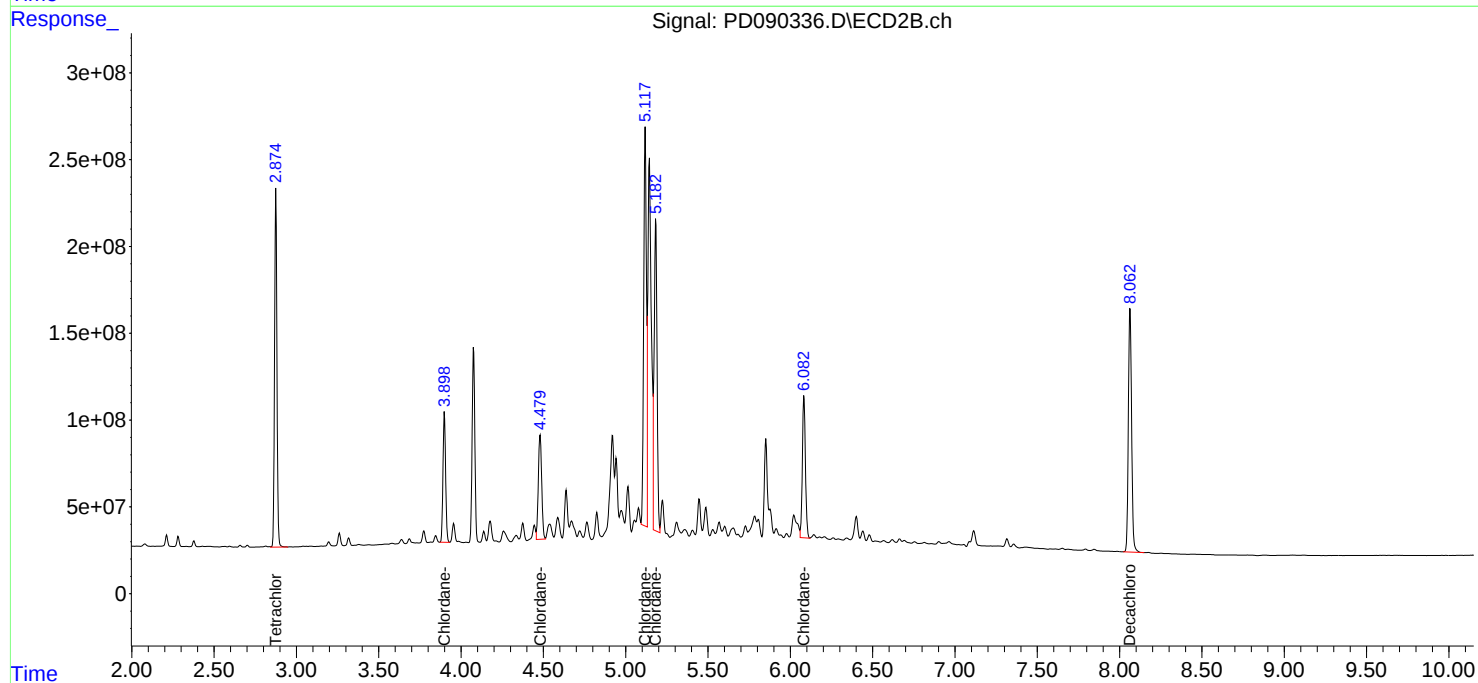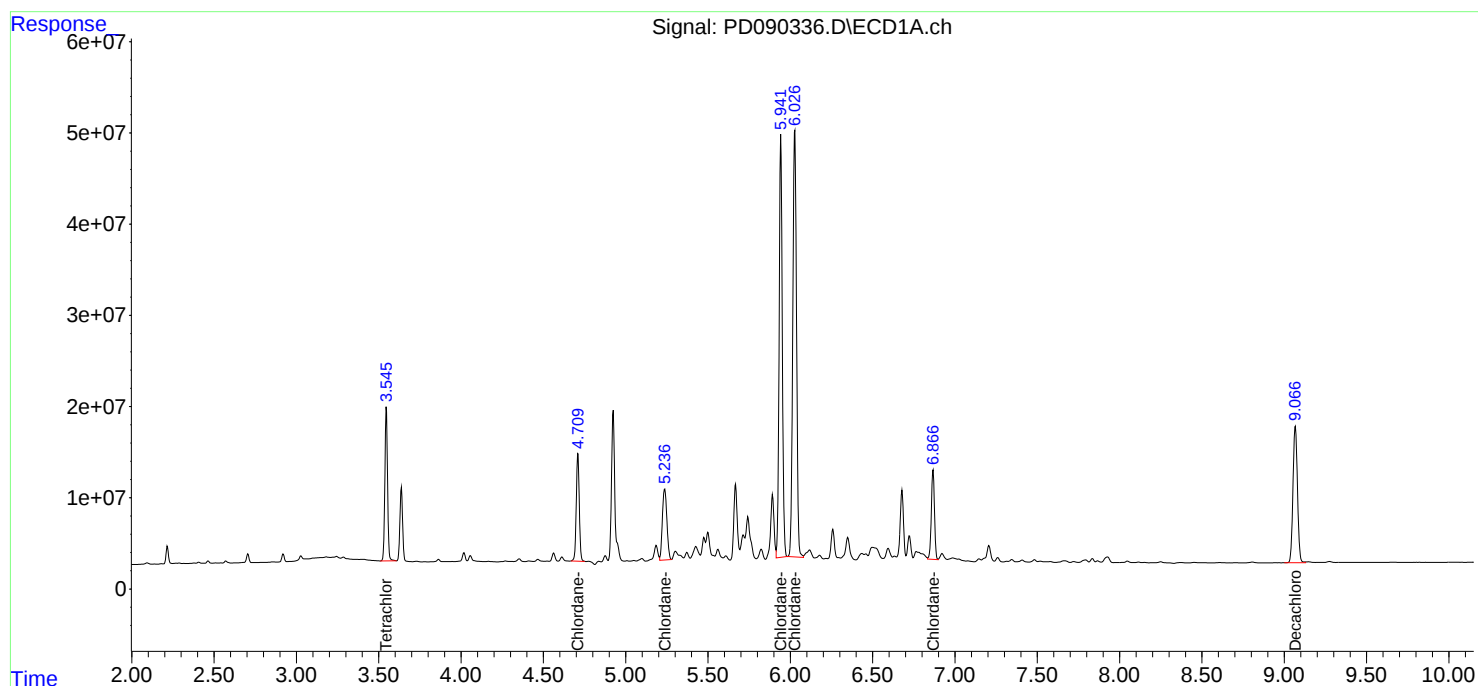


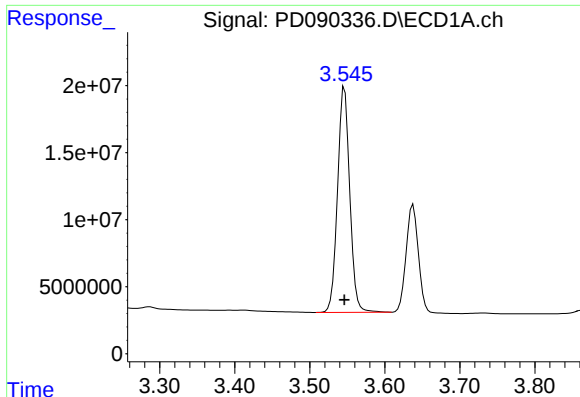

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 190863770
Conc: 72.55 ng/ml

Instrument :
ECD_D
ClientSampleId :

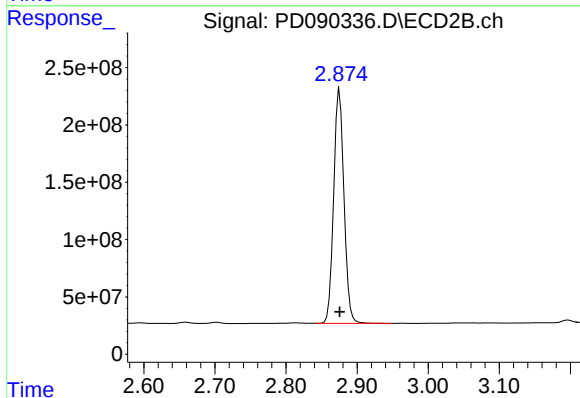


#1 Tetrachloro-m-xylene

R.T.: 2.875 min
Delta R.T.: 0.000 min
Response: 2062054846
Conc: 72.45 ng/ml

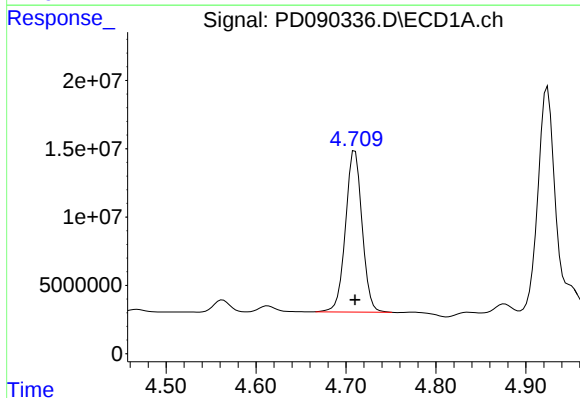


#23 Chlordane-1

R.T.: 4.710 min
Delta R.T.: 0.000 min
Response: 151238542
Conc: 738.95 ng/ml

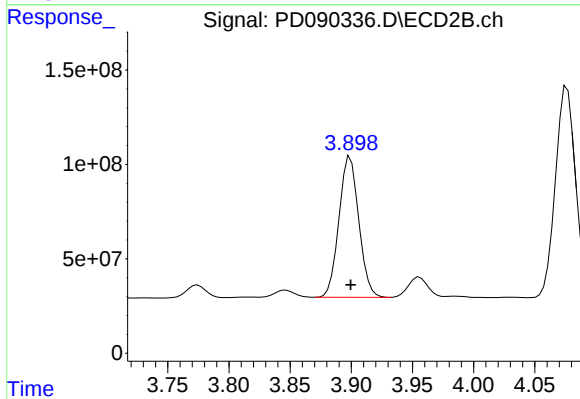

#23 Chlordane-1


R.T.: 3.899 min
Delta R.T.: 0.000 min
Response: 841095146
Conc: 717.73 ng/ml

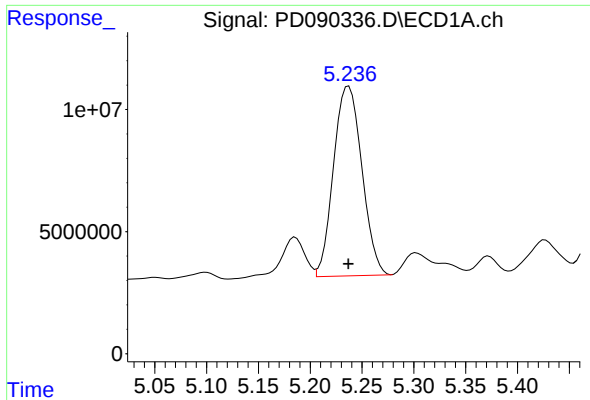

#24 Chlordane-2


R.T.: 5.237 min
Delta R.T.: 0.000 min
Response: 147861417
Conc: 720.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

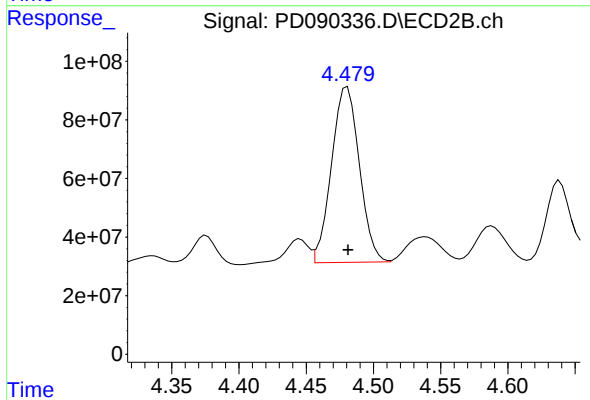


#24 Chlordane-2

R.T.: 4.481 min
Delta R.T.: 0.000 min
Response: 860596721
Conc: 710.55 ng/ml

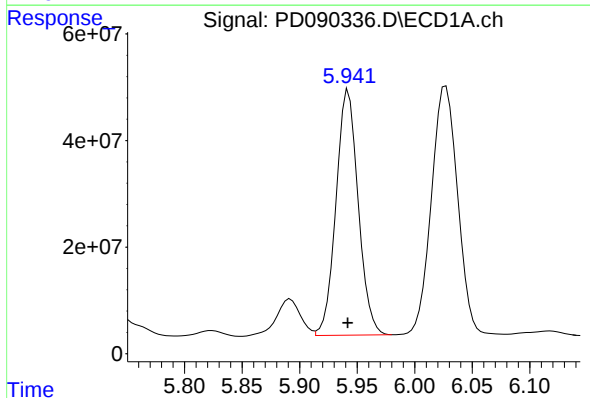


#25 Chlordane-3

R.T.: 5.942 min
Delta R.T.: 0.000 min
Response: 619716728
Conc: 751.21 ng/ml

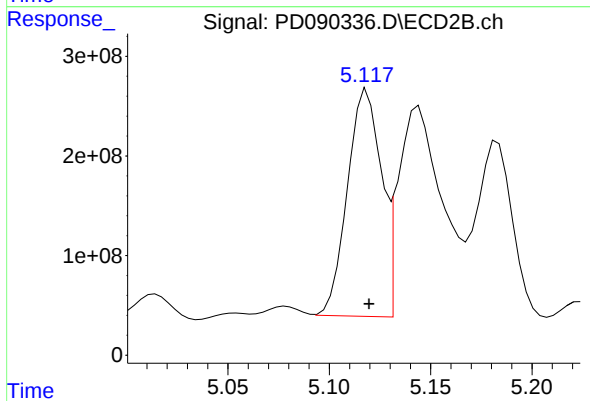

#25 Chlordane-3


R.T.: 5.119 min
Delta R.T.: 0.000 min
Response: 2640767796
Conc: 721.02 ng/ml

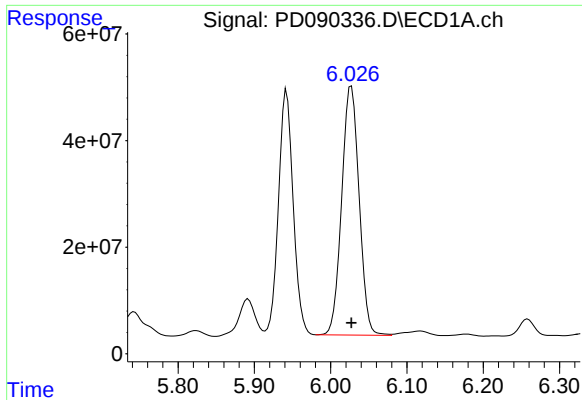

#26 Chlordane-4


R.T.: 6.027 min
Delta R.T.: 0.000 min
Response: 742263570
Conc: 744.19 ng/ml

Instrument :
ECD_D
ClientSampleId :

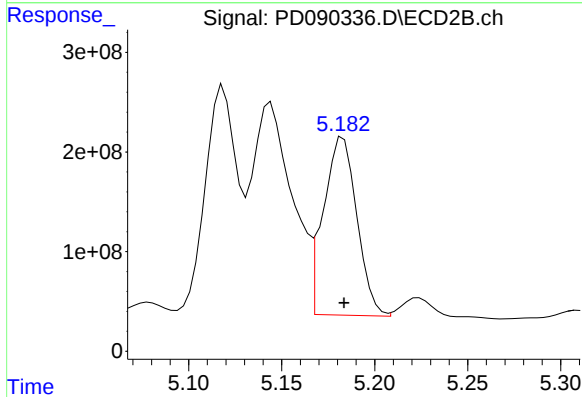


#26 Chlordane-4

R.T.: 5.183 min
Delta R.T.: 0.000 min
Response: 2240753558
Conc: 714.11 ng/ml

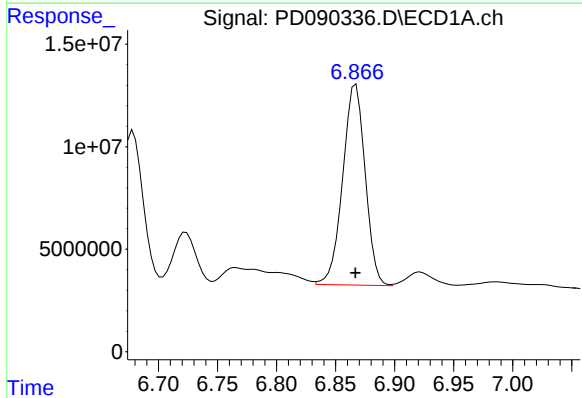


#27 Chlordane-5

R.T.: 6.867 min
Delta R.T.: 0.000 min
Response: 129652093
Conc: 742.14 ng/ml

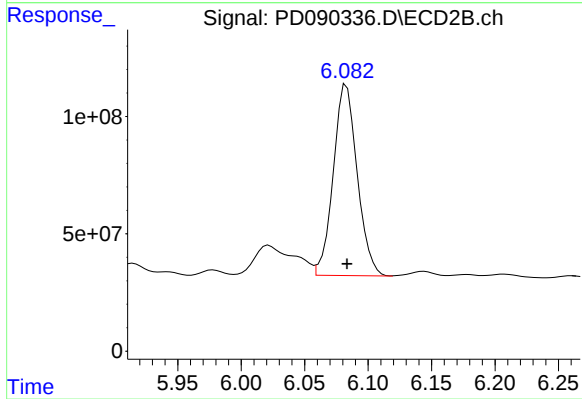

#27 Chlordane-5


R.T.: 6.083 min
Delta R.T.: 0.000 min
Response: 1067832955
Conc: 715.43 ng/ml

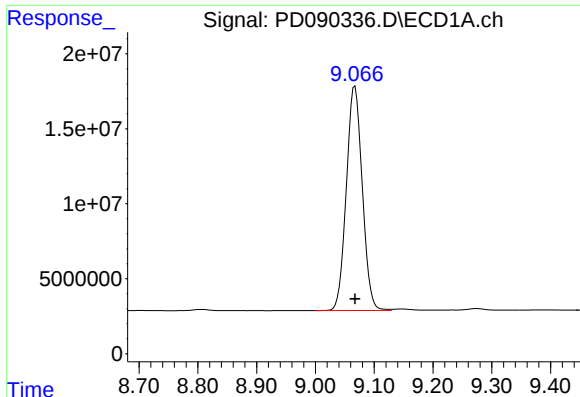

#28 Decachlorobiphenyl

R.T.: 9.067 min
Delta R.T.: 0.000 min
Response: 281781663
Conc: 71.11 ng/ml

Instrument :
ECD_D
ClientSampleId :

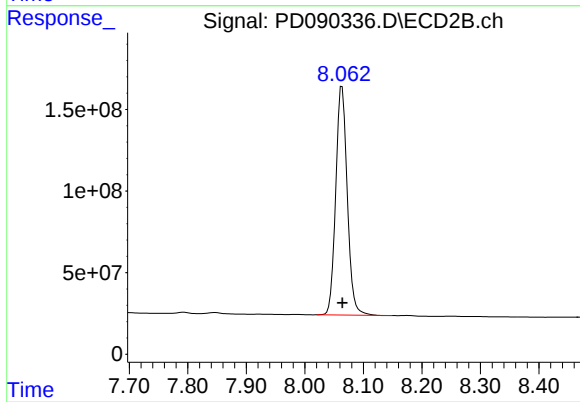

#28 Decachlorobiphenyl

R.T.: 8.064 min
Delta R.T.: 0.000 min
Response: 1917390153
Conc: 71.36 ng/ml