

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091825\
 Data File : PD090338.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 18 Sep 2025 12:18
 Operator : AR\AJ
 Sample : PCHLORICC250
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PCHLORICC250

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 19 05:32:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091825.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 19 05:30:47 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.876	67997012	730.0E6	25.848	25.647
28)	SA Decachlor...	9.067	8.064	105.1E6	698.0E6	26.518	25.978
Target Compounds							
23)	Chlordane-1	4.710	3.900	51385123	305.8E6	251.066	260.949
24)	Chlordane-2	5.236	4.481	54197903	319.7E6	263.983	263.993
25)	Chlordane-3	5.942	5.119	201.6E6	955.9E6	244.394	260.996
26)	Chlordane-4	6.027	5.183	248.2E6	822.4E6	248.801	262.095
27)	Chlordane-5	6.866	6.083	43845948	387.2E6	250.978	259.385



(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091825\
Data File : PD090338.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 18 Sep 2025 12:18
Operator : AR\AJ
Sample : PCHLORICC250
Misc :
ALS Vial : 13 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 19 05:32:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091825.M
Quant Title : GC Extractables
QLast Update : Fri Sep 19 05:30:47 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

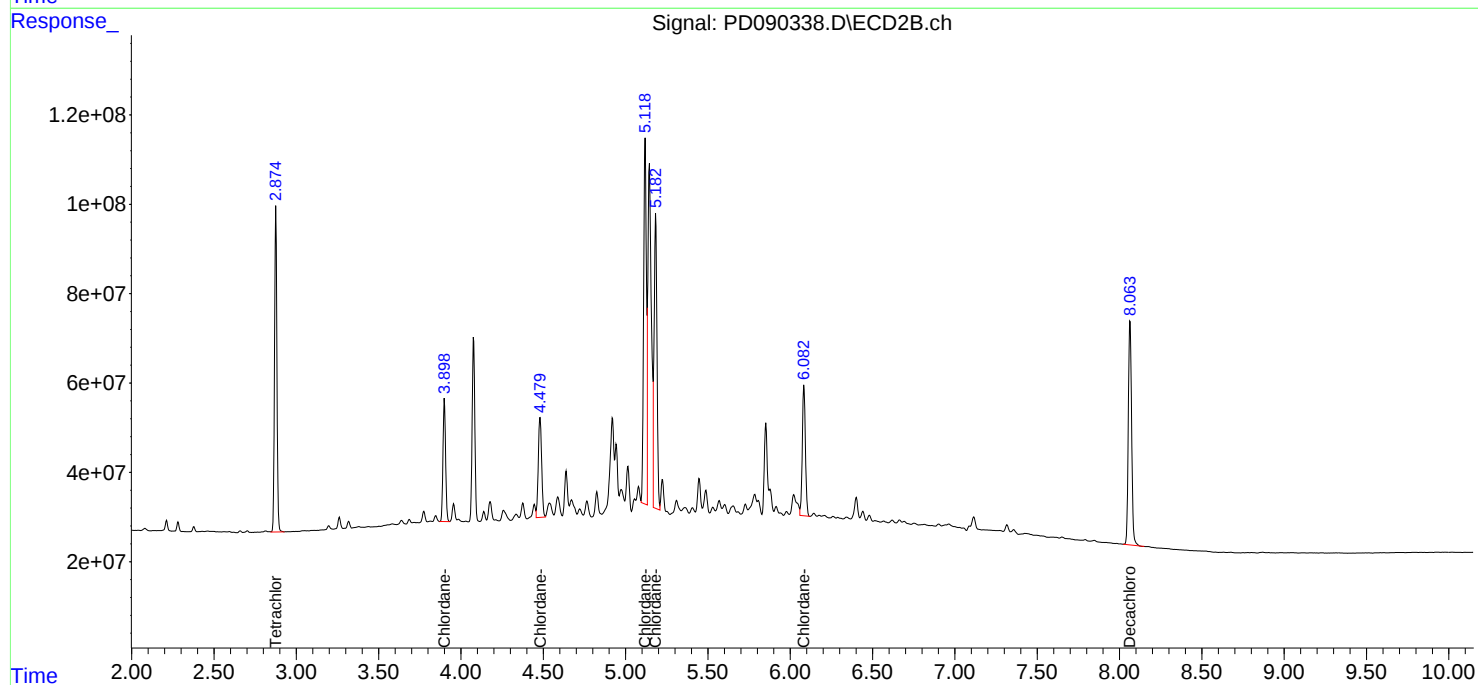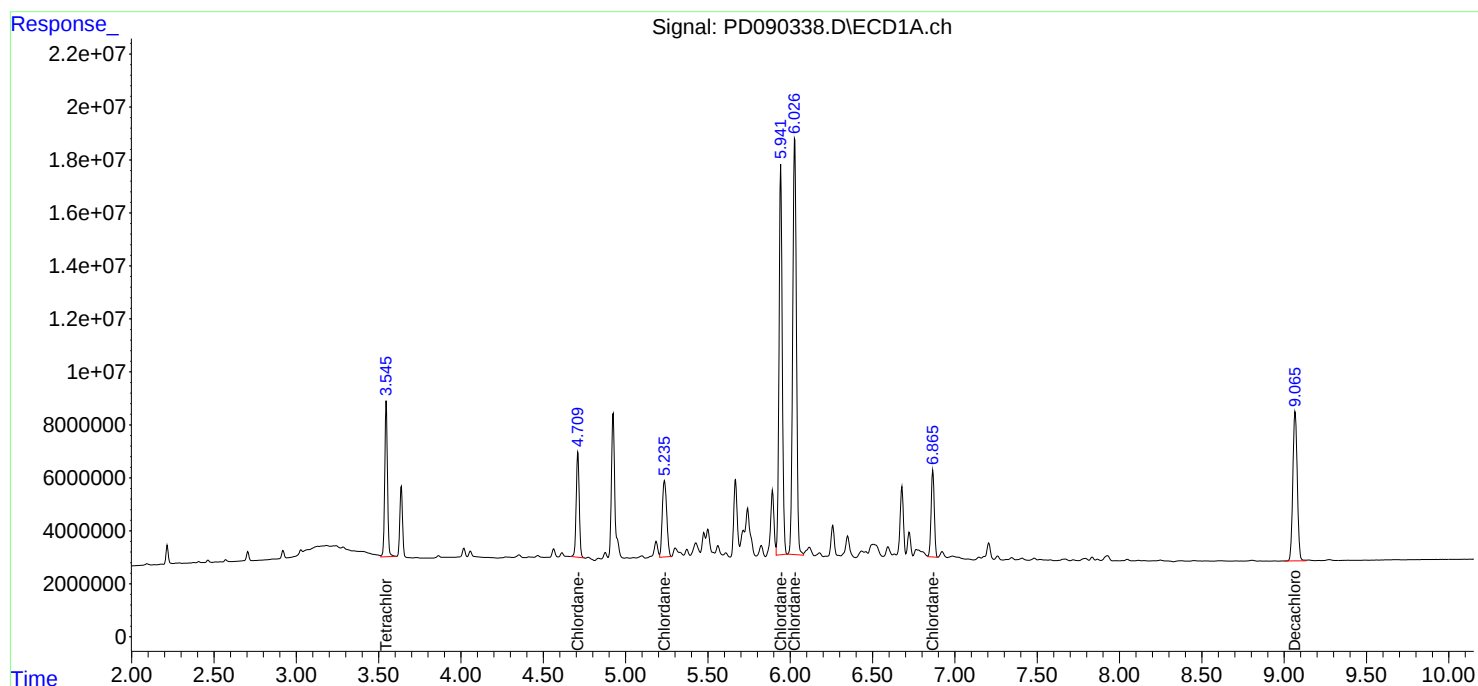


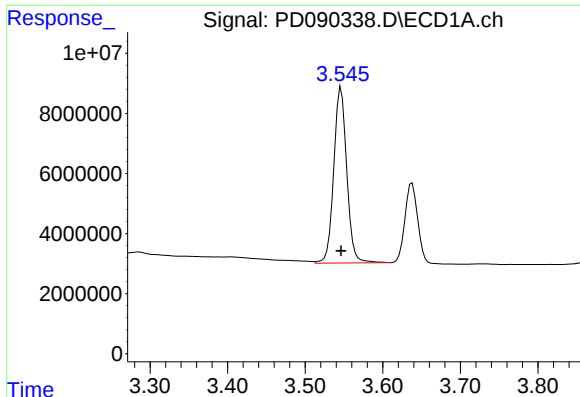

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 67997012
Conc: 25.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

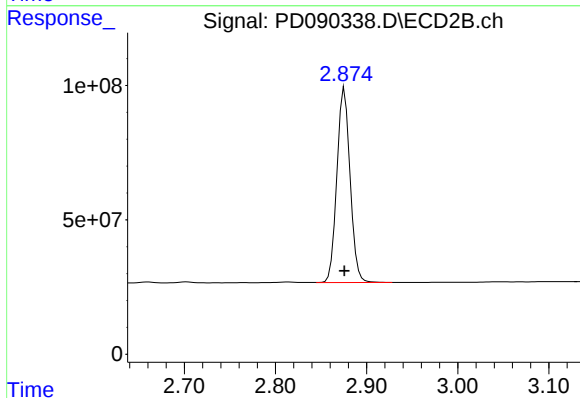


#1 Tetrachloro-m-xylene

R.T.: 2.876 min
Delta R.T.: 0.000 min
Response: 729985984
Conc: 25.65 ng/ml

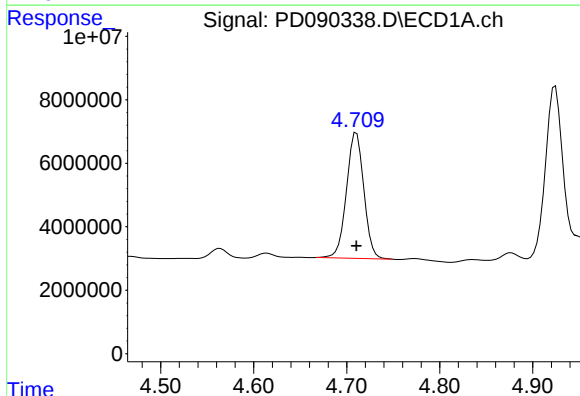


#23 Chlordane-1

R.T.: 4.710 min
Delta R.T.: 0.000 min
Response: 51385123
Conc: 251.07 ng/ml

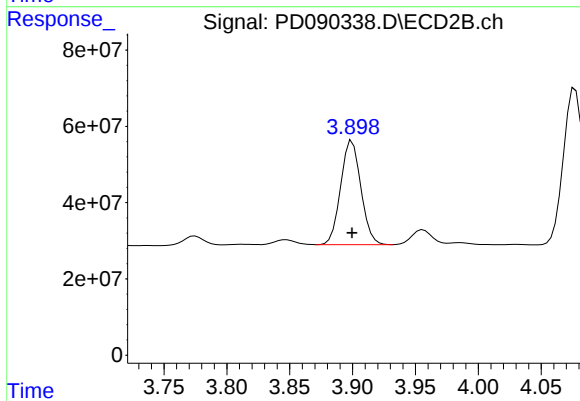

#23 Chlordane-1


R.T.: 3.900 min
Delta R.T.: 0.000 min
Response: 305800648
Conc: 260.95 ng/ml

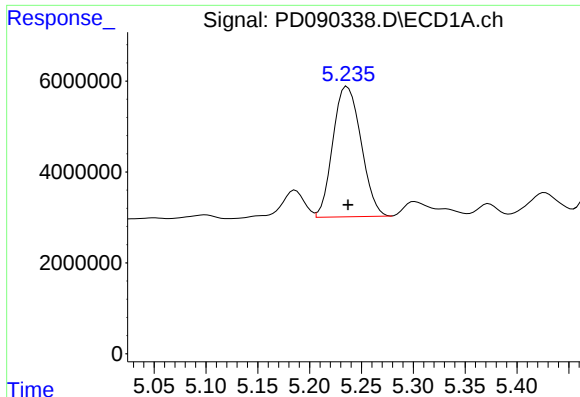

#24 Chlordane-2


R.T.: 5.236 min
Delta R.T.: 0.000 min
Response: 54197903
Conc: 263.98 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

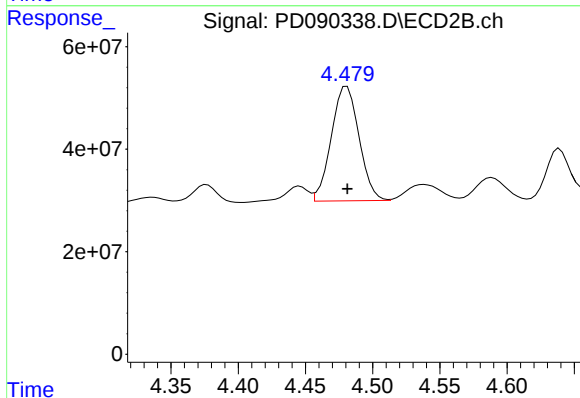


#24 Chlordane-2

R.T.: 4.481 min
Delta R.T.: 0.000 min
Response: 319739454
Conc: 263.99 ng/ml

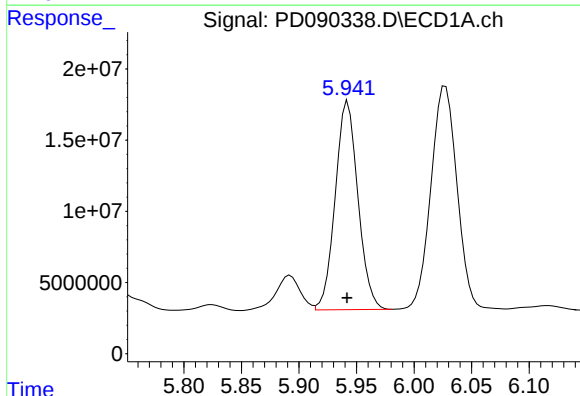


#25 Chlordane-3

R.T.: 5.942 min
Delta R.T.: 0.000 min
Response: 201613624
Conc: 244.39 ng/ml

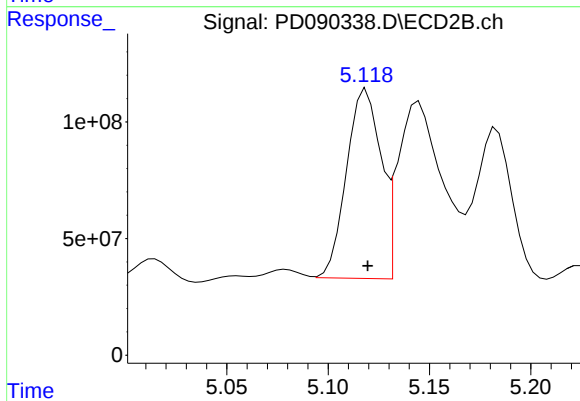

#25 Chlordane-3


R.T.: 5.119 min
Delta R.T.: 0.000 min
Response: 955911110
Conc: 261.00 ng/ml

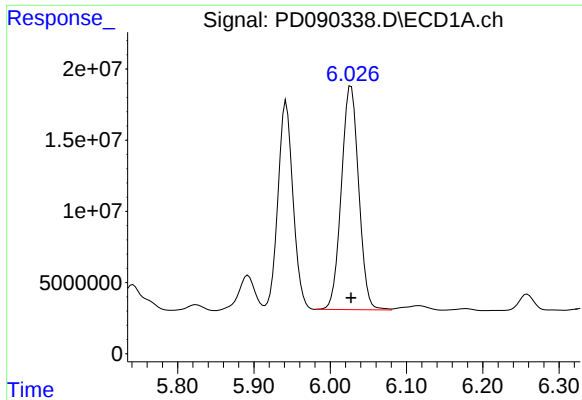

#26 Chlordane-4


R.T.: 6.027 min
Delta R.T.: 0.000 min
Response: 248155739
Conc: 248.80 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

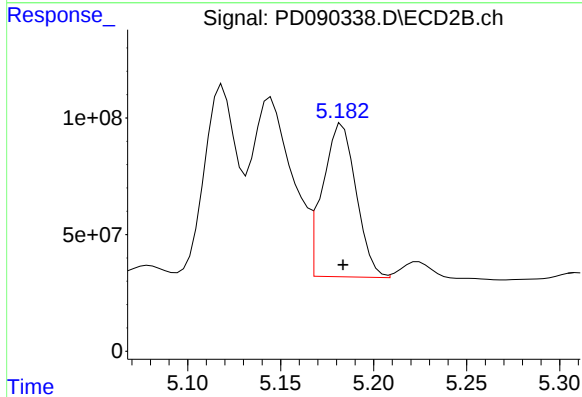


#26 Chlordane-4

R.T.: 5.183 min
Delta R.T.: 0.000 min
Response: 822404729
Conc: 262.10 ng/ml

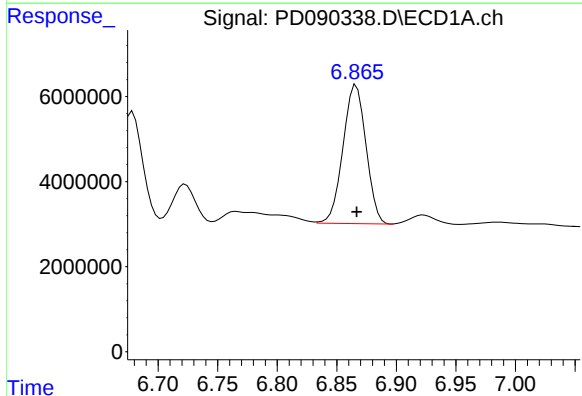


#27 Chlordane-5

R.T.: 6.866 min
Delta R.T.: 0.000 min
Response: 43845948
Conc: 250.98 ng/ml

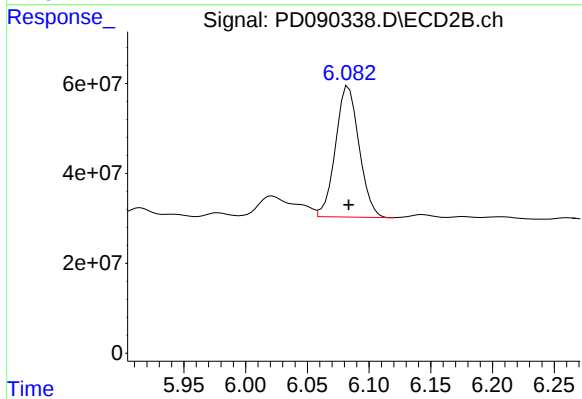

#27 Chlordane-5


R.T.: 6.083 min
Delta R.T.: 0.000 min
Response: 387150624
Conc: 259.38 ng/ml

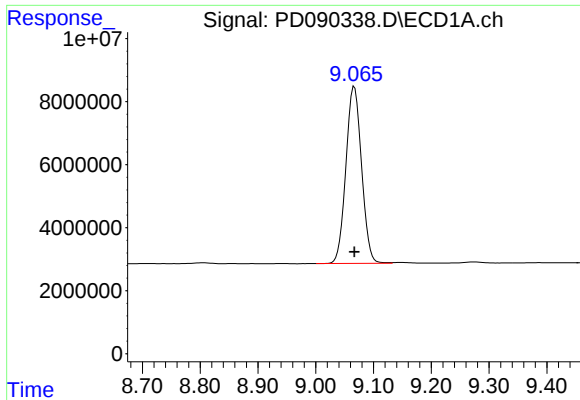

#28 Decachlorobiphenyl

R.T.: 9.067 min
Delta R.T.: 0.000 min
Response: 105074820
Conc: 26.52 ng/ml

Instrument :
ECD_D
ClientSampleId :
PCHLORICC250

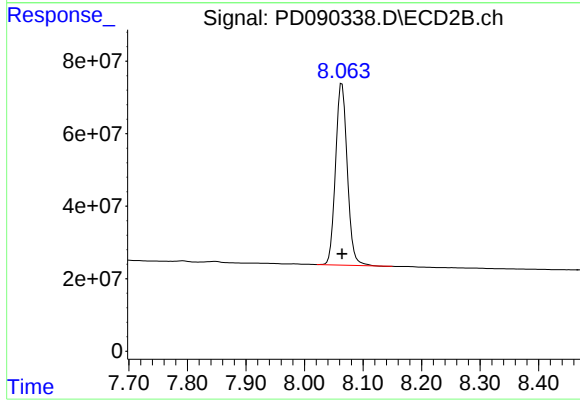

#28 Decachlorobiphenyl

R.T.: 8.064 min
Delta R.T.: 0.000 min
Response: 698002727
Conc: 25.98 ng/ml