

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091919\
 Data File : PD054754.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Sep 2019 14:03
 Operator : SG\AJ
 Sample : K4890-05
 Misc :
 ALS Vial : 15 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AS0

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 01:14:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091819CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 18 17:43:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds							
1)	SA Tetrachlo...	3.294	3.965	7331512	8861574	10.854	10.863
27)	SA Decachlor...	7.973	9.001	20983175	22827083	23.810	22.199
Target Compounds							
3)	MA gamma-BHC...	4.006	0.000	3161121	0	3.309	N.D. #
20)	A Methoxychlor	6.734	0.000	2064268	0	5.495	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091919\
Data File : PD054754.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Sep 2019 14:03
Operator : SG\AJ
Sample : K4890-05
Misc :
ALS Vial : 15 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0AS0

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 01:14:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091819CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 18 17:43:20 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

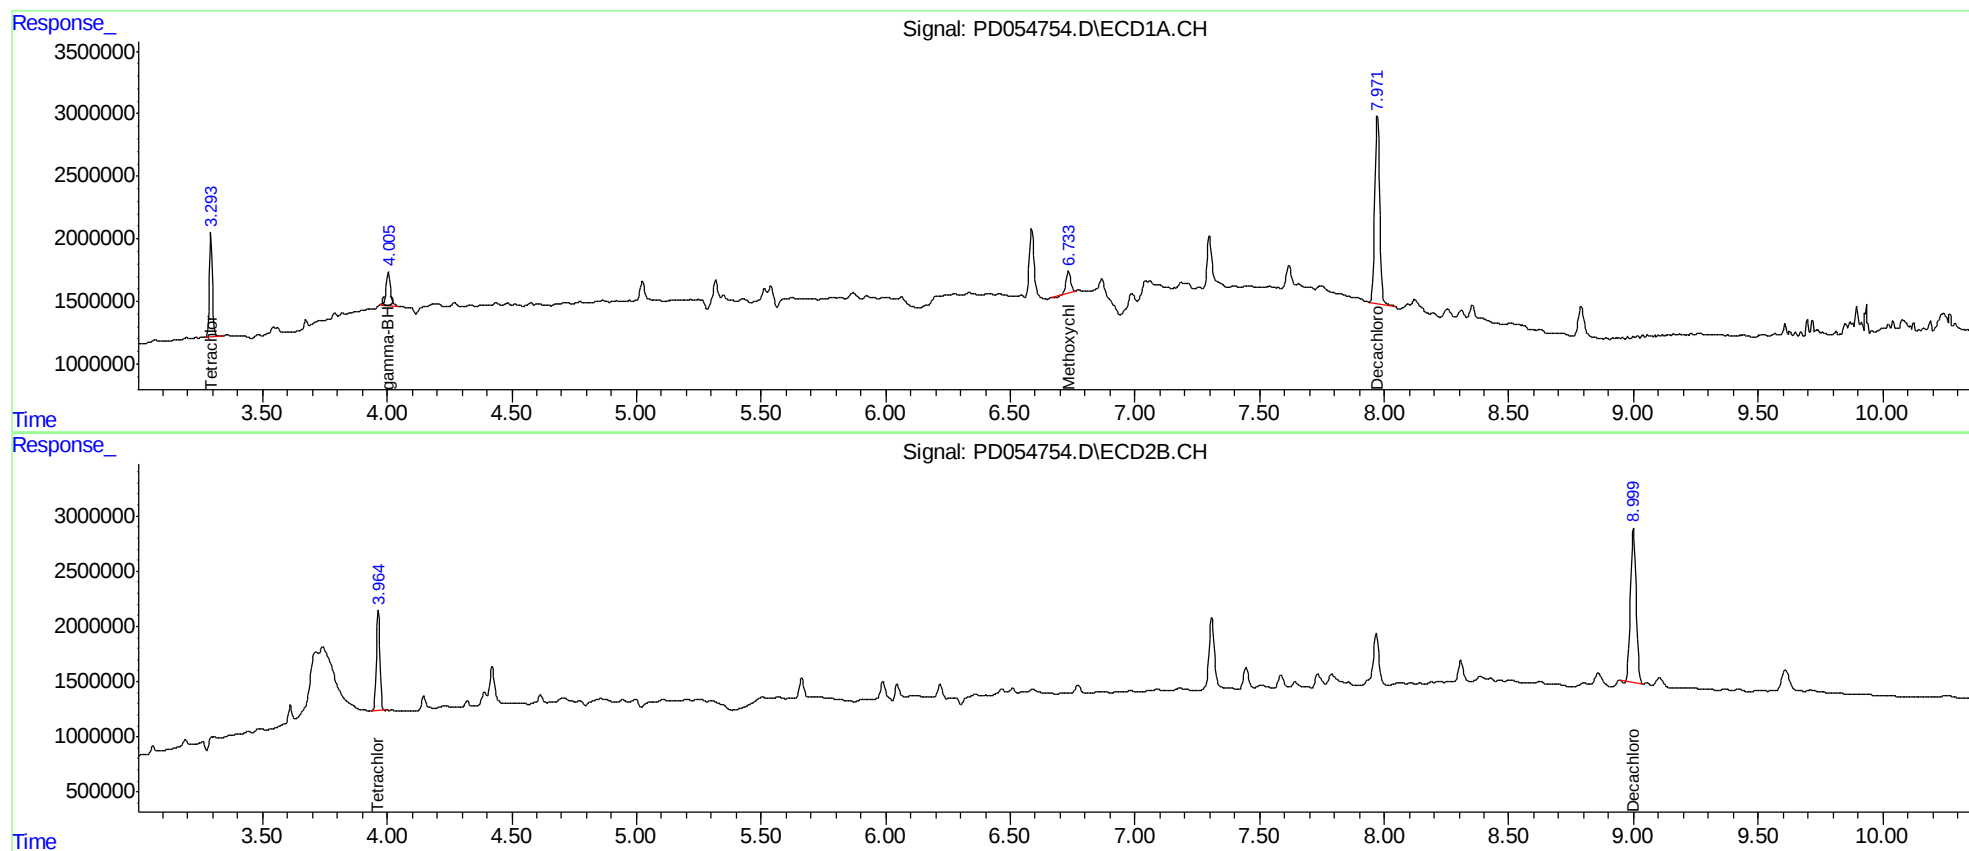


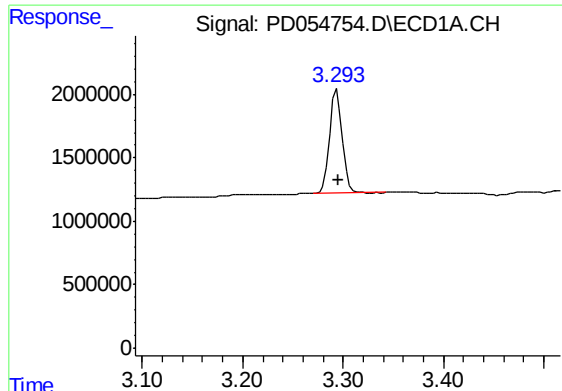

#1 Tetrachloro-m-xylene


R.T.: 3.294 min
Delta R.T.: 0.000 min
Response: 7331512
Conc: 10.85 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AS0

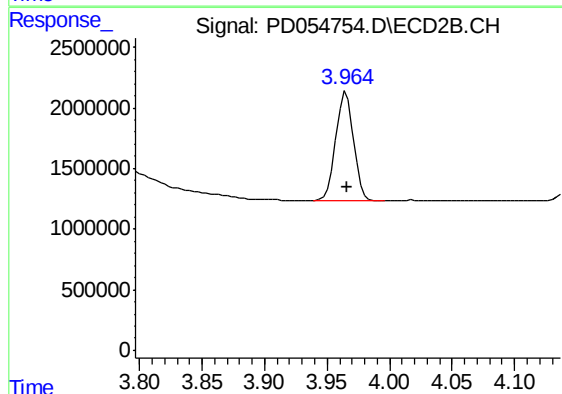


#1 Tetrachloro-m-xylene

R.T.: 3.965 min
Delta R.T.: 0.000 min
Response: 8861574
Conc: 10.86 ng/ml

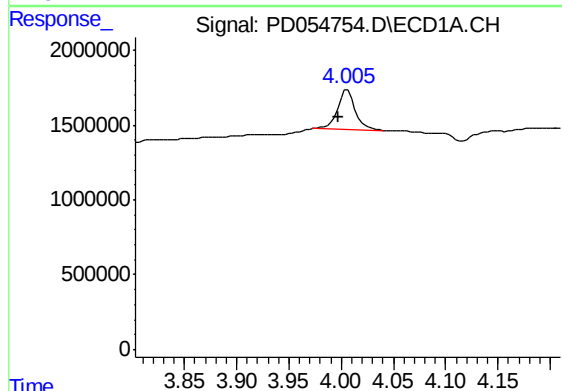


#3 gamma-BHC (Lindane)

R.T.: 4.006 min
Delta R.T.: 0.009 min
Response: 3161121
Conc: 3.31 ng/ml

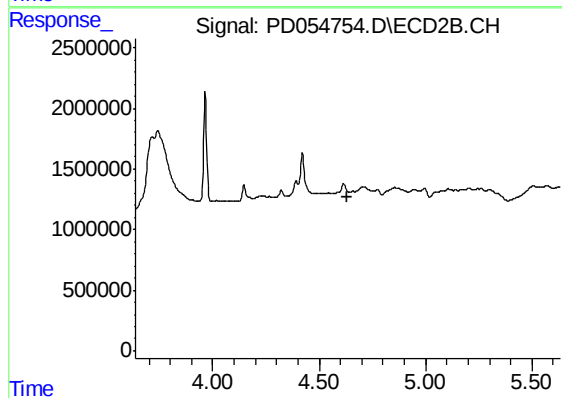

#3 gamma-BHC (Lindane)


R.T.: 0.000 min
Exp R.T. : 4.635 min
Response: 0
Conc: N.D.

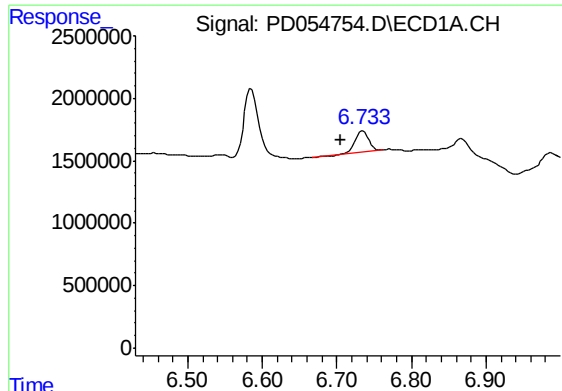

#20 Methoxychlor


R.T.: 6.734 min
Delta R.T.: 0.030 min
Response: 2064268
Conc: 5.50 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AS0

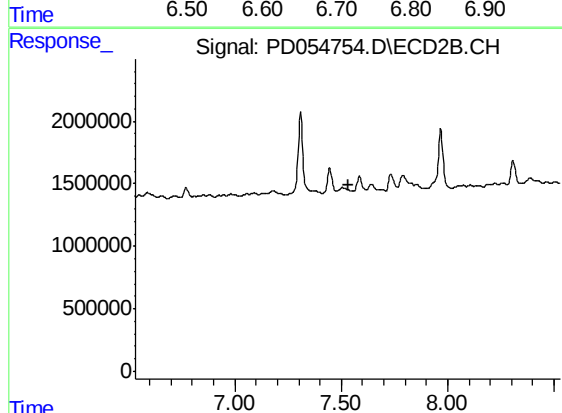


#20 Methoxychlor

R.T.: 0.000 min
Exp R.T. : 7.532 min
Response: 0
Conc: N.D.

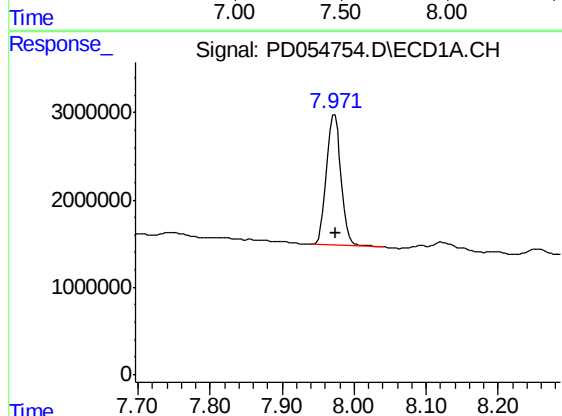

#27 Decachlorobiphenyl

R.T.: 7.973 min
Delta R.T.: -0.002 min
Response: 20983175
Conc: 23.81 ng/ml

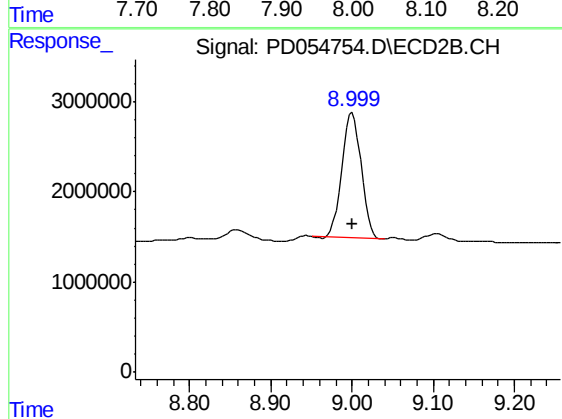

#27 Decachlorobiphenyl

R.T.: 9.001 min
Delta R.T.: 0.000 min
Response: 22827083
Conc: 22.20 ng/ml