

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091919\
 Data File : PD054769.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Sep 2019 17:38
 Operator : SG\AJ
 Sample : K4890-13
 Misc :
 ALS Vial : 29 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AS6

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 01:18:21 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091819CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 18 17:43:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	3.294	3.965	5880624	7267414	8.706	8.909
27) SA Decachlor...	7.973	9.000	18859672	20052036	21.400	19.501
Target Compounds						
21) B Endrin ke...	0.000	7.679	0	17539358	N.D.	15.647


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091919\
Data File : PD054769.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Sep 2019 17:38
Operator : SG\AJ
Sample : K4890-13
Misc :
ALS Vial : 29 Sample Multiplier: 1

Instrument :
ECD_D
ClientSampleId :
C0AS6

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 01:18:21 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091819CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 18 17:43:20 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

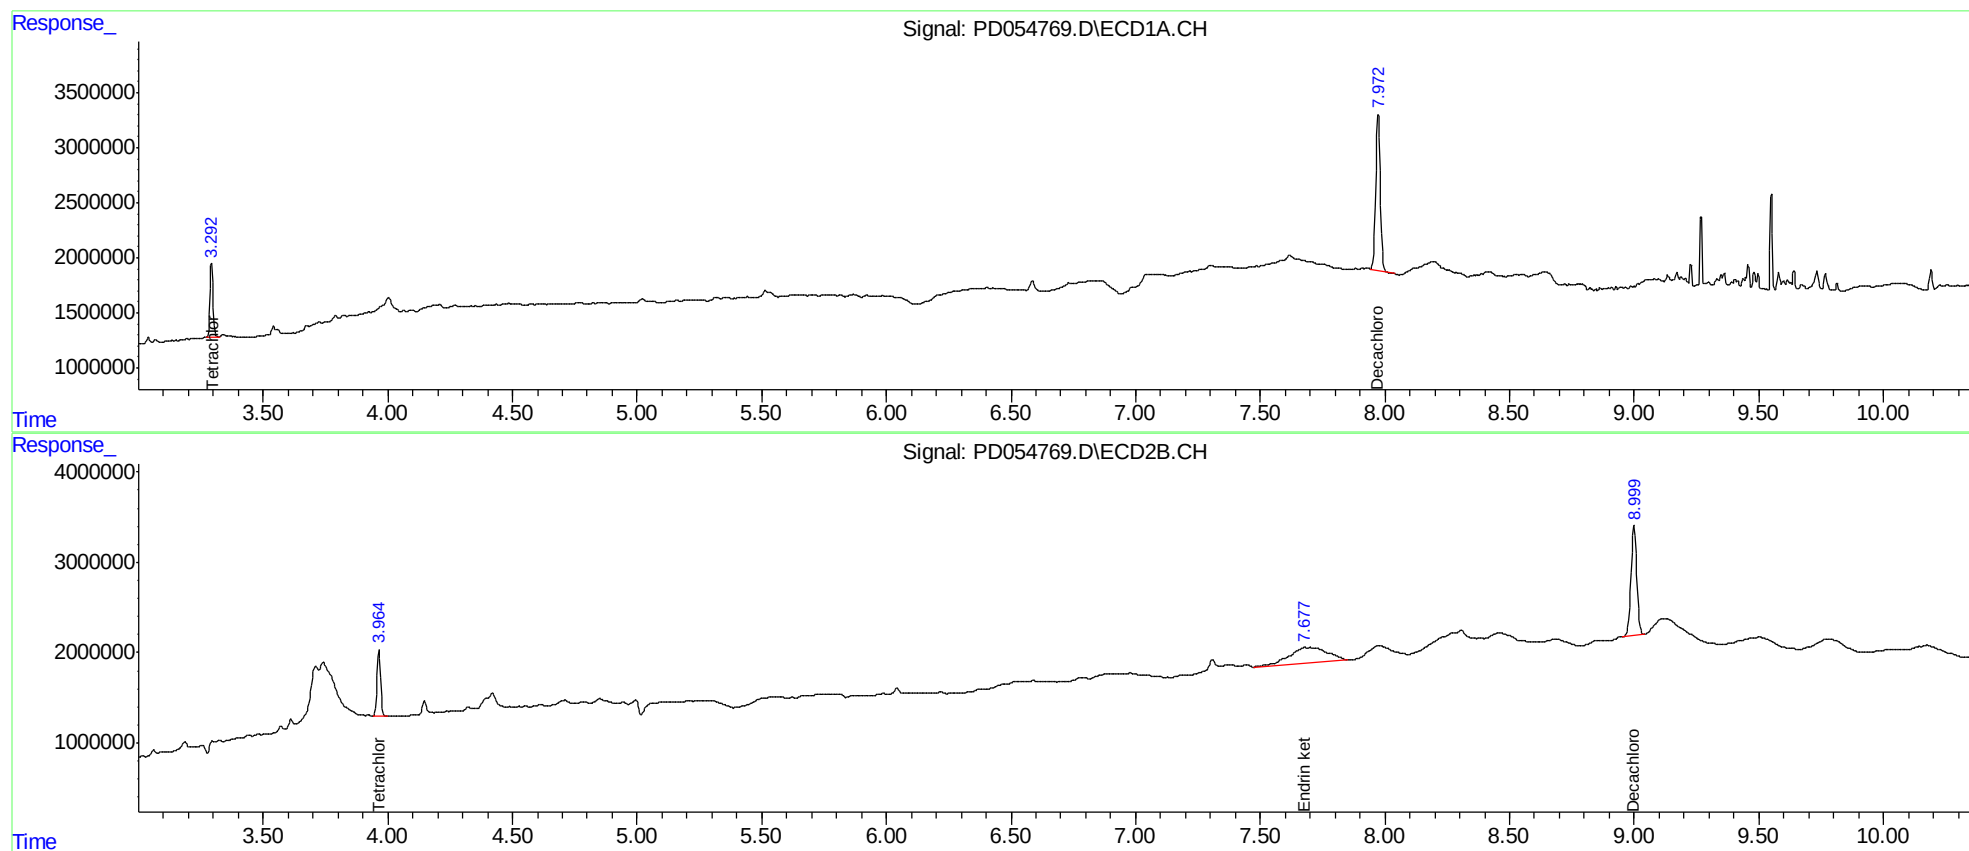


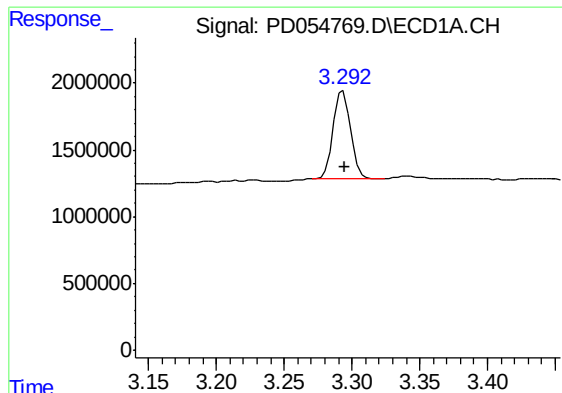

#1 Tetrachloro-m-xylene


R.T.: 3.294 min
Delta R.T.: -0.001 min
Response: 5880624
Conc: 8.71 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AS6

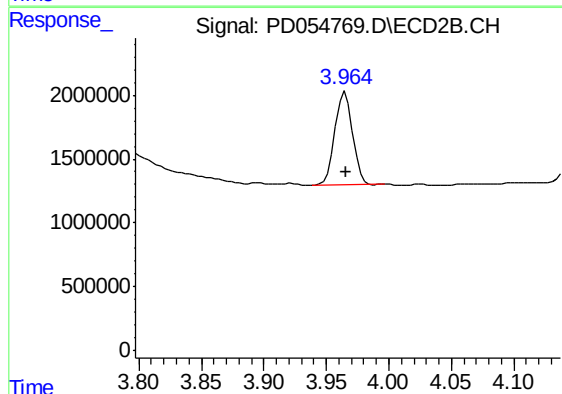


#1 Tetrachloro-m-xylene

R.T.: 3.965 min
Delta R.T.: 0.000 min
Response: 7267414
Conc: 8.91 ng/ml

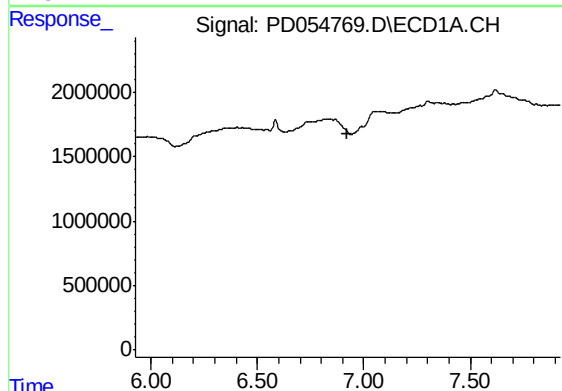


#21 Endrin ketone

R.T.: 0.000 min
Exp R.T. : 6.924 min
Response: 0
Conc: N.D.

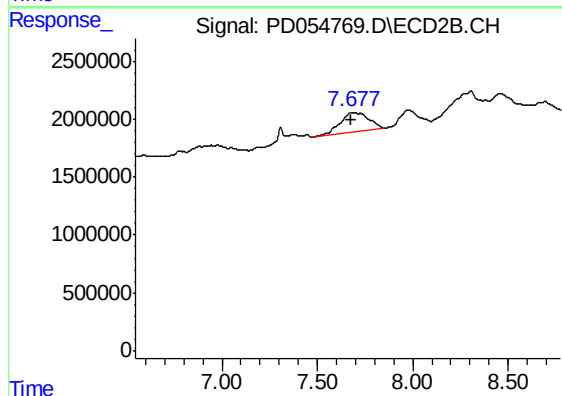

#21 Endrin ketone


R.T.: 7.679 min
Delta R.T.: 0.003 min
Response: 17539358
Conc: 15.65 ng/ml

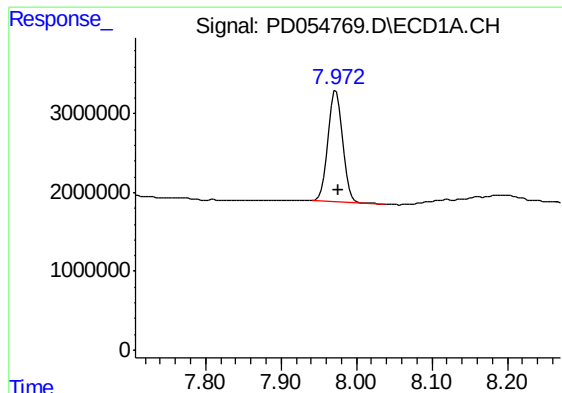

#27 Decachlorobiphenyl

R.T.: 7.973 min
Delta R.T.: -0.002 min
Response: 18859672
Conc: 21.40 ng/ml

Instrument :
ECD_D
ClientSampleId :
C0AS6

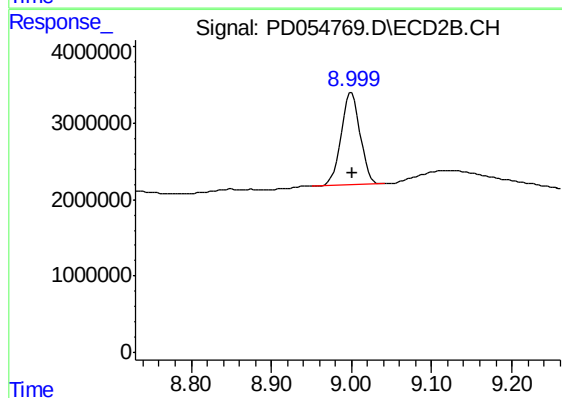

#27 Decachlorobiphenyl

R.T.: 9.000 min
Delta R.T.: 0.000 min
Response: 20052036
Conc: 19.50 ng/ml