

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091919\
 Data File : PD054765.D
 Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
 Acq On : 19 Sep 2019 16:42
 Operator : SG\AJ
 Sample : K4890-16
 Misc :
 ALS Vial : 25 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 C0AT0

Manual Integrations
 APPROVED

Ankita
 9/20/2019 4:28:22 PM

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 01:17:15 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091819CLP.M
 Quant Title : GC Extractables
 QLast Update : Wed Sep 18 17:43:20 2019
 Response via : Initial Calibration
 Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.294	3.965	13801400	15979509	20.432	19.589
27) SA Decachlor...	7.975	8.998	23214480	32347577	26.342	31.458m
Target Compounds						
15) B Endosulfa...	6.064	6.853	1875152	2329808	2.185m	2.288m
16) A 4,4'-DDD	5.921	6.772	2128454	4690686	2.748m	4.941 #

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091919\
Data File : PD054765.D
Signal(s) : Signal #1: ECD1A.CH Signal #2: ECD2B.CH
Acq On : 19 Sep 2019 16:42
Operator : SG\AJ
Sample : K4890-16
Misc :
ALS Vial : 25 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 01:17:15 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091819CLP.M
Quant Title : GC Extractables
QLast Update : Wed Sep 18 17:43:20 2019
Response via : Initial Calibration
Integrator: ChemStation 6890 Scale Mode: Large solvent peaks clipped

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

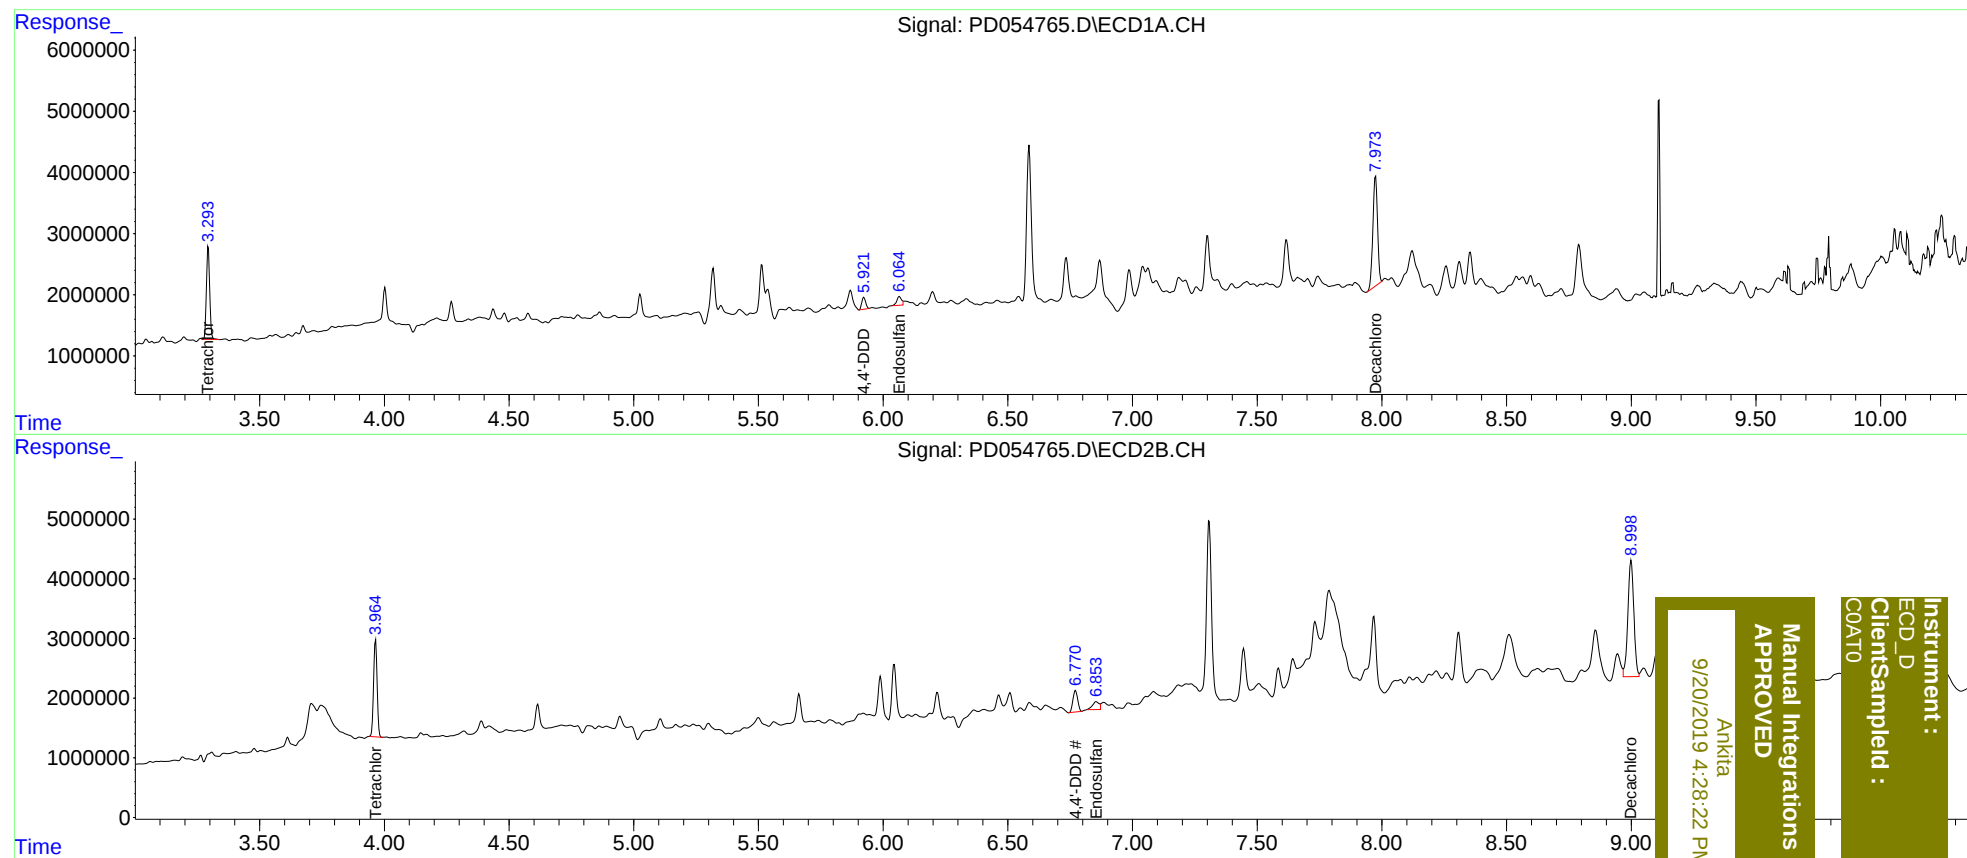

9/20/2019 4:28:22 PM
Ankita

Manual Integrations
APPROVED

Instrument :
ECD_D
ClientSampled :
COATO