

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091922\
 Data File : PD071937.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2022 18:37
 Operator : AR\AJ
 Sample : N4648-01
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 N48854-1040

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/19/2022
 Supervised By : Ankita Jodhani 09/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 01:07:21 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091022.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 10 22:11:50 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	2.804	3.561	20346550	249.3E6	8.321m	8.689m
28) SA Decachlor...	7.992	9.086	13955366	79907588	5.539	8.595 #

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091922\
Data File : PD071937.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2022 18:37
Operator : AR\AJ
Sample : N4648-01
Misc :
ALS Vial : 11 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
N48854-1040


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/19/2022
Supervised By : Ankita Jodhani 09/19/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 01:07:21 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091022.M
Quant Title : GC Extractables
QLast Update : Sat Sep 10 22:11:50 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

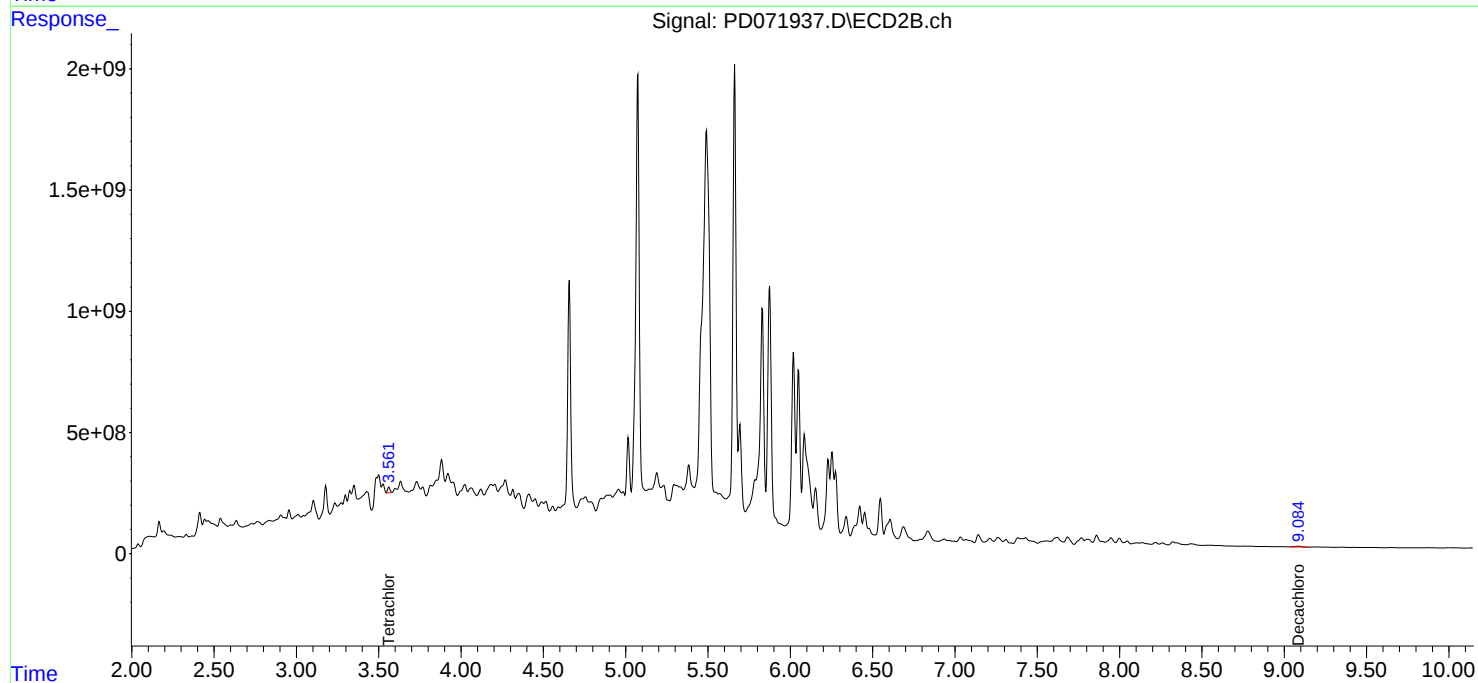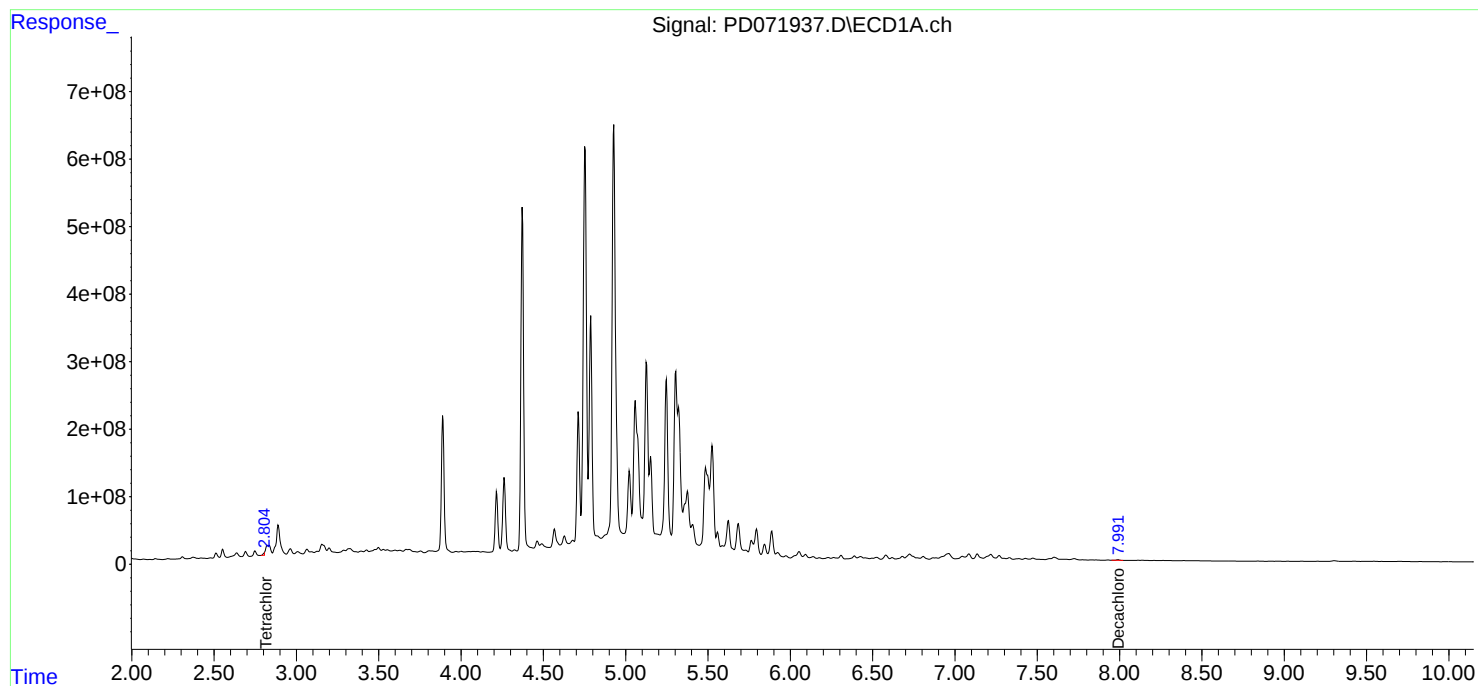

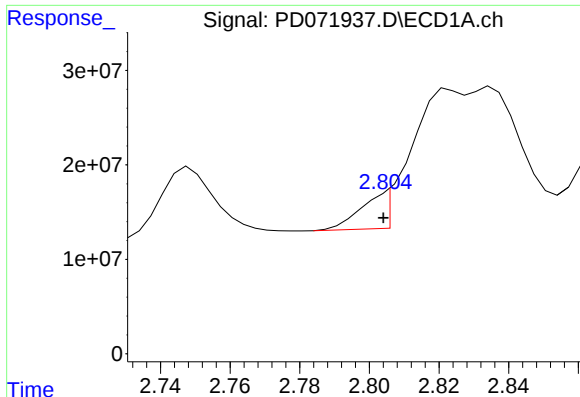

#1 Tetrachloro-m-xylene

R.T.: 2.804 min
Delta R.T.: 0.000 min
Response: 20346550
Conc: 8.32 ng/ml

Instrument :

ECD_D

ClientSampleId :


N48854-1040

Manual Integrations

APPROVED


Reviewed By :Abdul Mirza 09/19/2022

Supervised By :Ankita Jodhani 09/19/2022

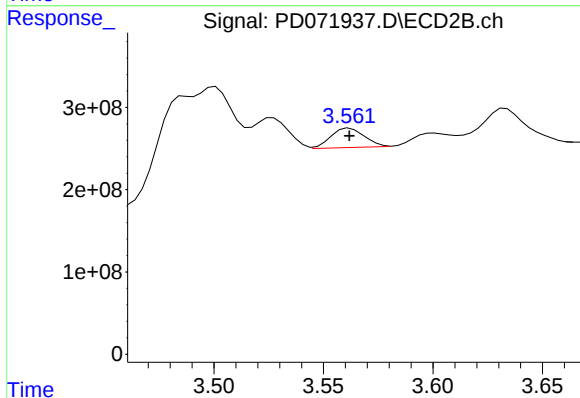


#1 Tetrachloro-m-xylene

R.T.: 3.561 min
Delta R.T.: -0.001 min
Response: 249327473
Conc: 8.69 ng/ml m

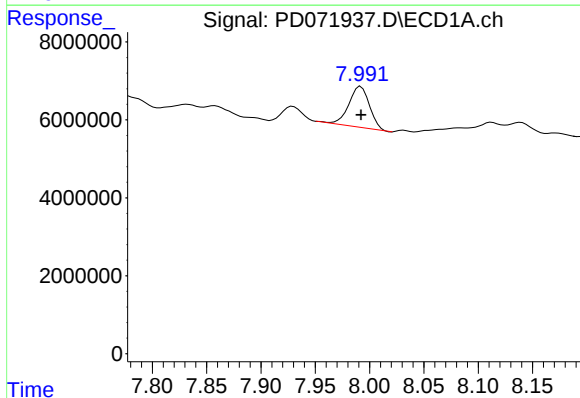

#28 Decachlorobiphenyl

R.T.: 7.992 min
Delta R.T.: 0.000 min
Response: 13955366
Conc: 5.54 ng/ml

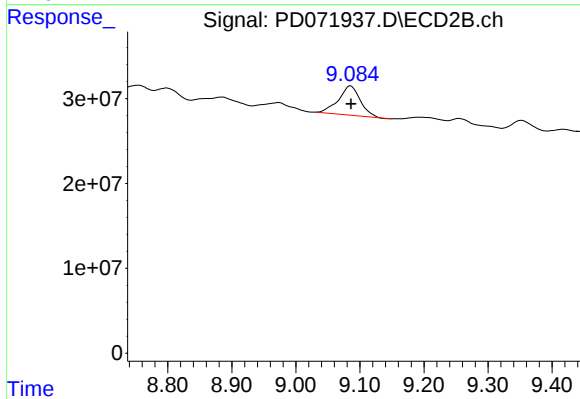

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: 0.000 min
Response: 79907588
Conc: 8.59 ng/ml