

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091922\
 Data File : PD071938.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 16 Sep 2022 18:50
 Operator : AR\AJ
 Sample : N4663-01
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 HW-43

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/19/2022
 Supervised By : Ankita Jodhani 09/19/2022

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 17 01:07:42 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091022.M
 Quant Title : GC Extractables
 QLast Update : Sat Sep 10 22:11:50 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 2 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
 Signal #1 Info : 30M x 0.32mm x 0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml

System Monitoring Compounds						
1) SA Tetrachlo...	2.803	3.560	35082925	353.9E6	14.347	12.331m
2) SA Decachlor...	7.990	9.086	23048656	105.5E6	9.149m	11.348

Target Compounds

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091922\
Data File : PD071938.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 16 Sep 2022 18:50
Operator : AR\AJ
Sample : N4663-01
Misc :
ALS Vial : 12 Sample Multiplier: 1



Instrument :
ECD_D
ClientSampleId :
HW-43


Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/19/2022
Supervised By : Ankita Jodhani 09/19/2022

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 17 01:07:42 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091022.M
Quant Title : GC Extractables
QLast Update : Sat Sep 10 22:11:50 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 2 µl
Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR1
Signal #1 Info : 30M x 0.32mm x0.2 Signal #2 Info : 30M x 0.32mm x 0.50µm

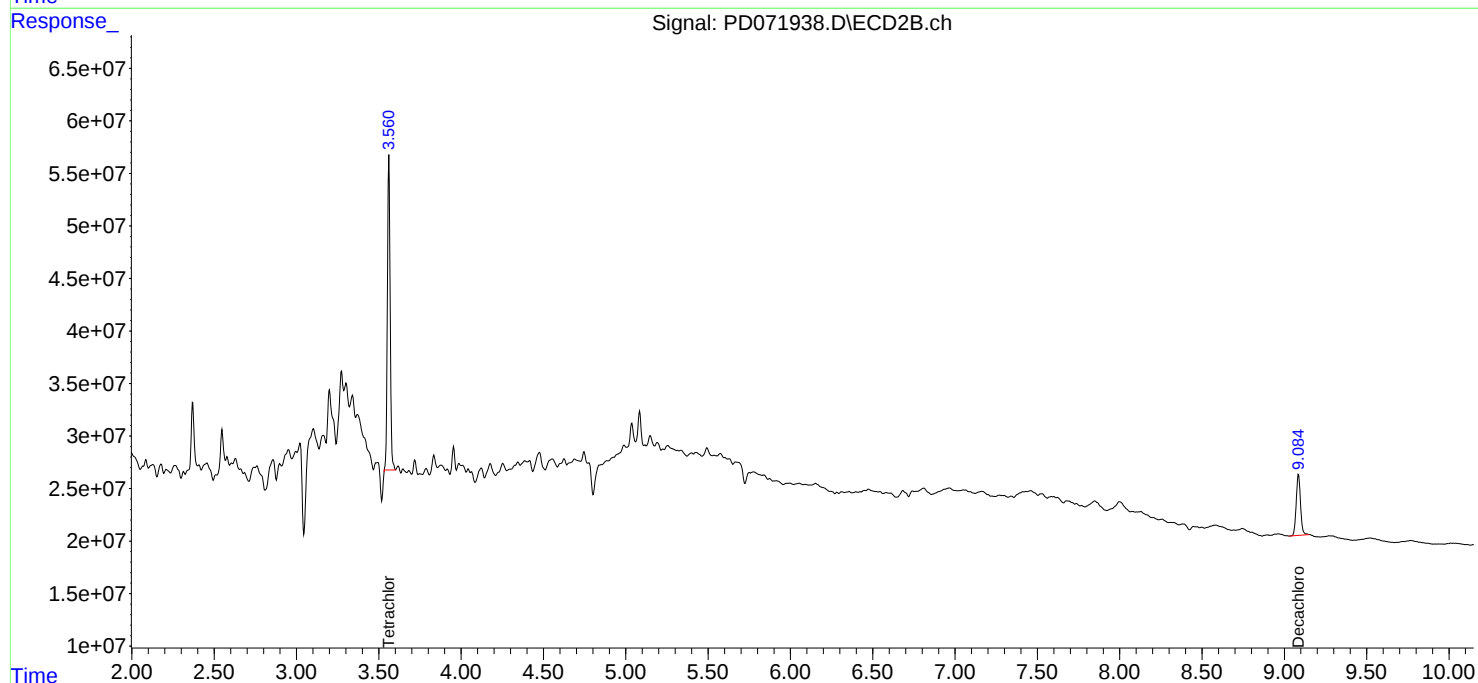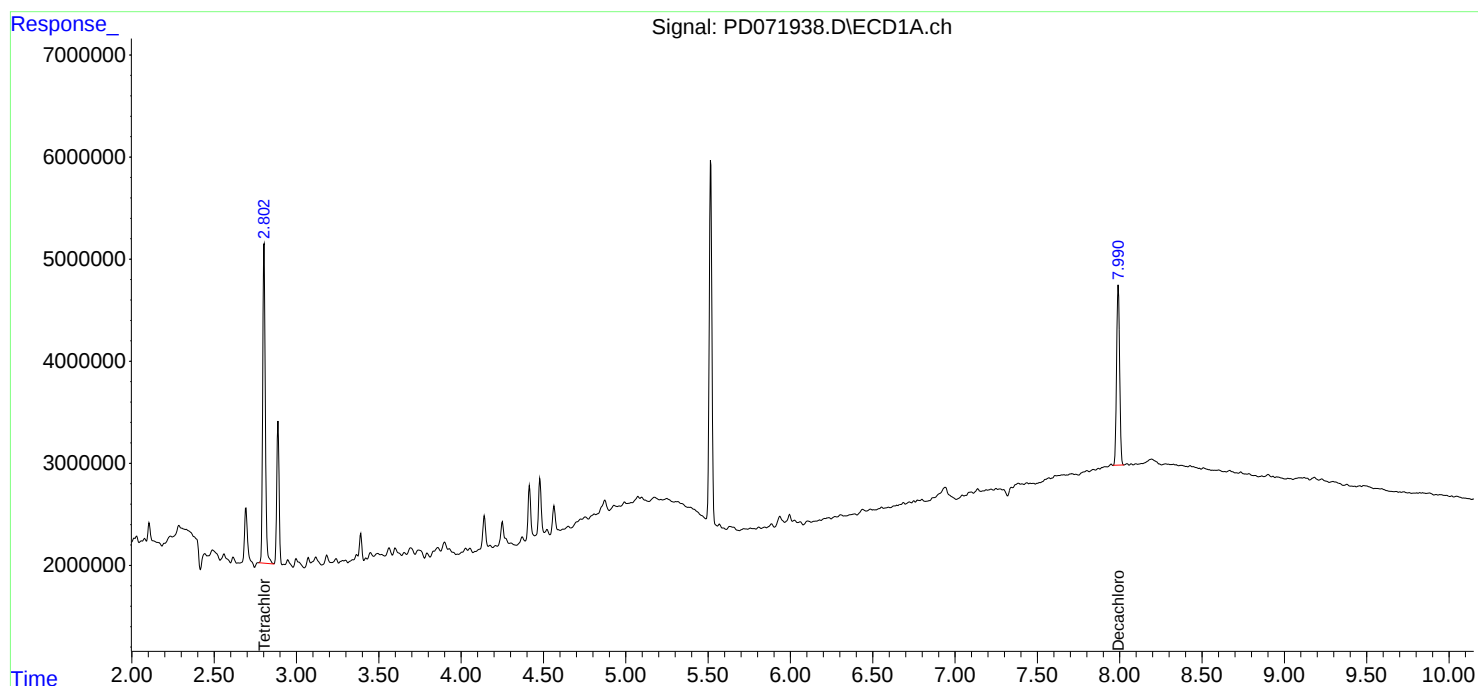

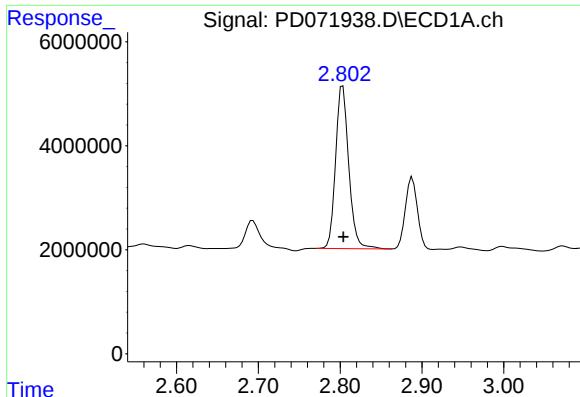


#1 Tetrachloro-m-xylene

R.T.: 2.803 min
Delta R.T.: 0.000 min
Response: 35082925
Conc: 14.35 ng/ml

Instrument :
ECD_D
ClientSampleId :
HW-43


Manual Integrations
APPROVED

Reviewed By :Abdul Mirza 09/19/2022
Supervised By :Ankita Jodhani 09/19/2022

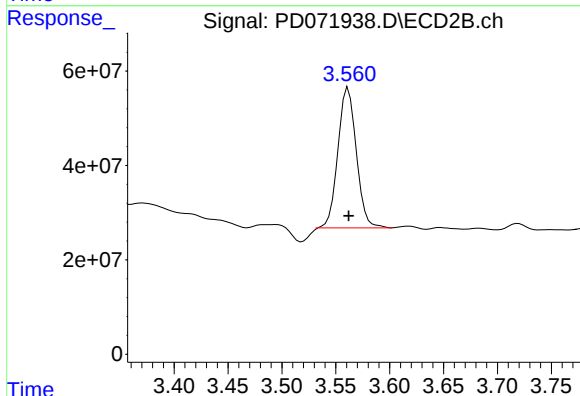


#1 Tetrachloro-m-xylene

R.T.: 3.560 min
Delta R.T.: -0.002 min
Response: 353857331
Conc: 12.33 ng/ml m

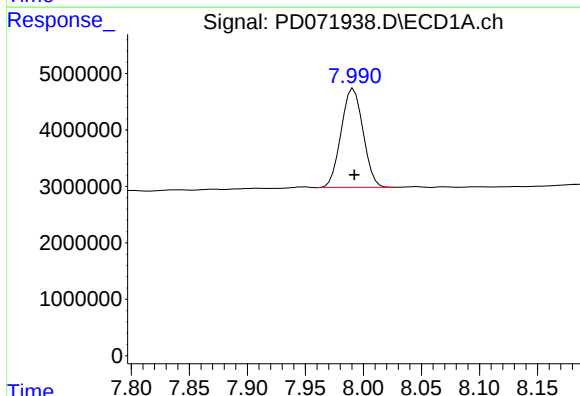

#28 Decachlorobiphenyl

R.T.: 7.990 min
Delta R.T.: -0.002 min
Response: 23048656
Conc: 9.15 ng/ml m

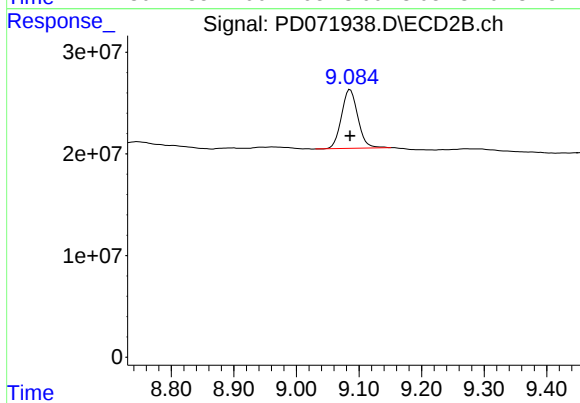

#28 Decachlorobiphenyl

R.T.: 9.086 min
Delta R.T.: 0.000 min
Response: 105500300
Conc: 11.35 ng/ml