

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091924\
 Data File : PD085386.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2024 22:53
 Operator : AR\AJ
 Sample : INDA201
 Misc :
 ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 04:50:42 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 04:48:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.490	2.894	11797063	37974404	9.838	10.074
27)	SA Decachlor...	8.965	8.089	33492580	53102646	20.885	20.105
Target Compounds							
2)	A alpha-BHC	3.935	3.405	21477847	54475618	9.433	9.937
3)	MA gamma-BHC...	4.262	3.740	23894875	51455819	9.994	9.951
4)	MA Heptachlor	4.857	4.092	19881954	47421675	9.677	10.105
9)	A Endosulfan I	5.998	5.258	17144142	41797481	9.883	10.129
13)	MA Dieldrin	6.270	5.525	36415179	92560946	19.287	20.156
14)	MA Endrin	6.496	5.802	30565115	83466856	19.487	20.551
16)	A 4,4'-DDD	6.629	5.943	25025922	66772357	19.352	20.060
17)	MA 4,4'-DDT	6.944	6.197	22462738	61088562	18.769	19.374
20)	A Methoxychlor	7.416	6.769	71196639	165.3E6	99.200	101.434


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091924\
Data File : PD085386.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2024 22:53
Operator : AR\AJ
Sample : INDA201
Misc :
ALS Vial : 11 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 04:50:42 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 04:48:53 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

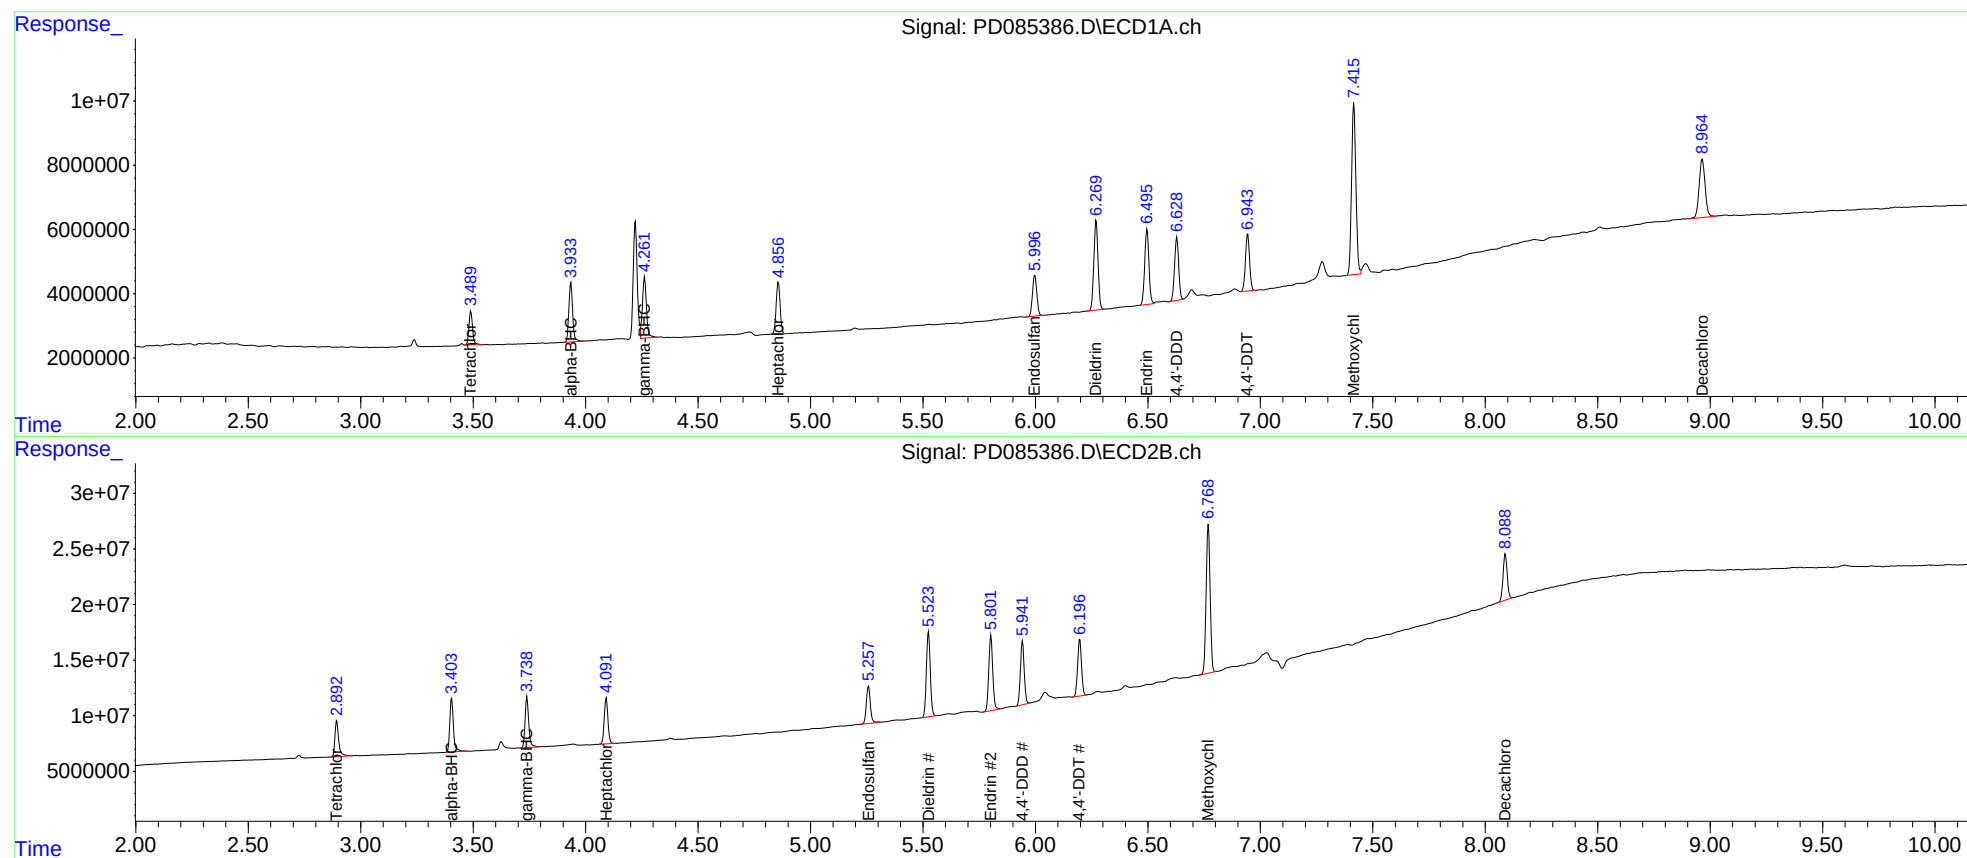

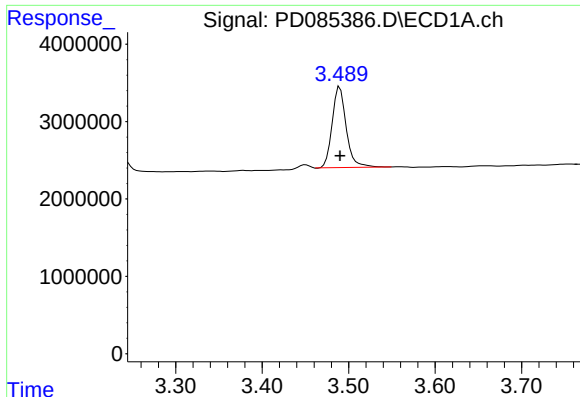


#1 Tetrachloro-m-xylene

R.T.: 3.490 min
Delta R.T.: 0.000 min
Response: 11797063
Conc: 9.84 ng/ml

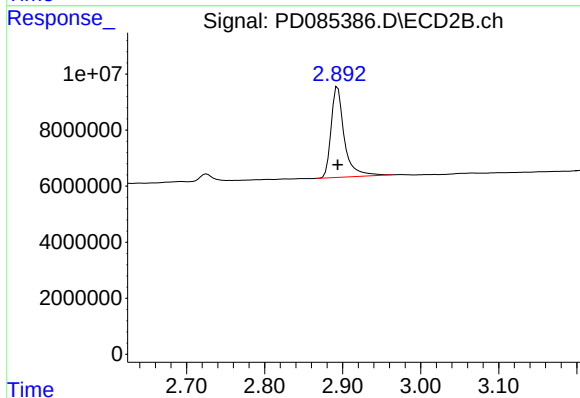


#1 Tetrachloro-m-xylene

R.T.: 2.894 min
Delta R.T.: 0.000 min
Response: 37974404
Conc: 10.07 ng/ml

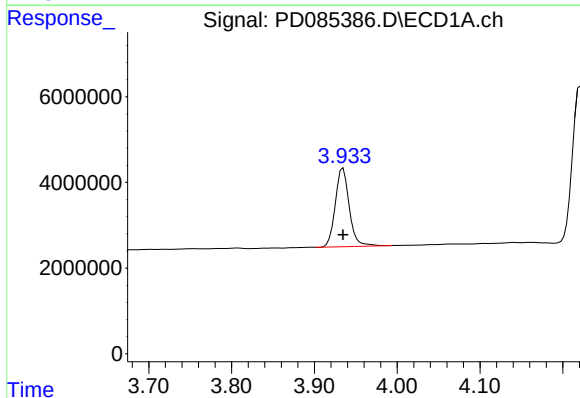


#2 alpha-BHC

R.T.: 3.935 min
Delta R.T.: 0.000 min
Response: 21477847
Conc: 9.43 ng/ml

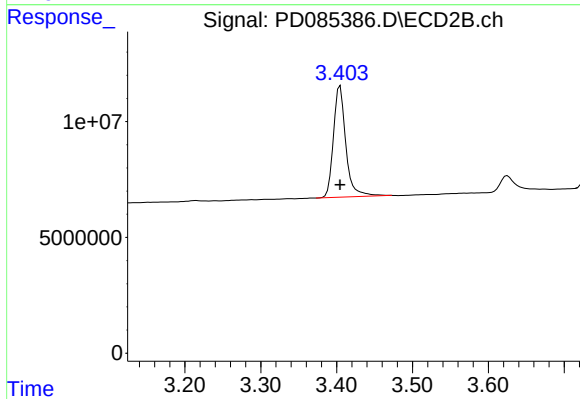


#2 alpha-BHC

R.T.: 3.405 min
Delta R.T.: 0.000 min
Response: 54475618
Conc: 9.94 ng/ml

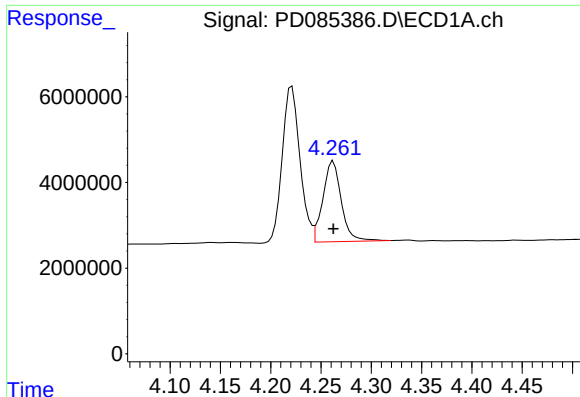


#3 gamma-BHC (Lindane)

R.T.: 4.262 min
Delta R.T.: 0.000 min
Response: 23894875
Conc: 9.99 ng/ml

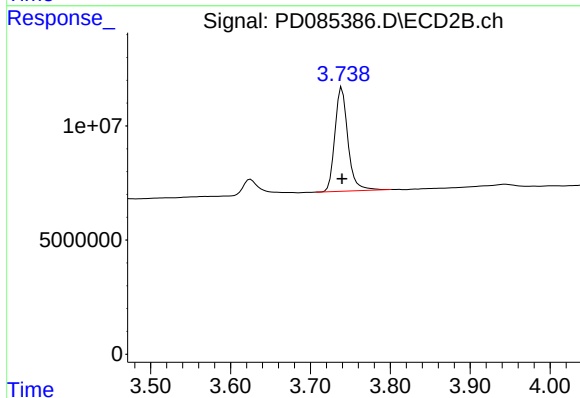


#3 gamma-BHC (Lindane)

R.T.: 3.740 min
Delta R.T.: 0.000 min
Response: 51455819
Conc: 9.95 ng/ml

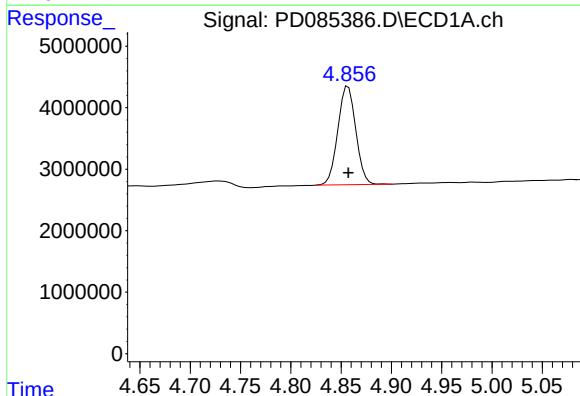


#4 Heptachlor

R.T.: 4.857 min
Delta R.T.: 0.000 min
Response: 19881954
Conc: 9.68 ng/ml

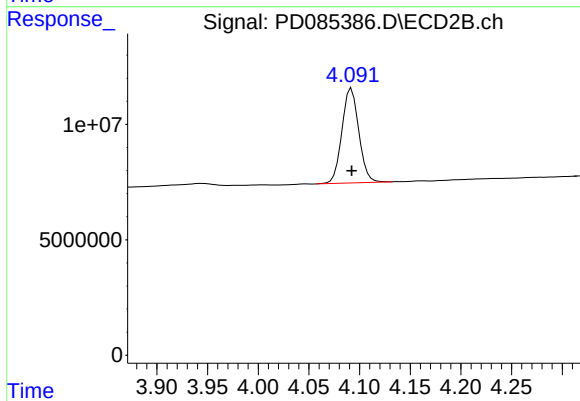


#4 Heptachlor

R.T.: 4.092 min
Delta R.T.: 0.000 min
Response: 47421675
Conc: 10.10 ng/ml

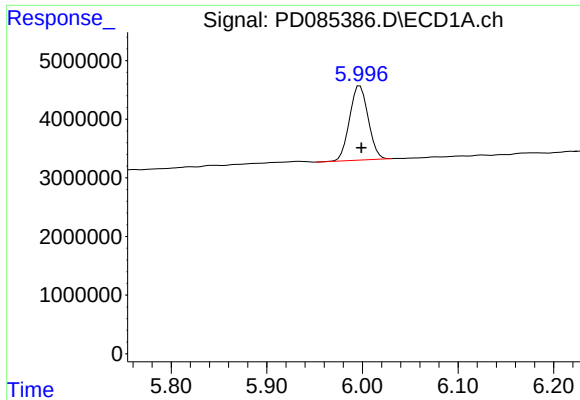


#9 Endosulfan I

R.T.: 5.998 min
Delta R.T.: -0.001 min
Response: 17144142
Conc: 9.88 ng/ml

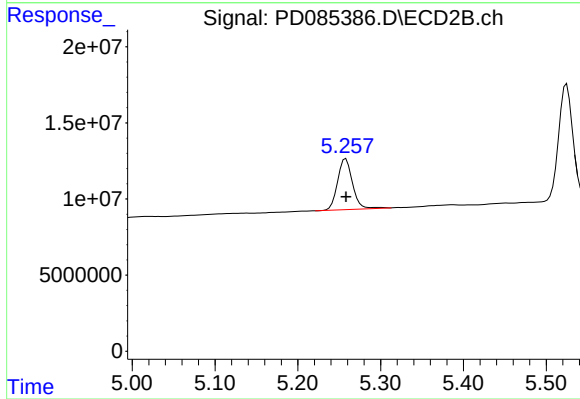


#9 Endosulfan I

R.T.: 5.258 min
Delta R.T.: 0.000 min
Response: 41797481
Conc: 10.13 ng/ml

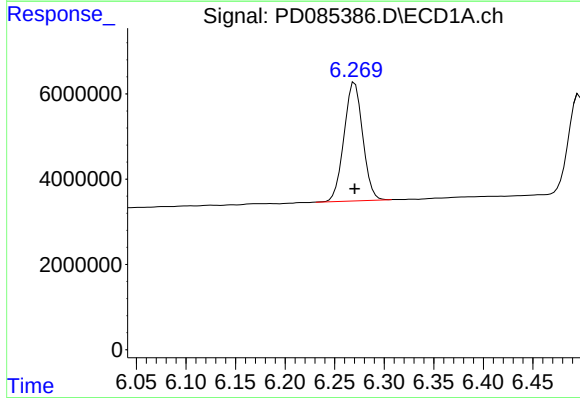


#13 Dieldrin

R.T.: 6.270 min
Delta R.T.: 0.000 min
Response: 36415179
Conc: 19.29 ng/ml

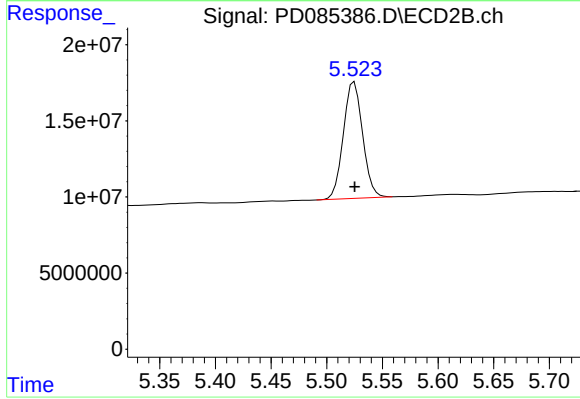


#13 Dieldrin

R.T.: 5.525 min
Delta R.T.: 0.000 min
Response: 92560946
Conc: 20.16 ng/ml

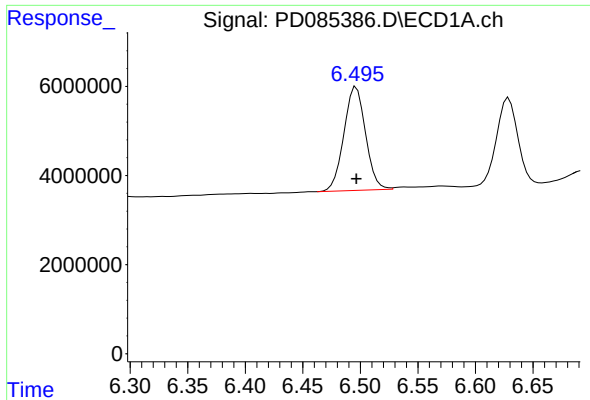


#14 Endrin

R.T.: 6.496 min
Delta R.T.: 0.000 min
Response: 30565115
Conc: 19.49 ng/ml

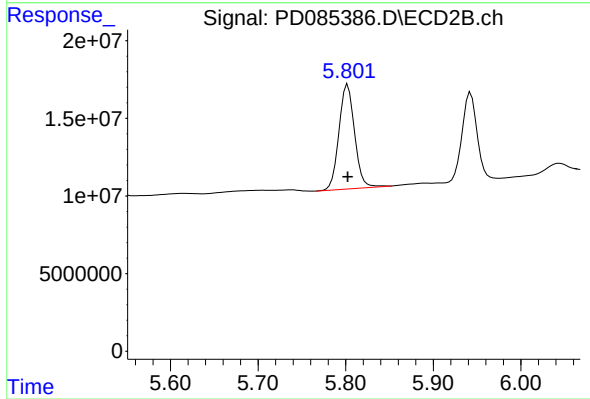


#14 Endrin

R.T.: 5.802 min
Delta R.T.: 0.000 min
Response: 83466856
Conc: 20.55 ng/ml

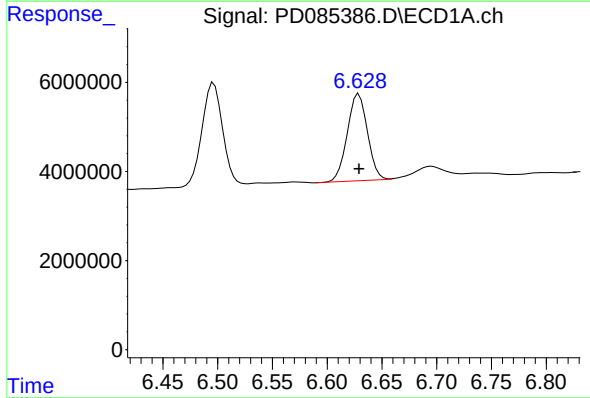


#16 4,4'-DDD

R.T.: 6.629 min
Delta R.T.: 0.000 min
Response: 25025922
Conc: 19.35 ng/ml

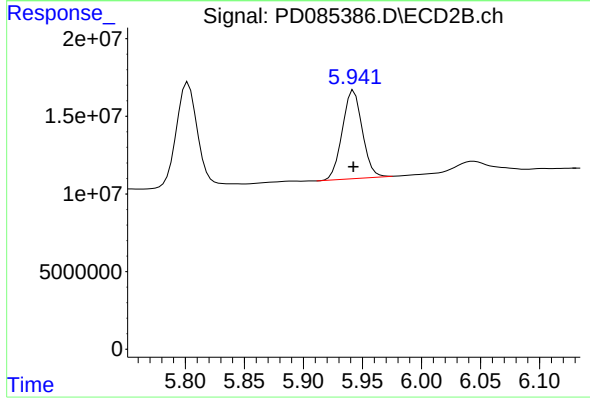


#16 4,4'-DDD

R.T.: 5.943 min
Delta R.T.: 0.000 min
Response: 66772357
Conc: 20.06 ng/ml

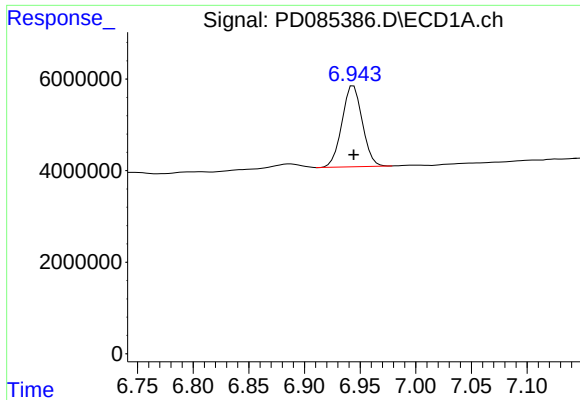


#17 4,4'-DDT

R.T.: 6.944 min
Delta R.T.: 0.000 min
Response: 22462738
Conc: 18.77 ng/ml

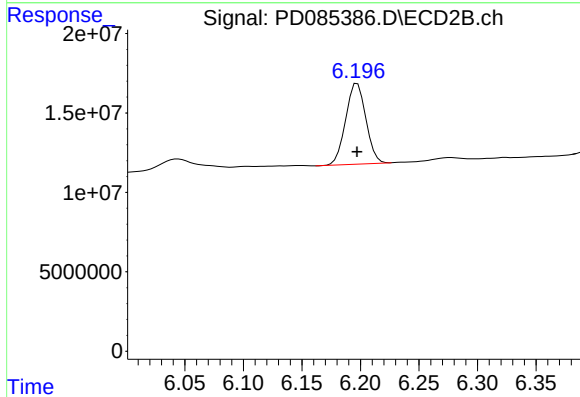


#17 4,4'-DDT

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 61088562
Conc: 19.37 ng/ml

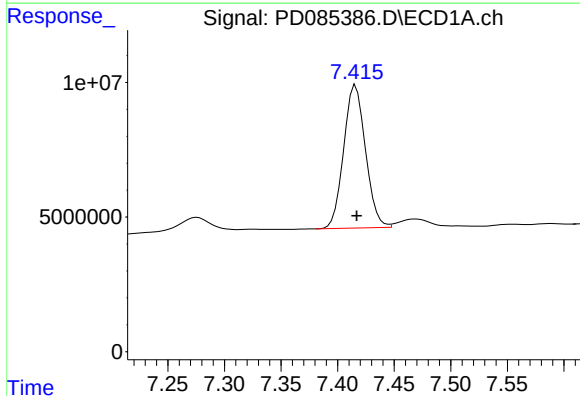


#20 Methoxychlor

R.T.: 7.416 min
Delta R.T.: 0.000 min
Response: 71196639
Conc: 99.20 ng/ml

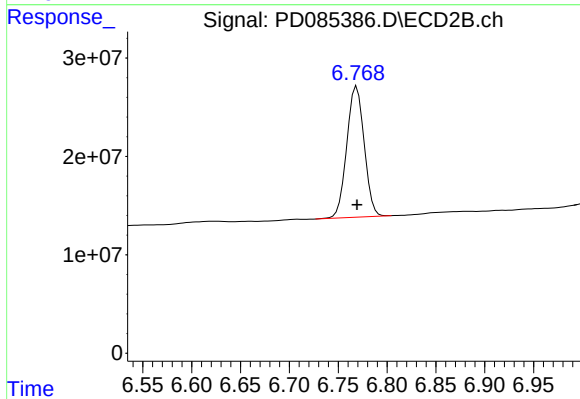


#20 Methoxychlor

R.T.: 6.769 min
Delta R.T.: 0.000 min
Response: 165299390
Conc: 101.43 ng/ml

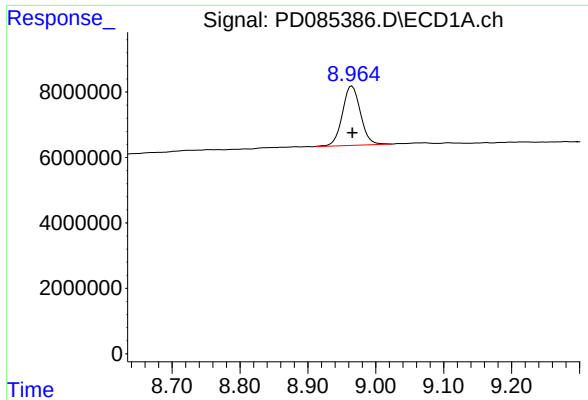

#27 Decachlorobiphenyl

R.T.: 8.965 min
Delta R.T.: 0.000 min
Response: 33492580
Conc: 20.89 ng/ml

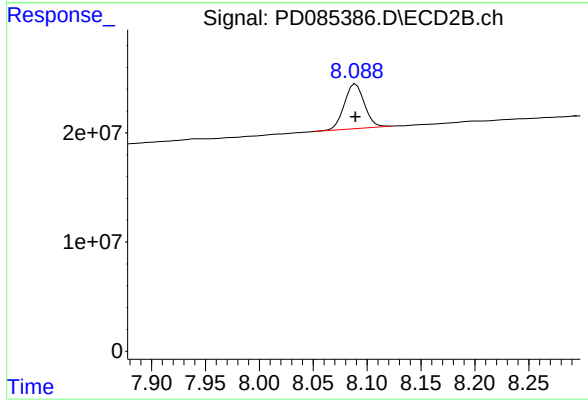

#27 Decachlorobiphenyl

R.T.: 8.089 min
Delta R.T.: 0.000 min
Response: 53102646
Conc: 20.10 ng/ml