

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091924\
 Data File : PD085388.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2024 23:20
 Operator : AR\AJ
 Sample : INDA301
 Misc :
 ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 04:51:00 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 04:48:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.490	2.894	23982365	75388073	20.000	20.000
27)	SA Decachlor...	8.965	8.089	64145831	105.7E6	40.000	40.000
Target Compounds							
2)	A alpha-BHC	3.935	3.405	45536834	109.6E6	20.000	20.000
3)	MA gamma-BHC...	4.262	3.740	47818679	103.4E6	20.000	20.000
4)	MA Heptachlor	4.857	4.092	41091713	93859736	20.000	20.000
9)	A Endosulfan I	5.999	5.258	34693516	82529601	20.000	20.000
13)	MA Dieldrin	6.270	5.525	75521435	183.7E6	40.000	40.000
14)	MA Endrin	6.496	5.802	62741058	162.5E6	40.000	40.000
16)	A 4,4'-DDD	6.629	5.942	51727298	133.1E6	40.000	40.000
17)	MA 4,4'-DDT	6.944	6.197	47870825	126.1E6	40.000	40.000
20)	A Methoxychlor	7.417	6.769	143.5E6	325.9E6	200.000	200.000


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091924\
Data File : PD085388.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2024 23:20
Operator : AR\AJ
Sample : INDA301
Misc :
ALS Vial : 13 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 04:51:00 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 04:48:53 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

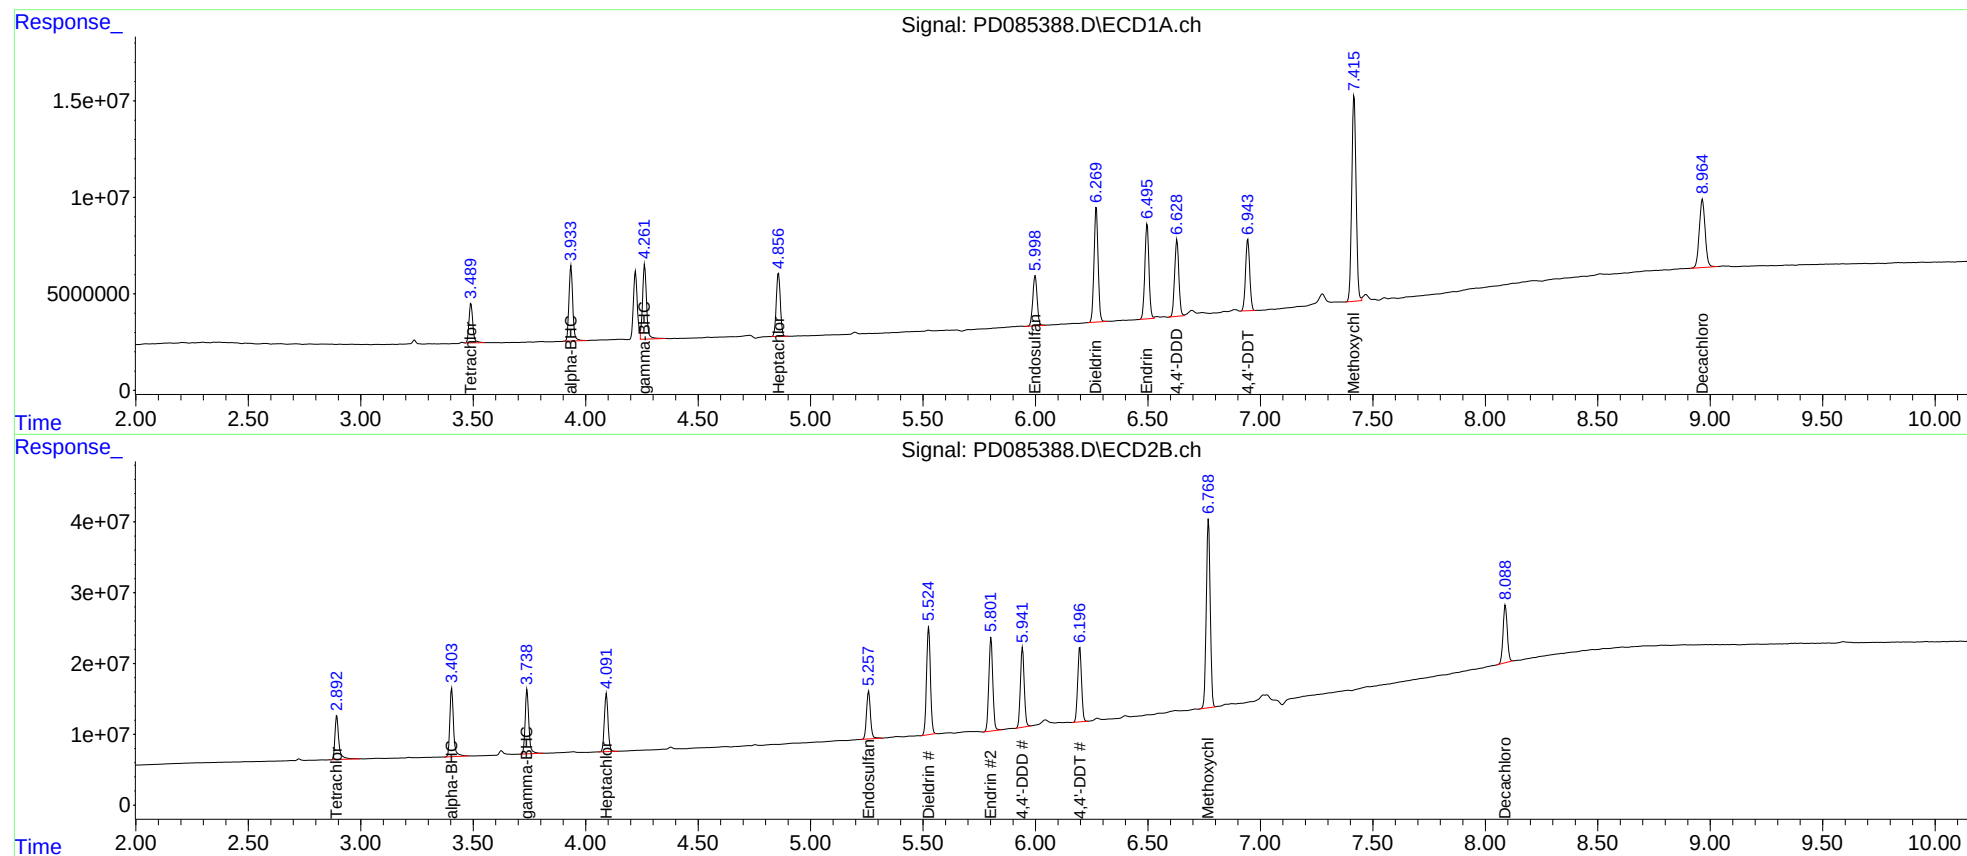

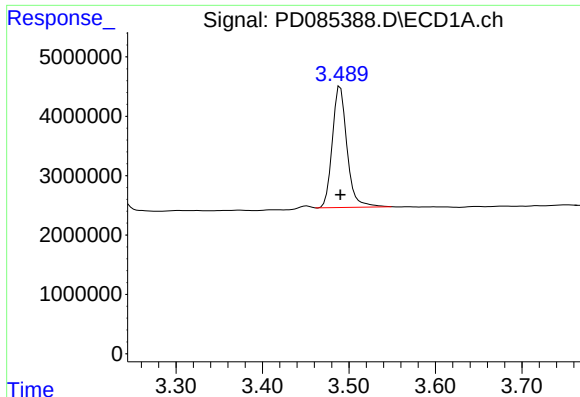


#1 Tetrachloro-m-xylene

R.T.: 3.490 min
Delta R.T.: 0.000 min
Response: 23982365
Conc: 20.00 ng/ml

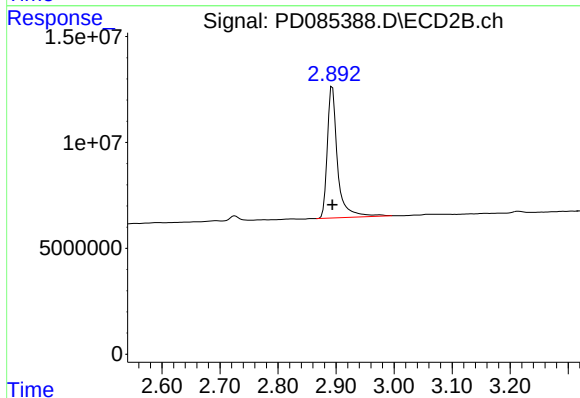


#1 Tetrachloro-m-xylene

R.T.: 2.894 min
Delta R.T.: 0.000 min
Response: 75388073
Conc: 20.00 ng/ml

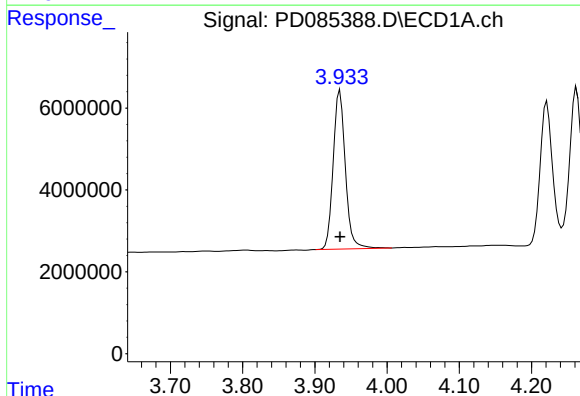


#2 alpha-BHC

R.T.: 3.935 min
Delta R.T.: 0.000 min
Response: 45536834
Conc: 20.00 ng/ml

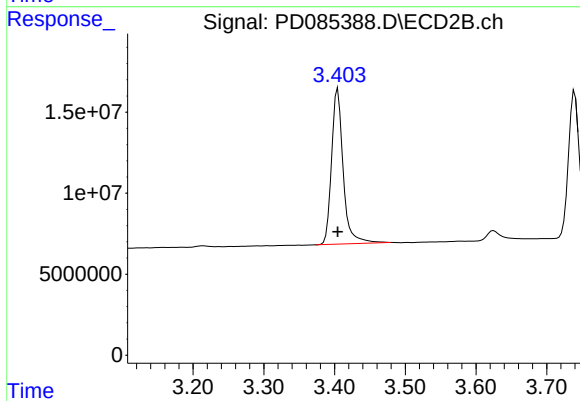

#2 alpha-BHC

R.T.: 3.405 min
Delta R.T.: 0.000 min
Response: 109645560
Conc: 20.00 ng/ml

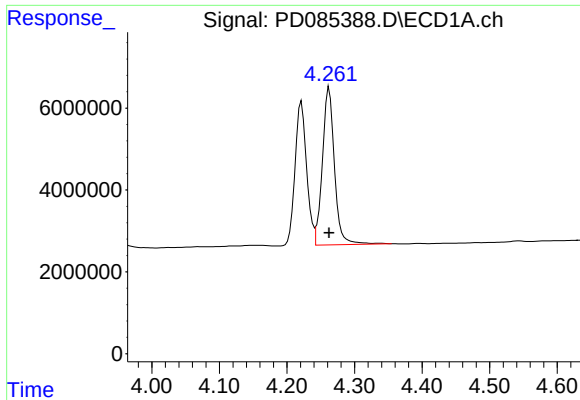


#3 gamma-BHC (Lindane)

R.T.: 4.262 min

Delta R.T.: 0.000 min

Response: 47818679

Conc: 20.00 ng/ml

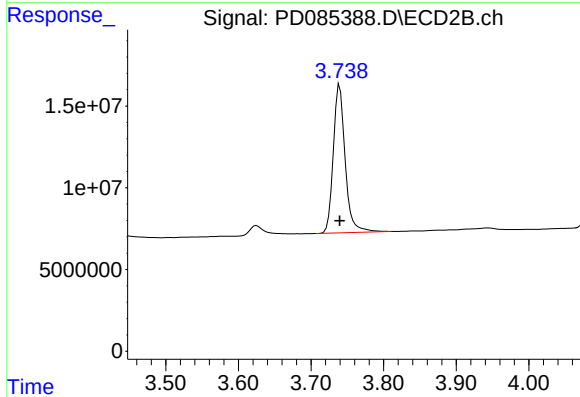


#3 gamma-BHC (Lindane)

R.T.: 3.740 min

Delta R.T.: 0.000 min

Response: 103423270

Conc: 20.00 ng/ml

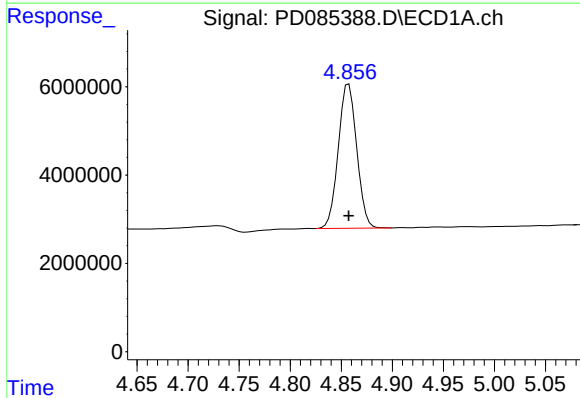


#4 Heptachlor

R.T.: 4.857 min

Delta R.T.: 0.000 min

Response: 41091713

Conc: 20.00 ng/ml

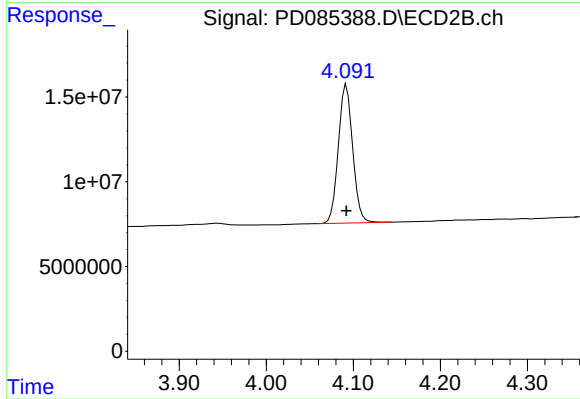


#4 Heptachlor

R.T.: 4.092 min

Delta R.T.: 0.000 min


Response: 93859736

Conc: 20.00 ng/ml

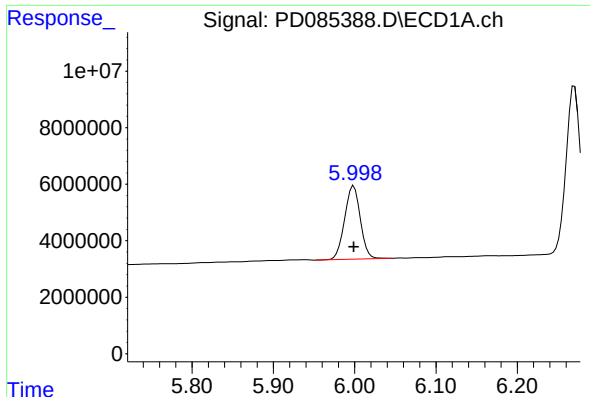


#9 Endosulfan I

R.T.: 5.999 min
Delta R.T.: 0.000 min
Response: 34693516
Conc: 20.00 ng/ml

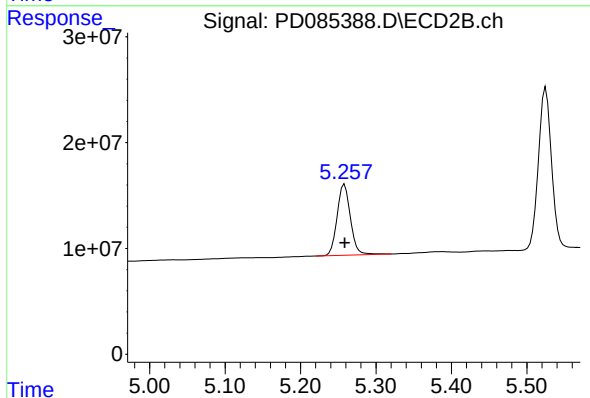


#9 Endosulfan I

R.T.: 5.258 min
Delta R.T.: 0.000 min
Response: 82529601
Conc: 20.00 ng/ml

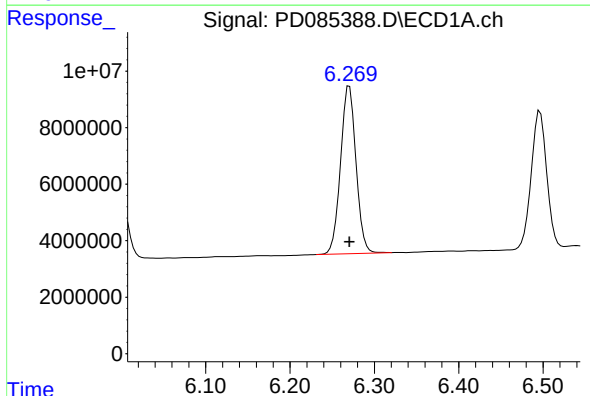


#13 Dieldrin

R.T.: 6.270 min
Delta R.T.: 0.000 min
Response: 75521435
Conc: 40.00 ng/ml

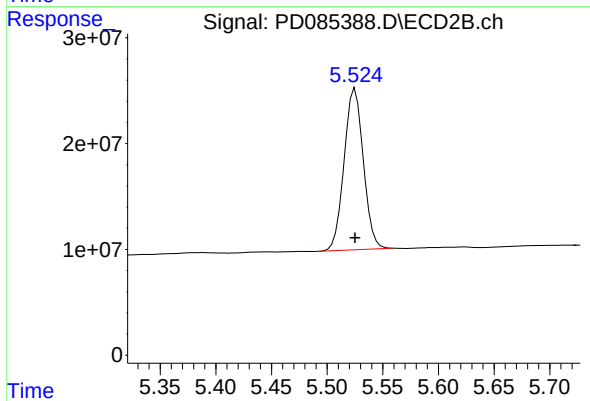


#13 Dieldrin

R.T.: 5.525 min
Delta R.T.: 0.000 min
Response: 183693419
Conc: 40.00 ng/ml

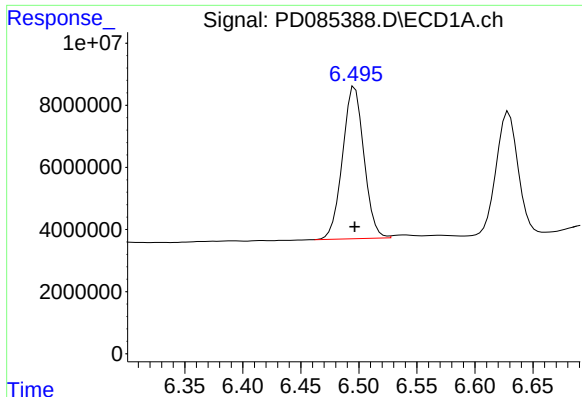


#14 Endrin

R.T.: 6.496 min
Delta R.T.: 0.000 min
Response: 62741058
Conc: 40.00 ng/ml

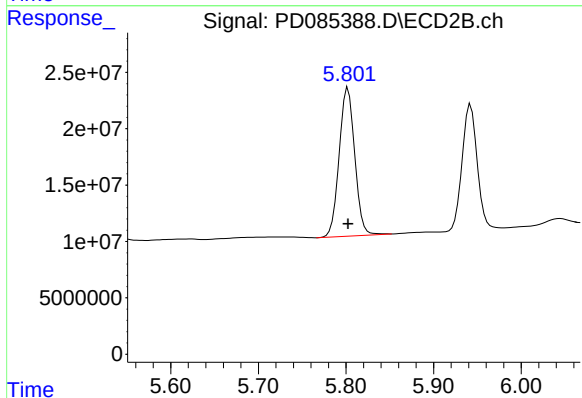


#14 Endrin

R.T.: 5.802 min
Delta R.T.: 0.000 min
Response: 162454522
Conc: 40.00 ng/ml

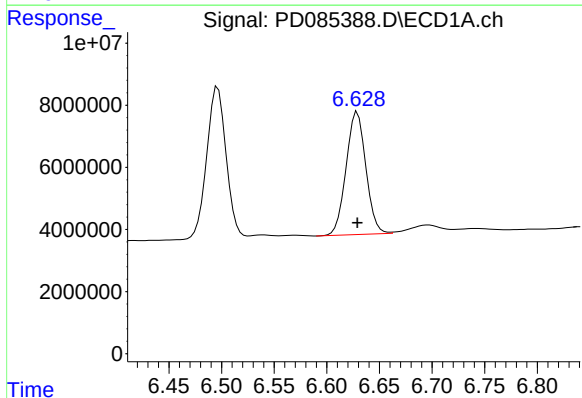


#16 4,4'-DDD

R.T.: 6.629 min
Delta R.T.: 0.000 min
Response: 51727298
Conc: 40.00 ng/ml

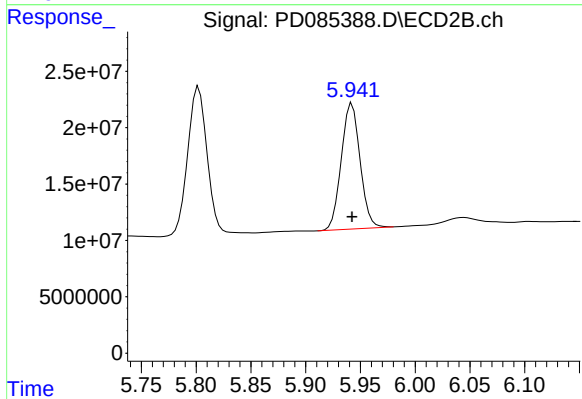


#16 4,4'-DDD

R.T.: 5.942 min
Delta R.T.: 0.000 min
Response: 133148286
Conc: 40.00 ng/ml

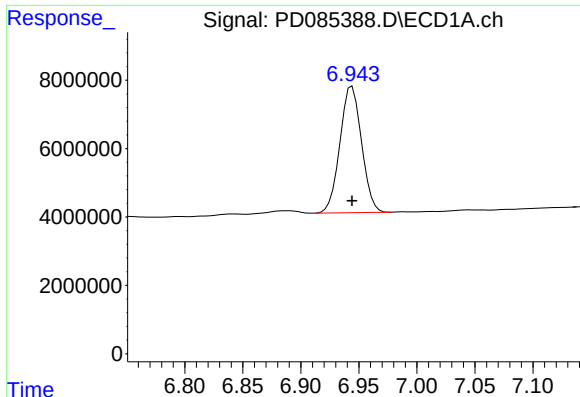


#17 4,4'-DDT

R.T.: 6.944 min
Delta R.T.: 0.000 min
Response: 47870825
Conc: 40.00 ng/ml

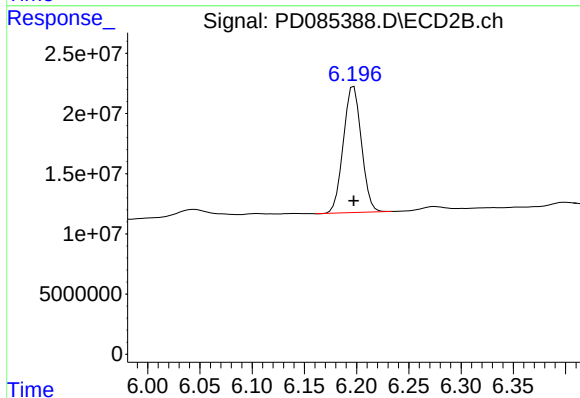


#17 4,4'-DDT

R.T.: 6.197 min
Delta R.T.: 0.000 min
Response: 126125709
Conc: 40.00 ng/ml

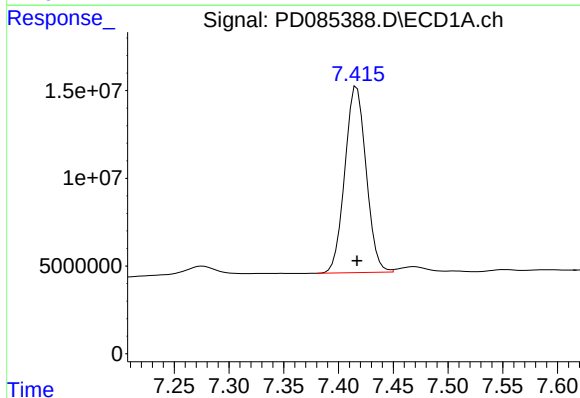


#20 Methoxychlor

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 143541291
Conc: 200.00 ng/ml

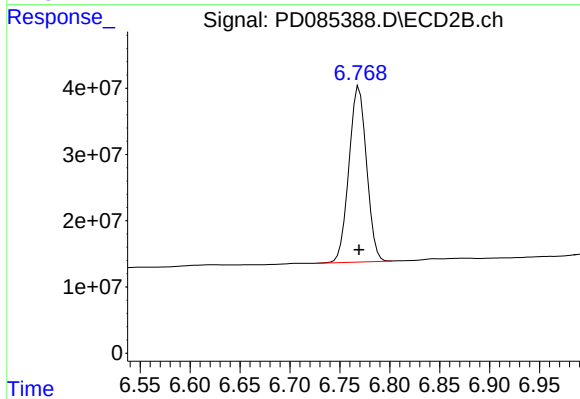


#20 Methoxychlor

R.T.: 6.769 min
Delta R.T.: 0.000 min
Response: 325924691
Conc: 200.00 ng/ml

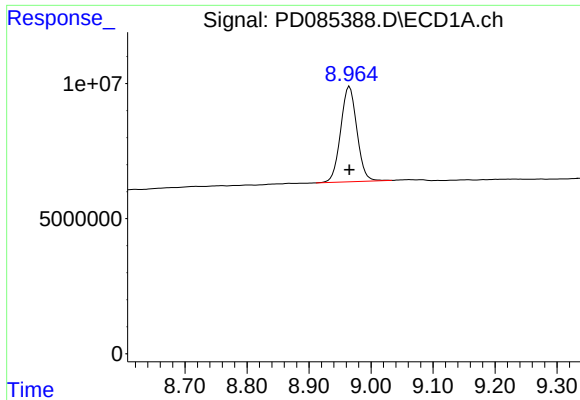

#27 Decachlorobiphenyl

R.T.: 8.965 min
Delta R.T.: 0.000 min
Response: 64145831
Conc: 40.00 ng/ml

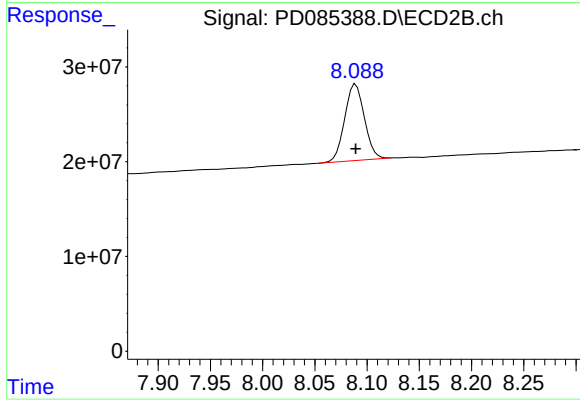

#27 Decachlorobiphenyl

R.T.: 8.089 min
Delta R.T.: 0.000 min
Response: 105651722
Conc: 40.00 ng/ml