

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091924\
 Data File : PD085391.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2024 00:00
 Operator : AR\AJ
 Sample : INDB401
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 04:22:20 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 04:09:21 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR2 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.490	2.894	52468315	157.9E6	41.893	40.577
27)	SA Decachlor...	8.965	8.090	131.2E6	221.9E6	80.013	81.581
Target Compounds							
5)	MB Aldrin	5.197	4.378	90849932	204.8E6	43.324	40.929
6)	B beta-BHC	4.447	4.033	39067817	92025464	41.086	39.974
7)	B delta-BHC	4.693	4.271	98110459	215.5E6	44.448	41.512
8)	B Heptachlo...	5.616	4.883	81447773	187.8E6	41.714	40.735
10)	B trans-Chl...	5.870	5.136	77581202	184.3E6	42.019	41.199
11)	B cis-Chlor...	5.951	5.200	80455070	188.3E6	41.802	40.886
12)	B 4,4'-DDE	6.121	5.386	148.1E6	349.3E6	87.294	83.294
15)	B Endosulfa...	6.708	6.095	137.6E6	304.5E6	80.806	81.970
18)	B Endrin al...	6.837	6.274	97301518	224.0E6	82.913	81.339
19)	B Endosulfa...	7.070	6.499	124.4E6	280.5E6	84.762	81.808
21)	B Endrin ke...	7.550	7.009	133.1E6	334.8E6	84.935	77.059


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091924\
Data File : PD085391.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2024 00:00
Operator : AR\AJ
Sample : INDB401
Misc :
ALS Vial : 16 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 04:22:20 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 04:09:21 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

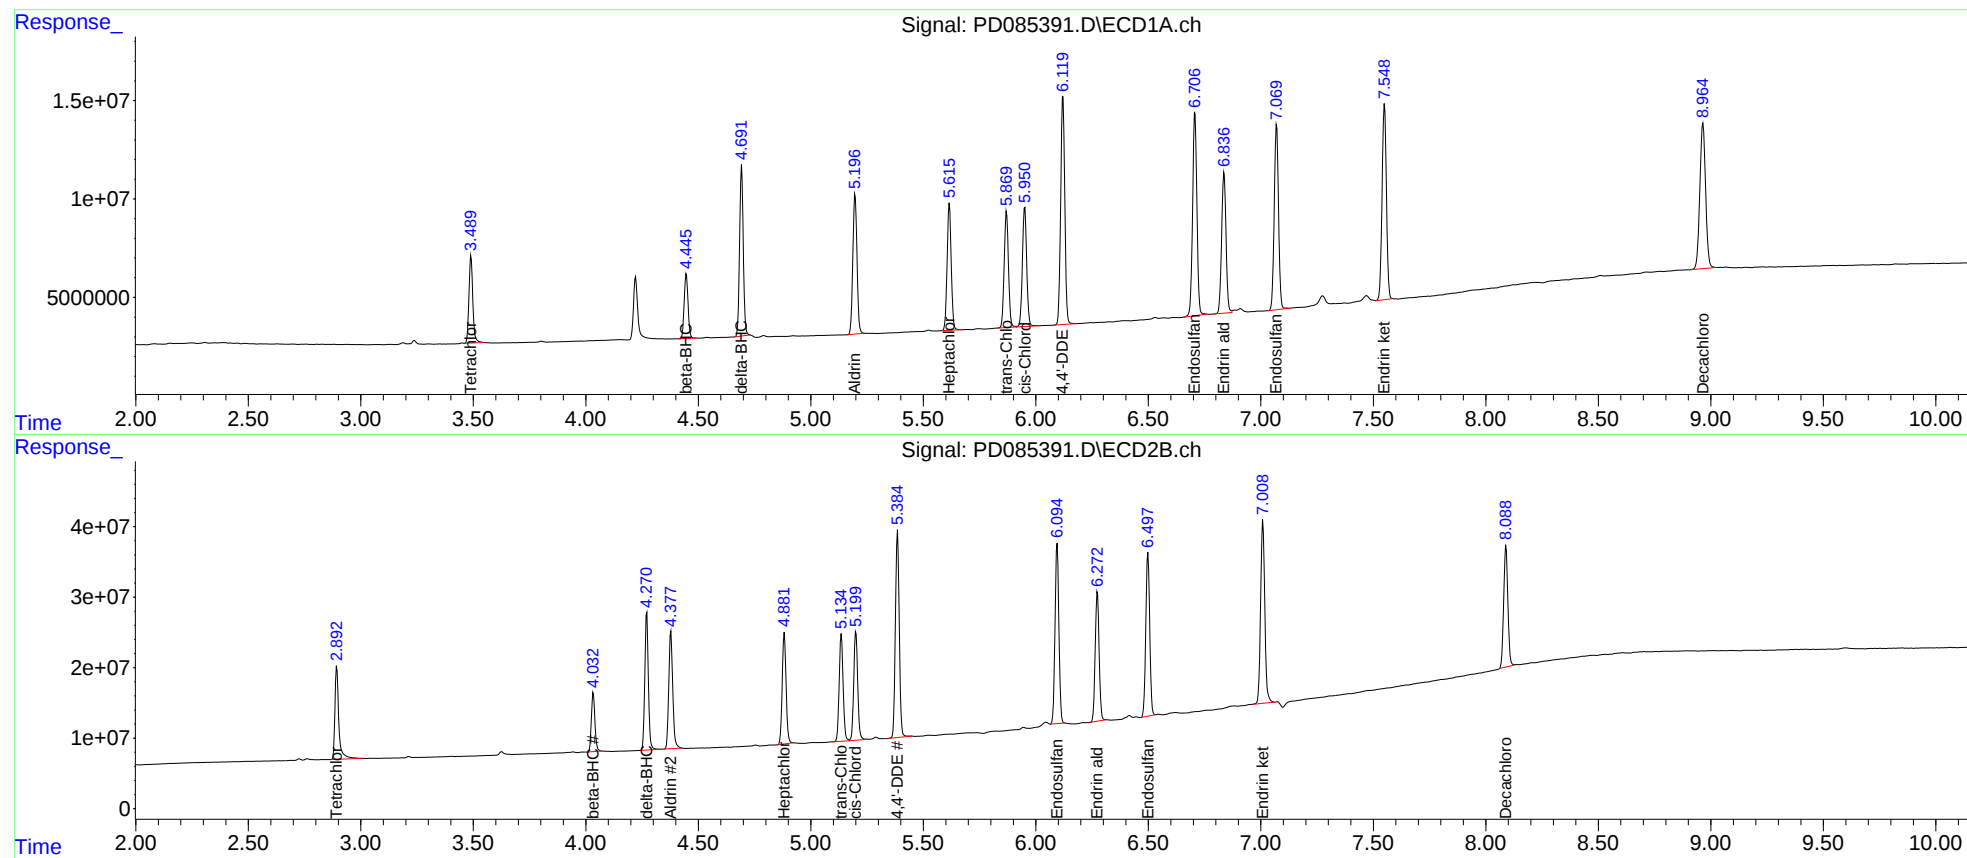

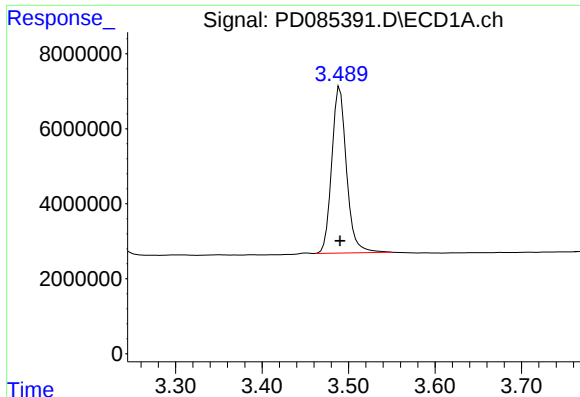


#1 Tetrachloro-m-xylene

R.T.: 3.490 min
Delta R.T.: 0.000 min
Response: 52468315
Conc: 41.89 ng/ml

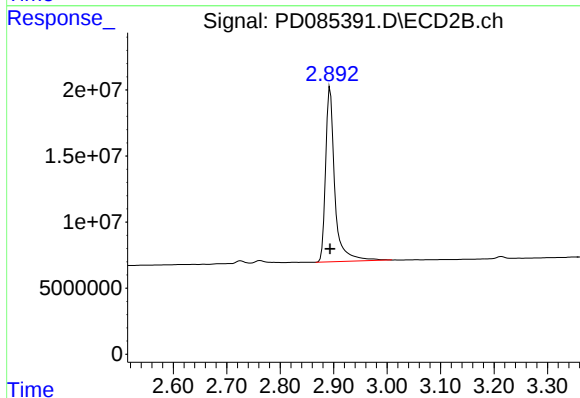


#1 Tetrachloro-m-xylene

R.T.: 2.894 min
Delta R.T.: 0.000 min
Response: 157878212
Conc: 40.58 ng/ml

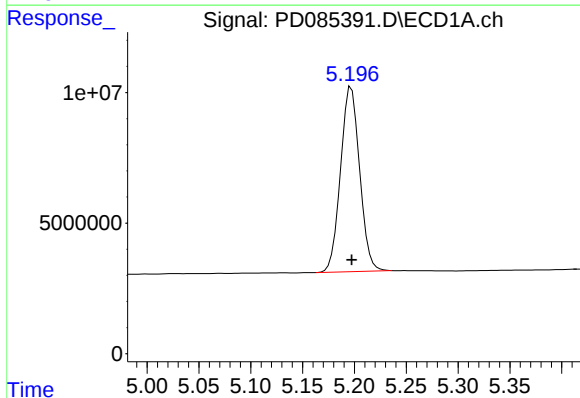


#5 Aldrin

R.T.: 5.197 min
Delta R.T.: 0.000 min
Response: 90849932
Conc: 43.32 ng/ml

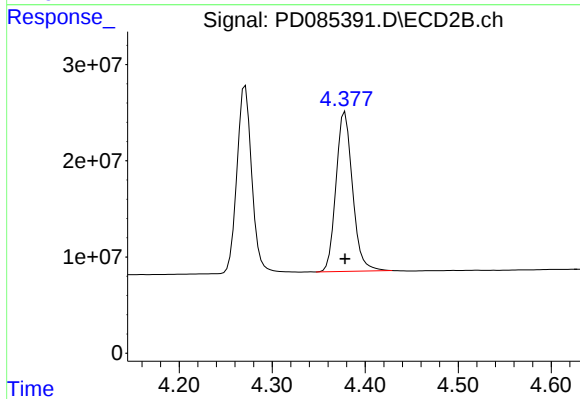


#5 Aldrin

R.T.: 4.378 min
Delta R.T.: 0.000 min
Response: 204776605
Conc: 40.93 ng/ml

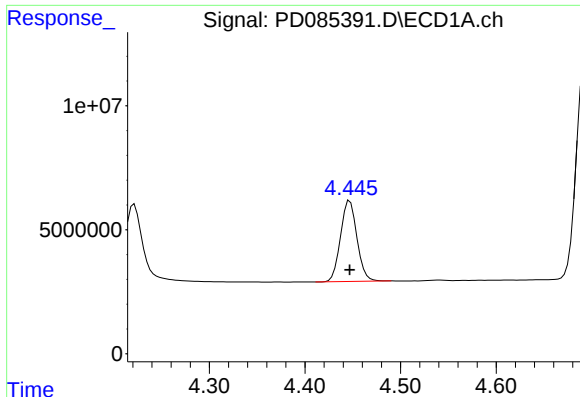


#6 beta-BHC

R.T.: 4.447 min
Delta R.T.: 0.000 min
Response: 39067817
Conc: 41.09 ng/ml

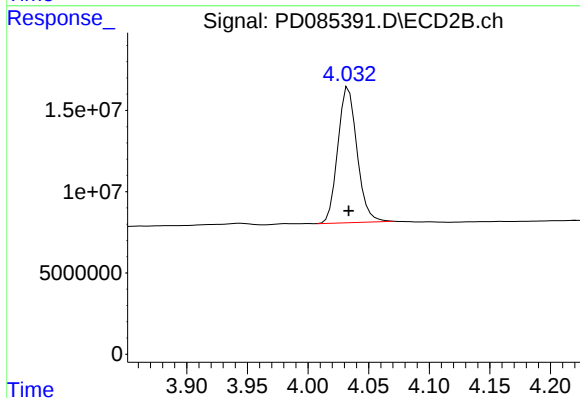


#6 beta-BHC

R.T.: 4.033 min
Delta R.T.: 0.000 min
Response: 92025464
Conc: 39.97 ng/ml

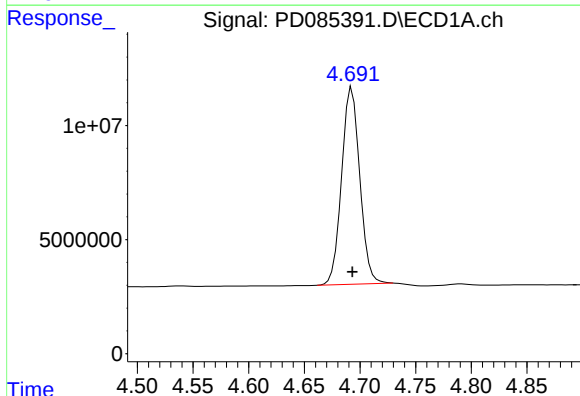


#7 delta-BHC

R.T.: 4.693 min
Delta R.T.: 0.000 min
Response: 98110459
Conc: 44.45 ng/ml

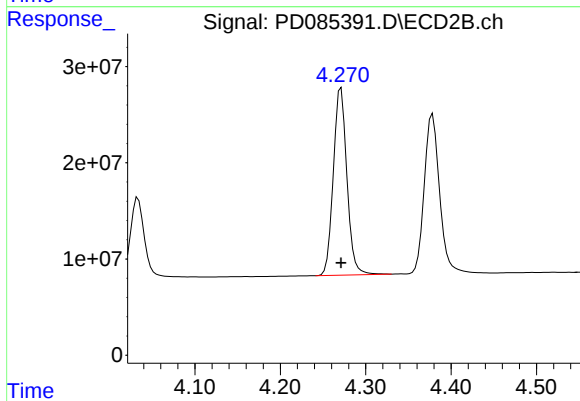


#7 delta-BHC

R.T.: 4.271 min
Delta R.T.: 0.000 min
Response: 215461445
Conc: 41.51 ng/ml

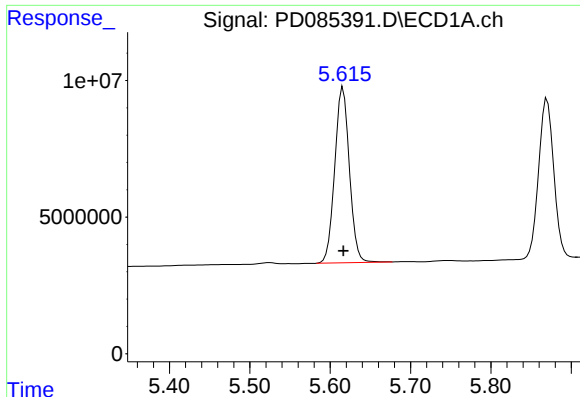


#8 Heptachlor epoxide

R.T.: 5.616 min
Delta R.T.: 0.000 min
Response: 81447773
Conc: 41.71 ng/ml

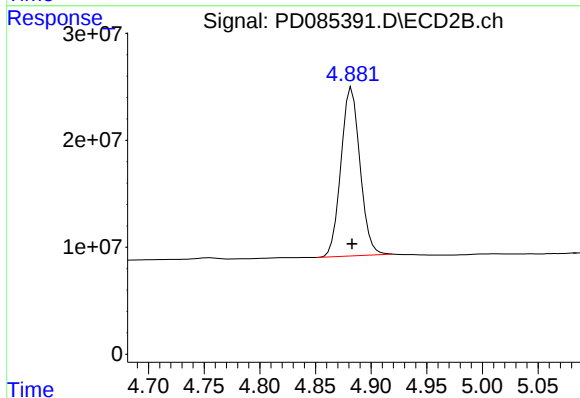


#8 Heptachlor epoxide

R.T.: 4.883 min
Delta R.T.: 0.000 min
Response: 187815010
Conc: 40.73 ng/ml

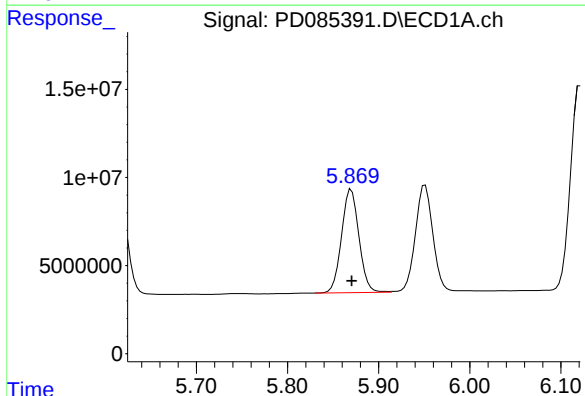


#10 trans-Chlordane

R.T.: 5.870 min
Delta R.T.: 0.000 min
Response: 77581202
Conc: 42.02 ng/ml

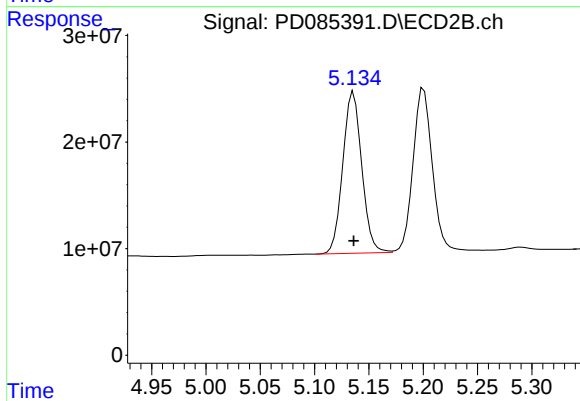


#10 trans-Chlordane

R.T.: 5.136 min
Delta R.T.: 0.000 min
Response: 184274213
Conc: 41.20 ng/ml

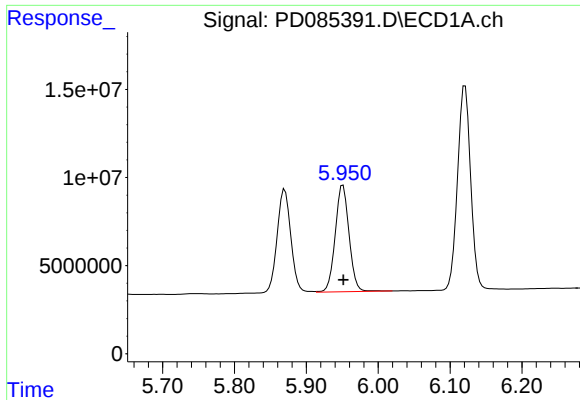


#11 cis-Chlordane

R.T.: 5.951 min
Delta R.T.: 0.000 min
Response: 80455070
Conc: 41.80 ng/ml

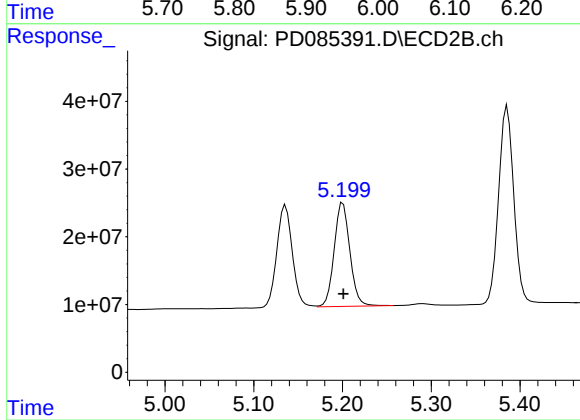


#11 cis-Chlordane

R.T.: 5.200 min
Delta R.T.: 0.000 min
Response: 188307886
Conc: 40.89 ng/ml

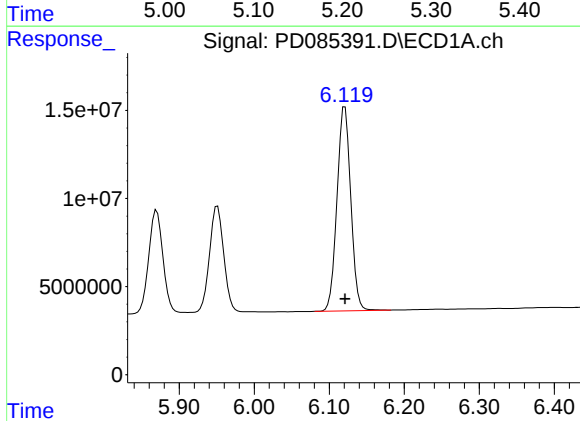


#12 4,4'-DDE

R.T.: 6.121 min
Delta R.T.: 0.000 min
Response: 148052321
Conc: 87.29 ng/ml

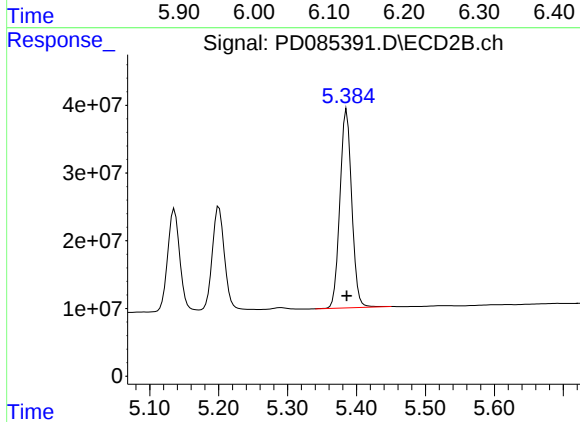


#12 4,4'-DDE

R.T.: 5.386 min
Delta R.T.: 0.000 min
Response: 349342291
Conc: 83.29 ng/ml

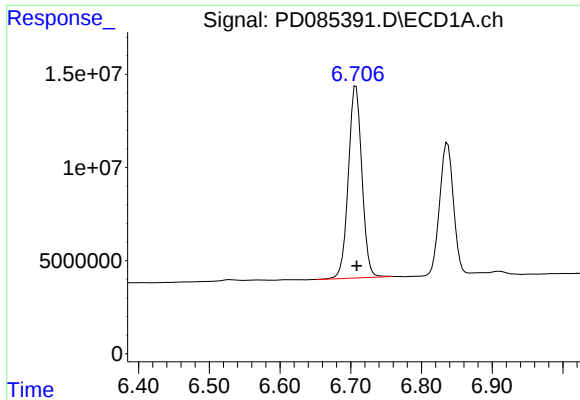


#15 Endosulfan II

R.T.: 6.708 min
Delta R.T.: -0.001 min
Response: 137576278
Conc: 80.81 ng/ml

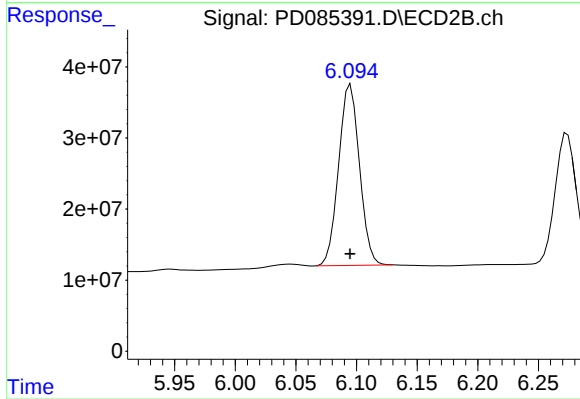


#15 Endosulfan II

R.T.: 6.095 min
Delta R.T.: 0.000 min
Response: 304505049
Conc: 81.97 ng/ml

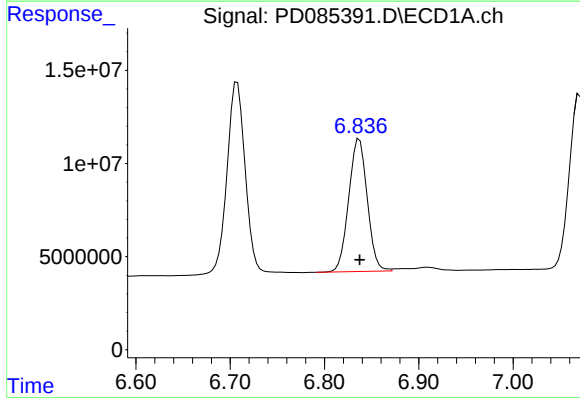


#18 Endrin aldehyde

R.T.: 6.837 min
Delta R.T.: 0.000 min
Response: 97301518
Conc: 82.91 ng/ml

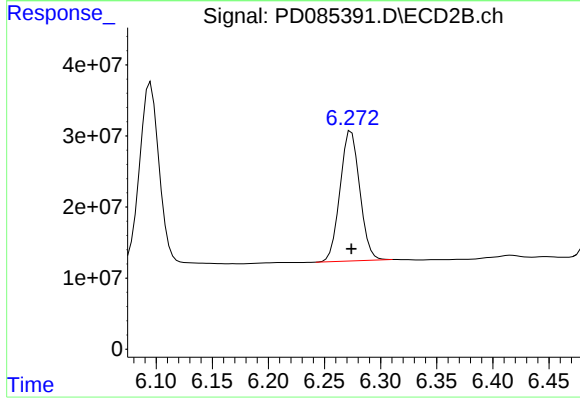


#18 Endrin aldehyde

R.T.: 6.274 min
Delta R.T.: 0.000 min
Response: 224010333
Conc: 81.34 ng/ml

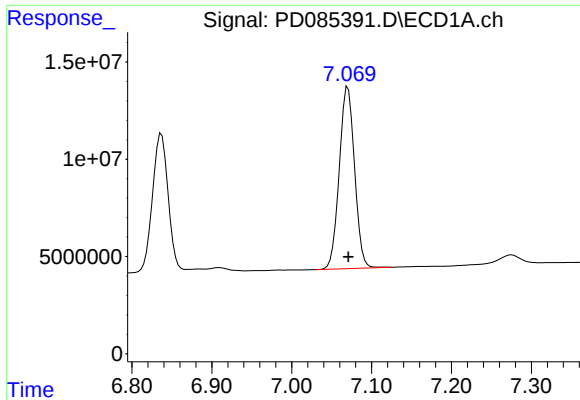


#19 Endosulfan Sulfate

R.T.: 7.070 min
Delta R.T.: 0.000 min
Response: 124417084
Conc: 84.76 ng/ml

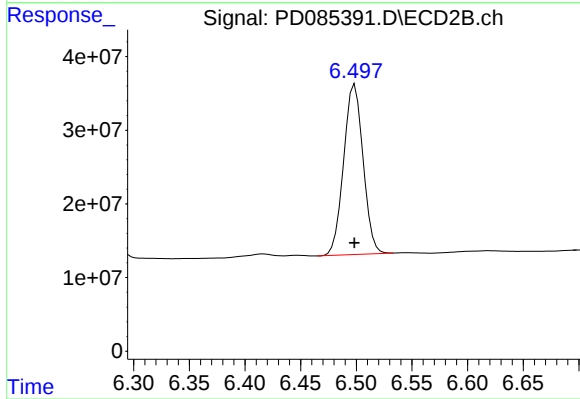


#19 Endosulfan Sulfate

R.T.: 6.499 min
Delta R.T.: 0.000 min
Response: 280547718
Conc: 81.81 ng/ml

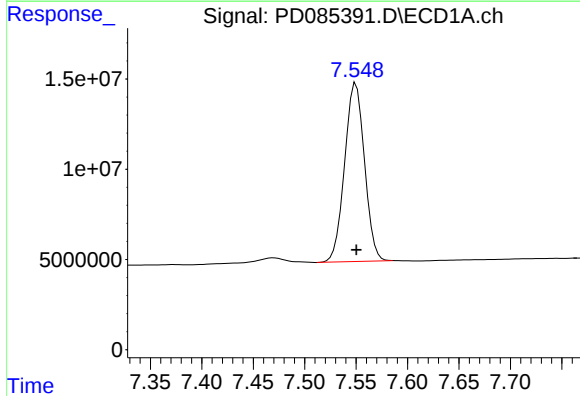


#21 Endrin ketone

R.T.: 7.550 min
Delta R.T.: 0.000 min
Response: 133083026
Conc: 84.93 ng/ml

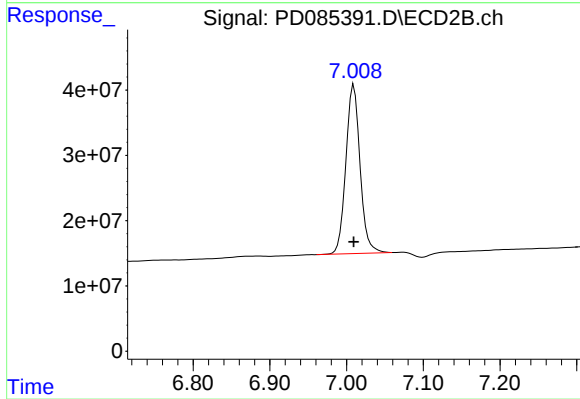


#21 Endrin ketone

R.T.: 7.009 min
Delta R.T.: 0.000 min
Response: 334825563
Conc: 77.06 ng/ml

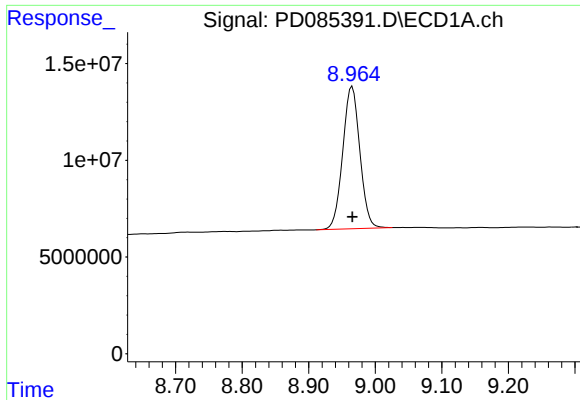

#27 Decachlorobiphenyl

R.T.: 8.965 min
Delta R.T.: 0.000 min
Response: 131240782
Conc: 80.01 ng/ml

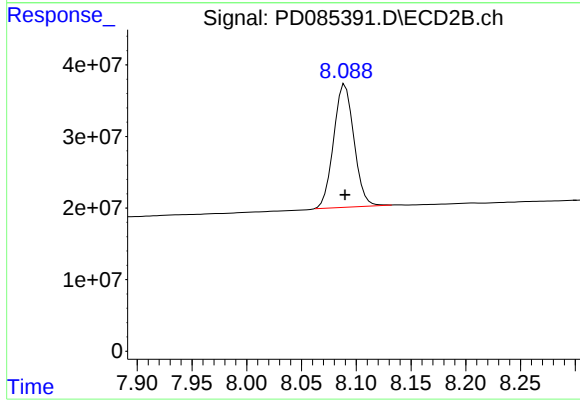

#27 Decachlorobiphenyl

R.T.: 8.090 min
Delta R.T.: 0.000 min
Response: 221866751
Conc: 81.58 ng/ml