

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091924\
 Data File : PD085392.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2024 00:14
 Operator : AR\AJ
 Sample : INDA501
 Misc :
 ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 04:51:29 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 04:48:53 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.491	2.893	104.4E6	298.5E6	87.032	79.188
27)	SA Decachlor...	8.964	8.090	257.9E6	443.5E6	160.807	167.892
Target Compounds							
2)	A alpha-BHC	3.935	3.404	223.9E6	459.3E6	98.334	83.787
3)	MA gamma-BHC...	4.263	3.739	212.9E6	427.9E6	89.054	82.738
4)	MA Heptachlor	4.858	4.092	190.3E6	388.2E6	92.628	82.719
9)	A Endosulfan I	5.998	5.258	149.8E6	334.6E6	86.338	81.074
13)	MA Dieldrin	6.270	5.525	344.2E6	752.1E6	182.300	163.780
14)	MA Endrin	6.497	5.802	285.9E6	658.8E6	182.257	162.217
16)	A 4,4'-DDD	6.629	5.942	233.9E6	550.8E6	180.909	165.481
17)	MA 4,4'-DDT	6.944	6.198	225.7E6	549.1E6	188.551	174.141
20)	A Methoxychlor	7.417	6.770	622.7E6	1265.0E6	867.584	776.283


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091924\
Data File : PD085392.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2024 00:14
Operator : AR\AJ
Sample : INDA501
Misc :
ALS Vial : 17 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 04:51:29 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 04:48:53 2024
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

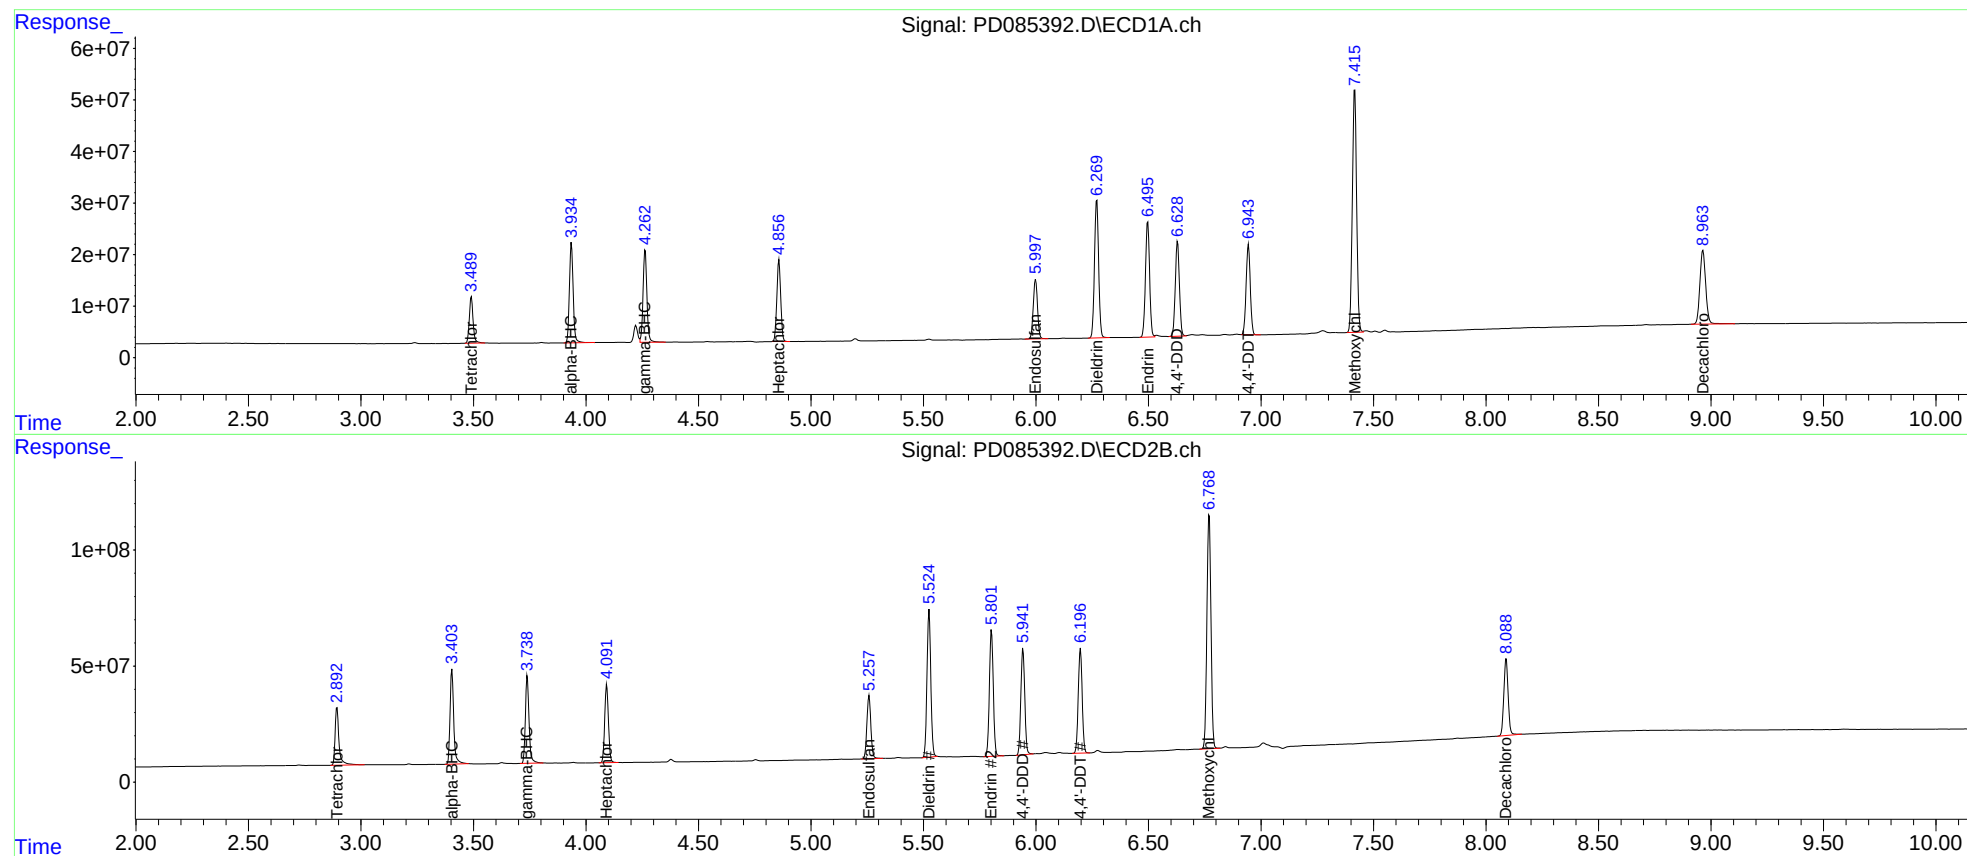

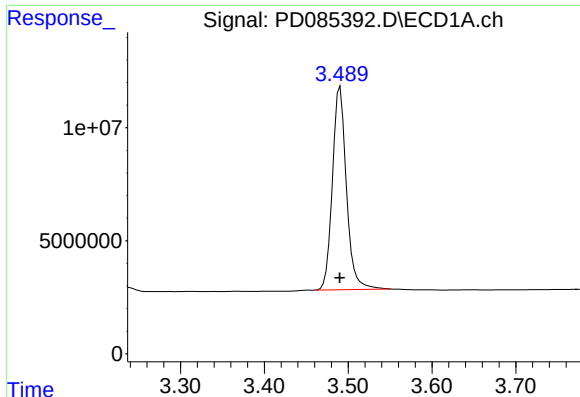


#1 Tetrachloro-m-xylene

R.T.: 3.491 min
Delta R.T.: 0.000 min
Response: 104361719
Conc: 87.03 ng/ml

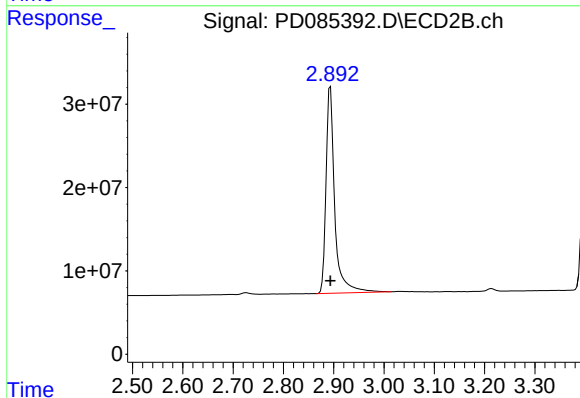


#1 Tetrachloro-m-xylene

R.T.: 2.893 min
Delta R.T.: 0.000 min
Response: 298492753
Conc: 79.19 ng/ml

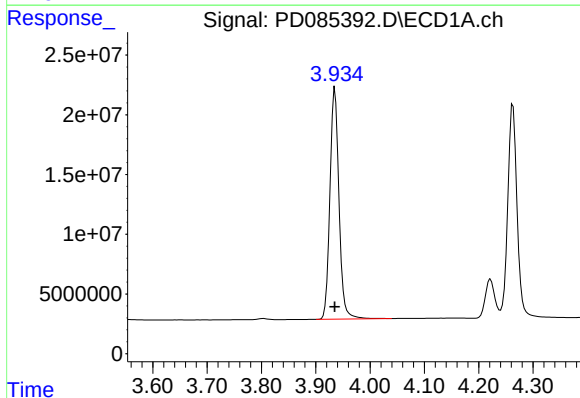


#2 alpha-BHC

R.T.: 3.935 min
Delta R.T.: 0.000 min
Response: 223890836
Conc: 98.33 ng/ml

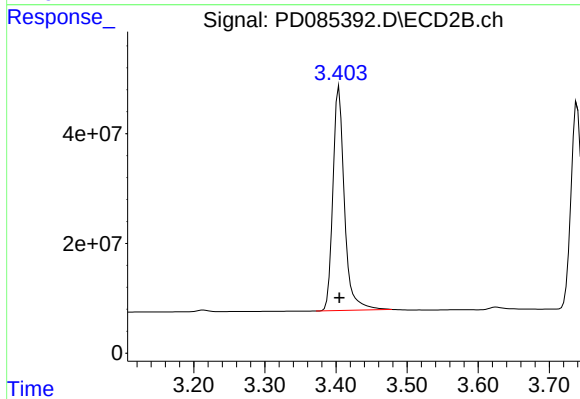


#2 alpha-BHC

R.T.: 3.404 min
Delta R.T.: 0.000 min
Response: 459344272
Conc: 83.79 ng/ml

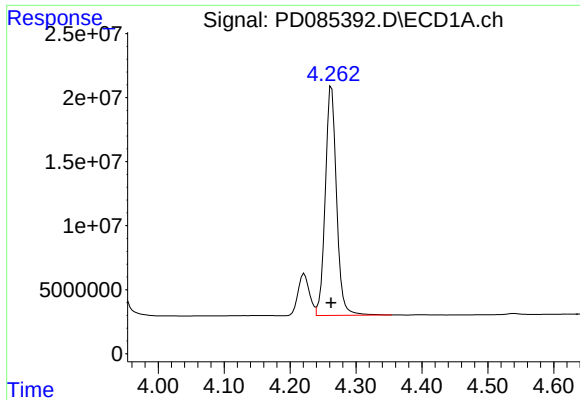


#3 gamma-BHC (Lindane)

R.T.: 4.263 min
Delta R.T.: 0.000 min
Response: 212921571
Conc: 89.05 ng/ml

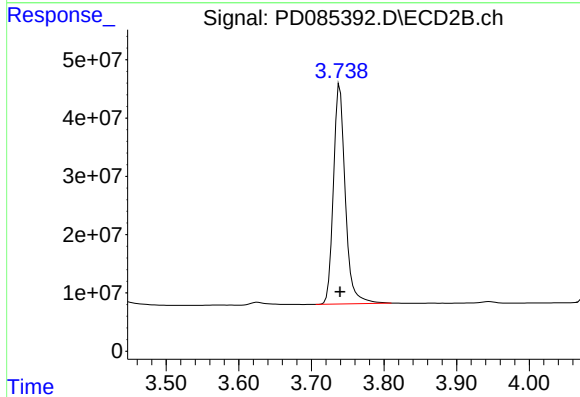


#3 gamma-BHC (Lindane)

R.T.: 3.739 min
Delta R.T.: 0.000 min
Response: 427850254
Conc: 82.74 ng/ml

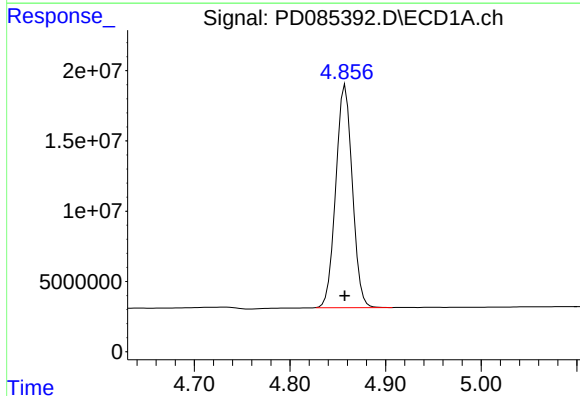


#4 Heptachlor

R.T.: 4.858 min
Delta R.T.: 0.000 min
Response: 190311688
Conc: 92.63 ng/ml

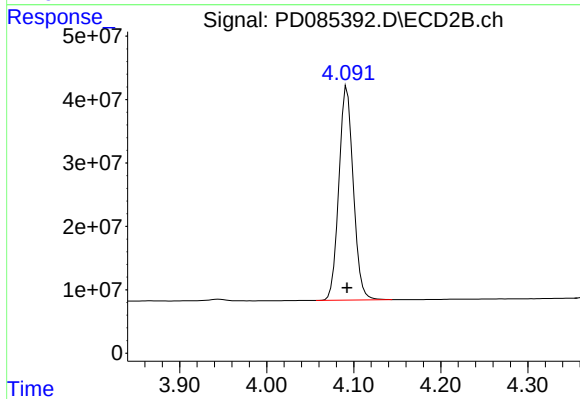


#4 Heptachlor

R.T.: 4.092 min
Delta R.T.: 0.000 min
Response: 388200116
Conc: 82.72 ng/ml

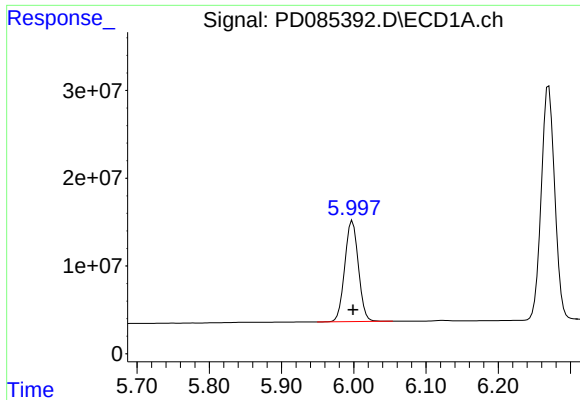


#9 Endosulfan I

R.T.: 5.998 min
Delta R.T.: 0.000 min
Response: 149768722
Conc: 86.34 ng/ml

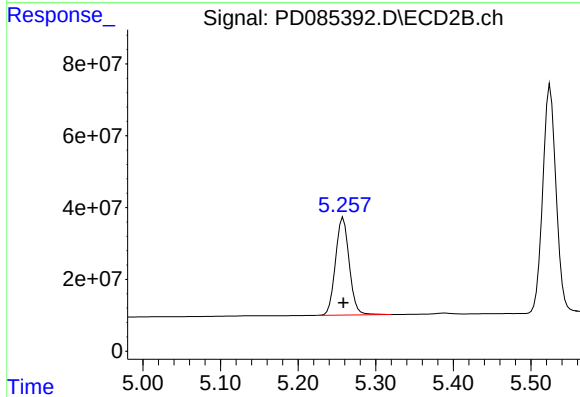


#9 Endosulfan I

R.T.: 5.258 min
Delta R.T.: 0.000 min
Response: 334550385
Conc: 81.07 ng/ml

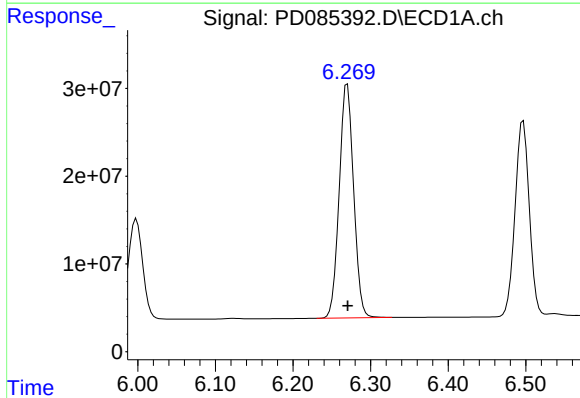


#13 Dieldrin

R.T.: 6.270 min
Delta R.T.: 0.000 min
Response: 344188849
Conc: 182.30 ng/ml

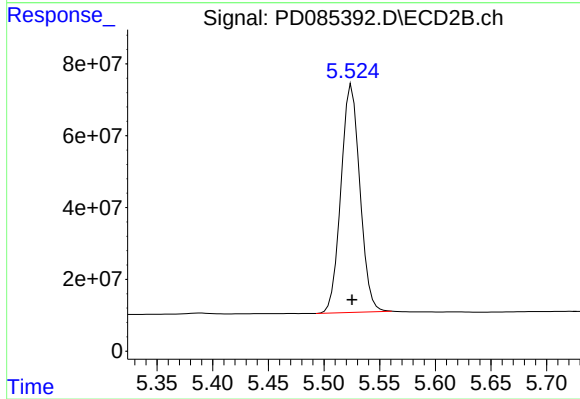


#13 Dieldrin

R.T.: 5.525 min
Delta R.T.: 0.000 min
Response: 752131711
Conc: 163.78 ng/ml

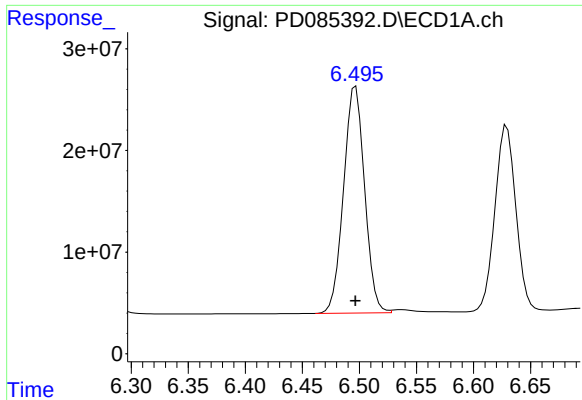


#14 Endrin

R.T.: 6.497 min
Delta R.T.: 0.000 min
Response: 285874504
Conc: 182.26 ng/ml

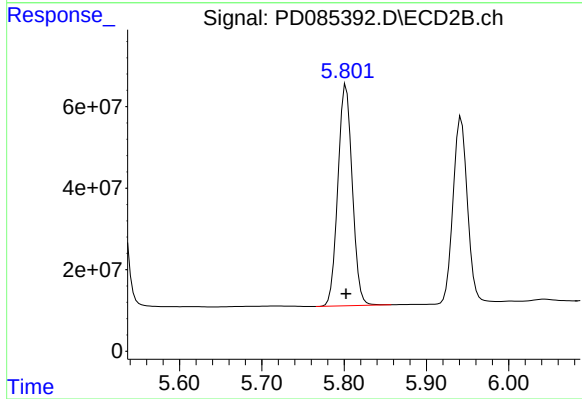


#14 Endrin

R.T.: 5.802 min
Delta R.T.: 0.000 min
Response: 658820383
Conc: 162.22 ng/ml

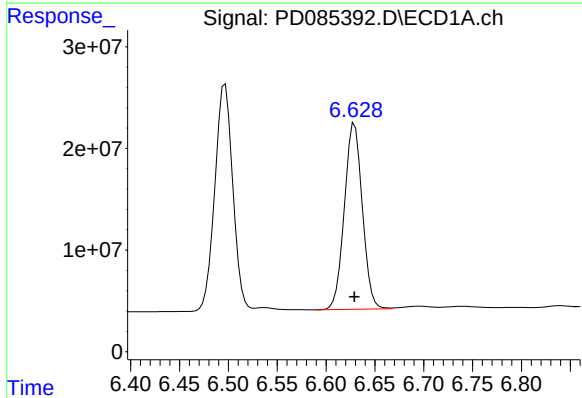


#16 4,4'-DDD

R.T.: 6.629 min
Delta R.T.: 0.000 min
Response: 233948119
Conc: 180.91 ng/ml

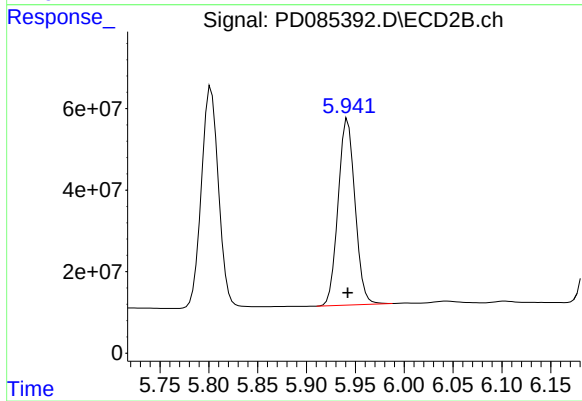


#16 4,4'-DDD

R.T.: 5.942 min
Delta R.T.: 0.000 min
Response: 550836184
Conc: 165.48 ng/ml

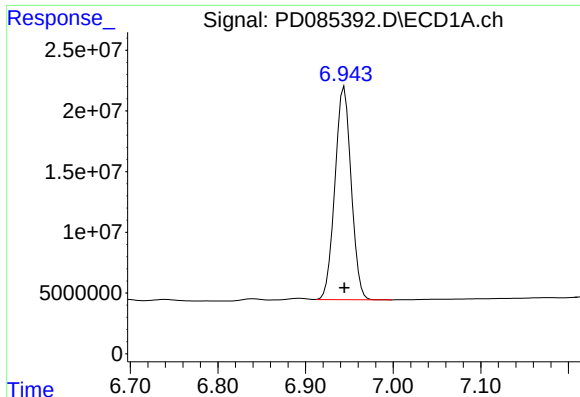


#17 4,4'-DDT

R.T.: 6.944 min
Delta R.T.: 0.000 min
Response: 225652619
Conc: 188.55 ng/ml

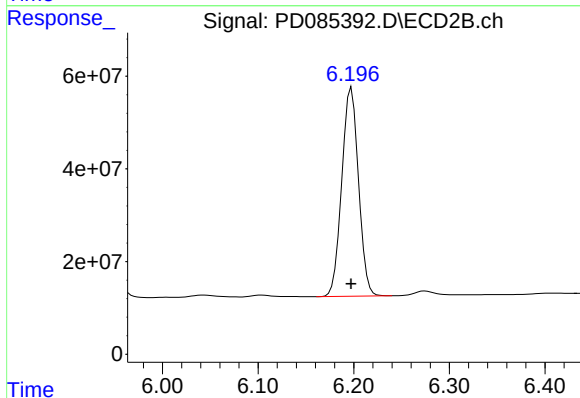


#17 4,4'-DDT

R.T.: 6.198 min
Delta R.T.: 0.000 min
Response: 549091189
Conc: 174.14 ng/ml

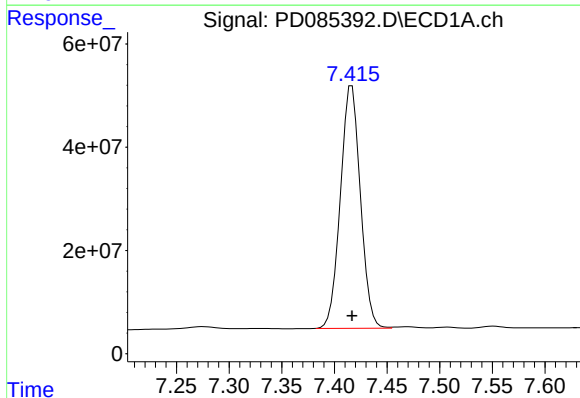


#20 Methoxychlor

R.T.: 7.417 min
Delta R.T.: 0.000 min
Response: 622670525
Conc: 867.58 ng/ml

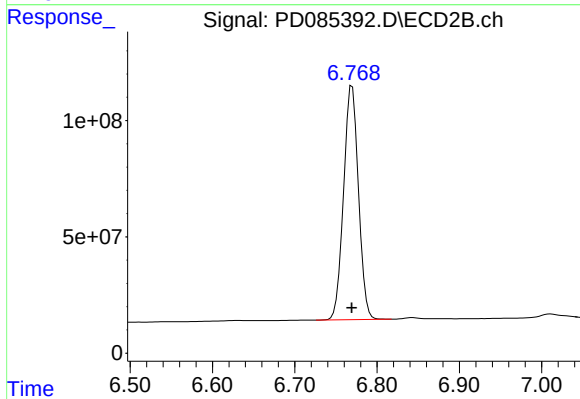


#20 Methoxychlor

R.T.: 6.770 min
Delta R.T.: 0.000 min
Response: 1265048554
Conc: 776.28 ng/ml

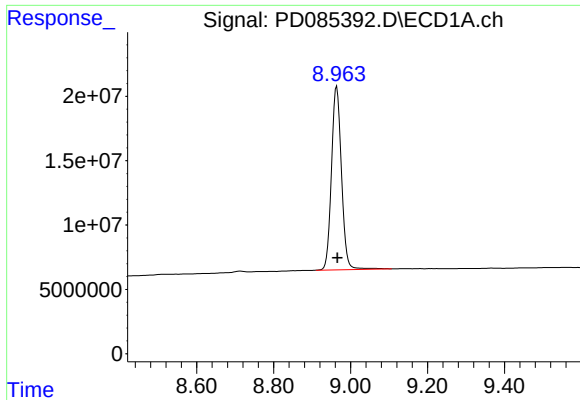

#27 Decachlorobiphenyl

R.T.: 8.964 min
Delta R.T.: -0.001 min
Response: 257876941
Conc: 160.81 ng/ml

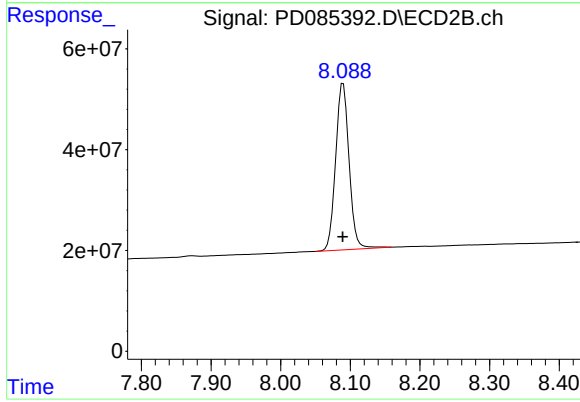

#27 Decachlorobiphenyl

R.T.: 8.090 min
Delta R.T.: 0.000 min
Response: 443451782
Conc: 167.89 ng/ml