

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091924\
 Data File : PD085408.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2024 05:07
 Operator : AR\AJ
 Sample : P3878-18DL2 40X
 Misc :
 ALS Vial : 32 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDCC1DL2

Manual Integrations
 APPROVED

Reviewed By : Abdul Mirza 09/23/2024
 Supervised By : Ankita Jodhani 09/23/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 06:27:38 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 05:48:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml
----------	------	------	--------	--------	-------	-------

System Monitoring Compounds

Target Compounds


2) A	alpha-BHC	3.935	3.403	104.1E6	180.7E6	44.071	32.729m#
3) MA	gamma-BHC...	4.254	3.737	346.3E6	194.9E6	138.435m	37.398m#
6) B	beta-BHC	4.444	4.031	11519970	15934708	12.080m	6.852m#
7) B	delta-BHC	4.693	4.269	162.2E6	321.7E6	71.165	61.067m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091924\
Data File : PD085408.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2024 05:07
Operator : AR\AJ
Sample : P3878-18DL2 40X
Misc :
ALS Vial : 32 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 06:27:38 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 05:48:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x 0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

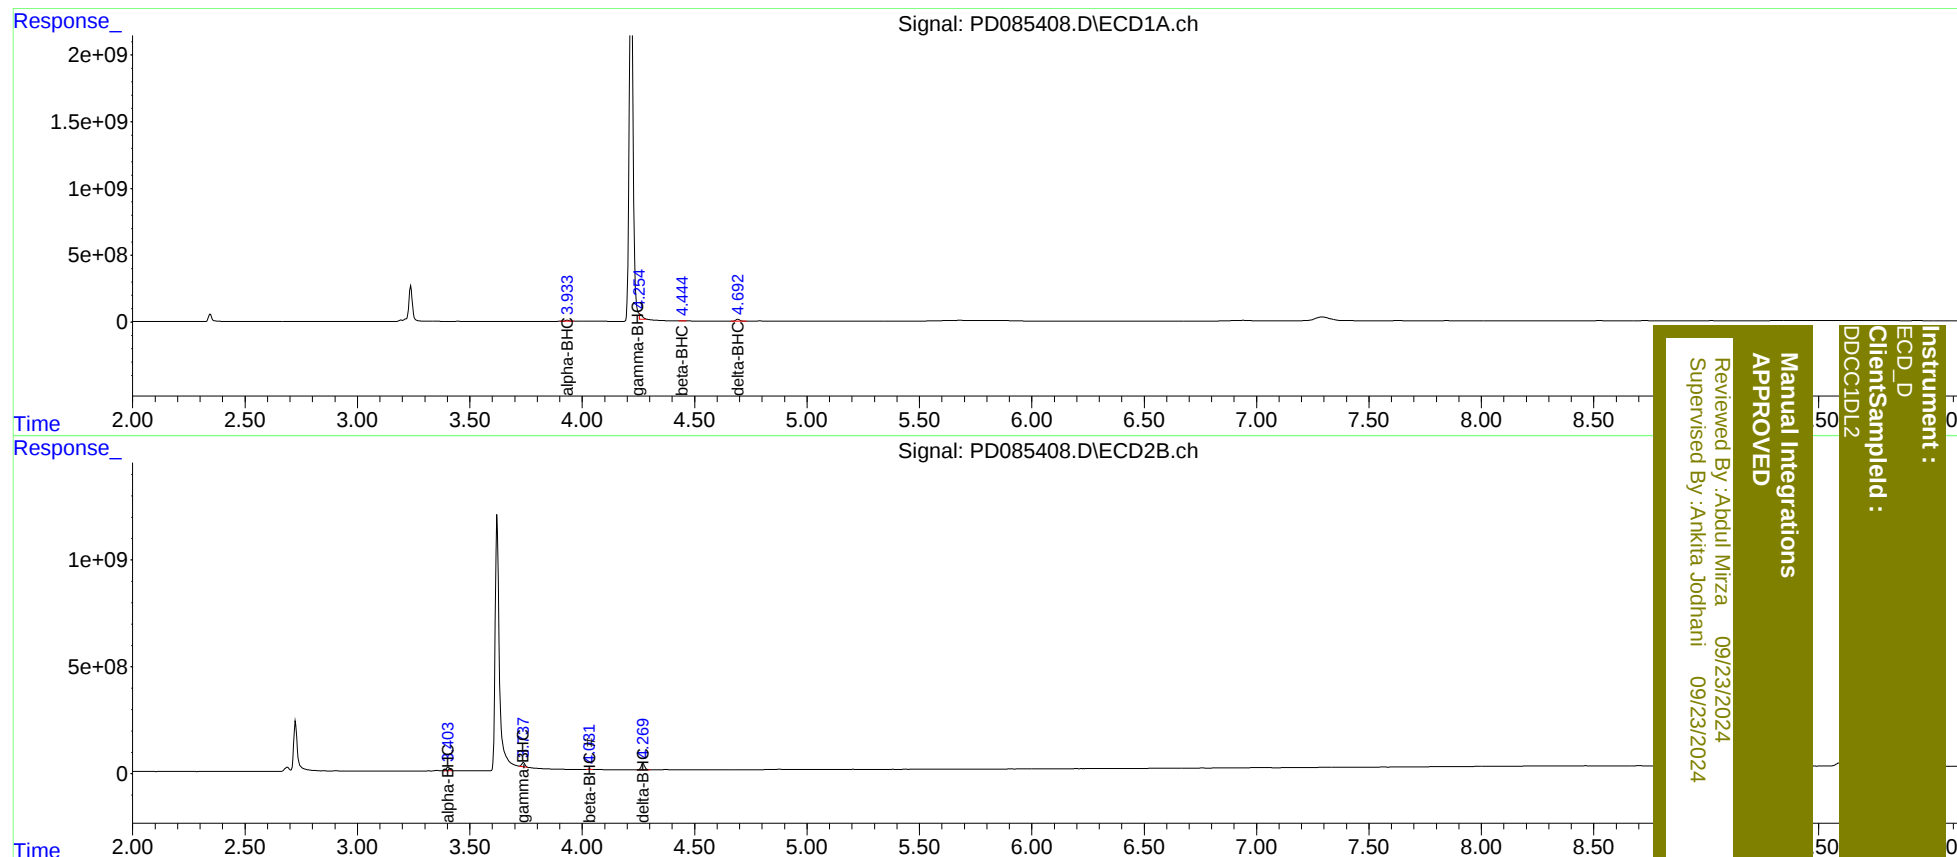

Instrument :
ECD_D
ClientSampled :
DDCC1DL2

Manual Integrations
APPROVED

Reviewed By : Abdul Mirza 09/23/2024
Supervised By : Ankita Jodhani 09/23/2024