

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091924\
 Data File : PD085415.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 20 Sep 2024 06:41
 Operator : AR\AJ
 Sample : P3898-15DL 10X
 Misc :
 ALS Vial : 39 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 DDC88DL

Manual Integrations
 APPROVED

Reviewed By :Yogesh
 Patel
 09/21/2024

Supervised By :mohammad
 ahmed
 09/22/2024

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 20 08:26:04 2024
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
 Quant Title : GC Extractables
 QLast Update : Fri Sep 20 05:48:22 2024
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds						
1) SA Tetrachlo...	3.472	2.905	12281016	53396981	10.141m	14.127m#
2) SA Decachlor...	8.966	8.087	2090469	3794420	1.274m	1.419m
Target Compounds						
2) A alpha-BHC	3.934	3.402	80432004	126.1E6	34.042	22.844m#
3) MA gamma-BHC...	4.253	3.737	335.3E6	283.8E6	134.031m	54.464m#
6) B beta-BHC	4.446	4.031	5189225	8630067	5.441m	3.711m#
7) B delta-BHC	4.693	4.269	90422616	181.7E6	39.666	34.500m

(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091924\
Data File : PD085415.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 20 Sep 2024 06:41
Operator : AR\AJ
Sample : P3898-15DL 10X
Misc :
ALS Vial : 39 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 20 08:26:04 2024
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091924CLP.M
Quant Title : GC Extractables
QLast Update : Fri Sep 20 05:48:22 2024
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

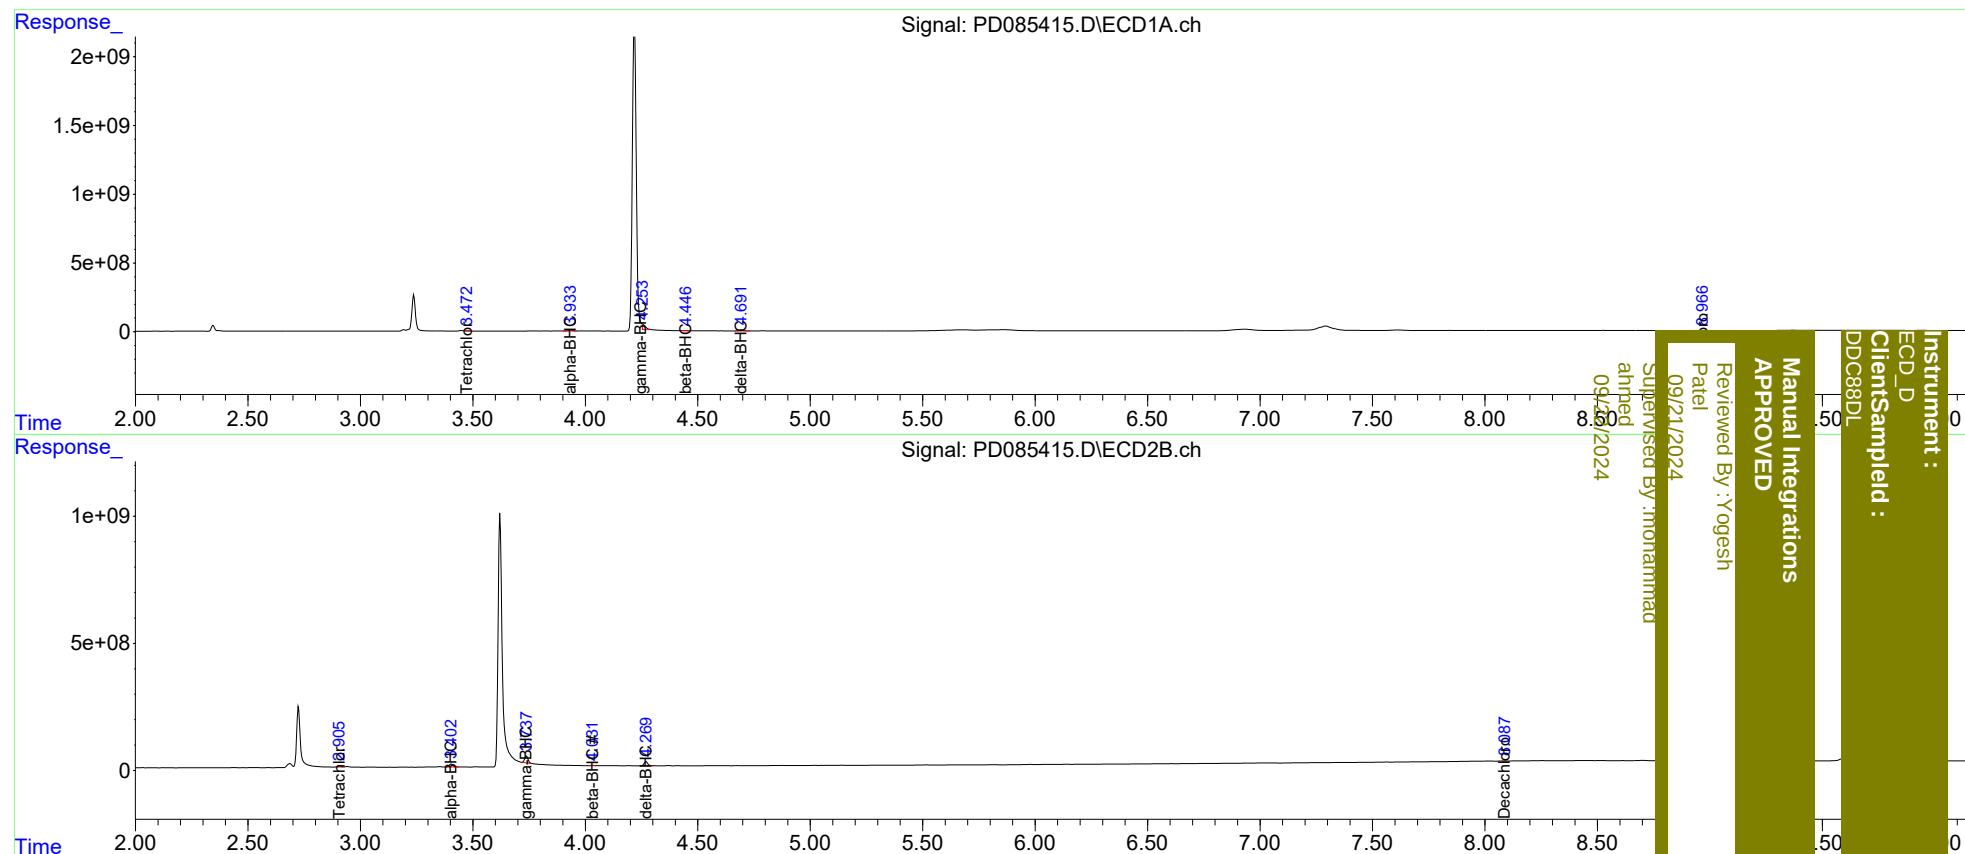

Manual Integrations
APPROVED

Reviewed By : Yogesh
Patel

09/21/2024

Supervised By : mohammad

09/20/2024

Instrument :
ECD_D
ClientSampled :
DDC88DL