

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD091925\  
 Data File : PD090349.D  
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
 Acq On : 19 Sep 2025 10:46  
 Operator : AR\AJ  
 Sample : PIBLK195  
 Misc :  
 ALS Vial : 2 Sample Multiplier: 1

Instrument :  
 ECD\_D  
 ClientSampleId :  
 PIBLK551

Integration File signal 1: autoint1.e  
 Integration File signal 2: autoint2.e  
 Quant Time: Sep 22 06:59:59 2025  
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD091725CLP.M  
 Quant Title : GC Extractables  
 QLast Update : Thu Sep 18 07:48:10 2025  
 Response via : Initial Calibration  
 Integrator: ChemStation

Volume Inj. : 1 µl  
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm


|                             | Compound        | RT#1   | RT#2   | Resp#1   | Resp#2   | ng/ml  | ng/ml  |
|-----------------------------|-----------------|--------|--------|----------|----------|--------|--------|
| -----                       |                 |        |        |          |          |        |        |
| System Monitoring Compounds |                 |        |        |          |          |        |        |
| 1)                          | SA Tetrachlo... | 3.552  | 2.875  | 50463182 | 463.4E6  | 19.359 | 20.332 |
| 27)                         | SA Decachlor... | 9.075  | 8.066  | 118.4E6  | 807.2E6  | 29.767 | 32.576 |
| Target Compounds            |                 |        |        |          |          |        |        |
| 3)                          | MA gamma-BHC... | 4.342  | 0.000  | 203062   | 0        | <MDL   | N.D. # |
| 6)                          | B beta-BHC      | 0.000  | 3.983f | 0        | 11826809 | N.D.   | 0.786  |
| 7)                          | B delta-BHC     | 4.780  | 0.000  | 939463   | 0        | 0.191  | N.D. # |
| 9)                          | A Endosulfan I  | 5.999f | 0.000  | 821769   | 0        | 0.183  | N.D. # |
| 10)                         | B trans-Chl...  | 5.999f | 0.000  | 821769   | 0        | 0.180  | N.D. # |
| 11)                         | B cis-Chlor...  | 5.999  | 0.000  | 821769   | 0        | 0.174  | N.D. # |
| 15)                         | B Endosulfa...  | 6.785  | 0.000  | 1143357  | 0        | 0.298  | N.D. # |
| -----                       |                 |        |        |          |          |        |        |


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Data\PD091925\  
Data File : PD090349.D  
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch  
Acq On : 19 Sep 2025 10:46  
Operator : AR\AJ  
Sample : PIBLK195  
Misc :  
ALS Vial : 2 Sample Multiplier: 1

Integration File signal 1: autoint1.e  
Integration File signal 2: autoint2.e  
Quant Time: Sep 22 06:59:59 2025  
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD\_D\Method\PD091725CLP.M  
Quant Title : GC Extractables  
QLast Update : Thu Sep 18 07:48:10 2025  
Response via : Initial Calibration  
Integrator: ChemStation

Volume Inj. : 1 µl  
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2  
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

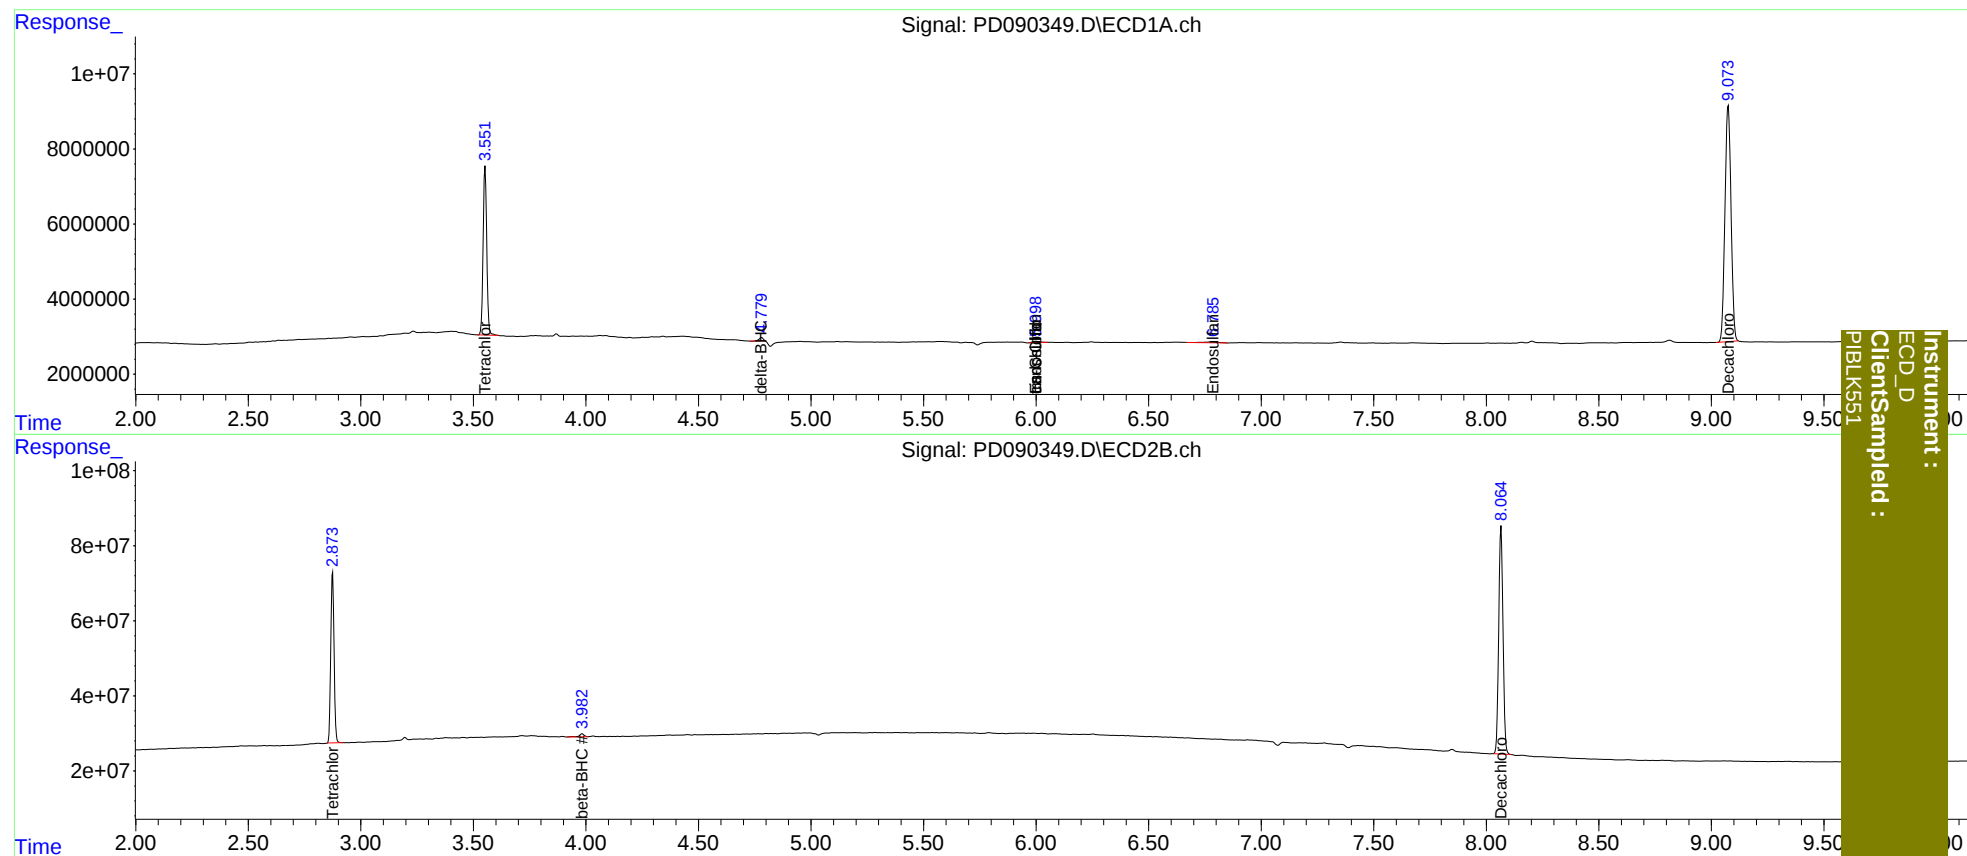


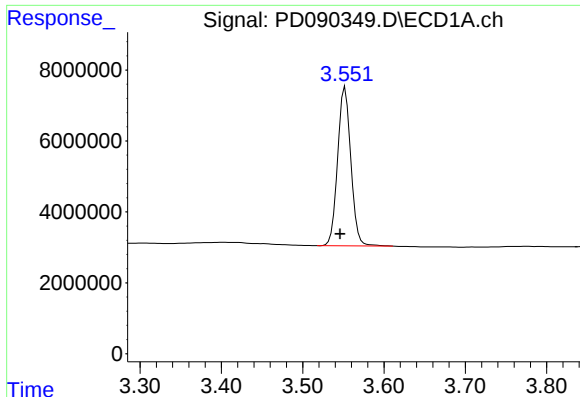

#1 Tetrachloro-m-xylene


R.T.: 3.552 min  
Delta R.T.: 0.006 min  
Response: 50463182  
Conc: 19.36 ng/ml

Instrument :  
ECD\_D  
ClientSampleId :  
PIBLK551

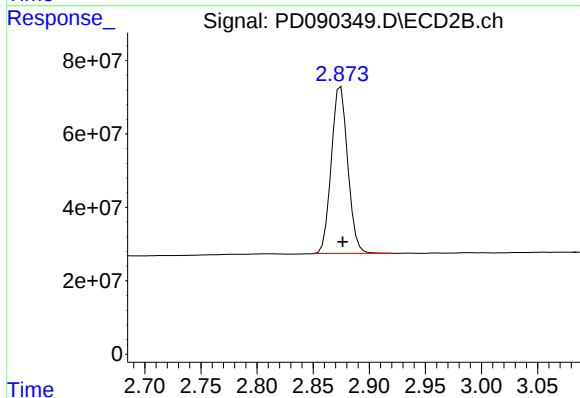


#1 Tetrachloro-m-xylene

R.T.: 2.875 min  
Delta R.T.: -0.002 min  
Response: 463416515  
Conc: 20.33 ng/ml

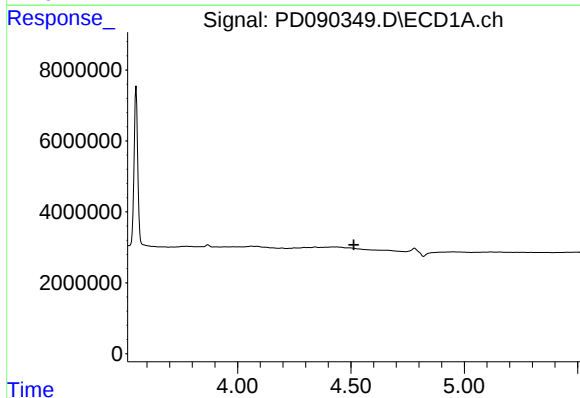


#6 beta-BHC

R.T.: 0.000 min  
Exp R.T. : 4.513 min  
Response: 0  
Conc: N.D.

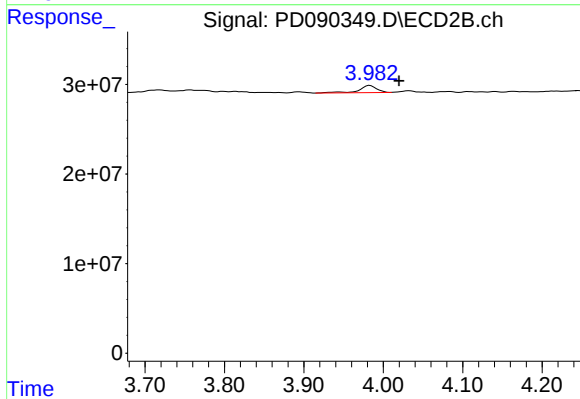

#6 beta-BHC


R.T.: 3.983 min  
Delta R.T.: -0.037 min  
Response: 11826809  
Conc: 0.79 ng/ml

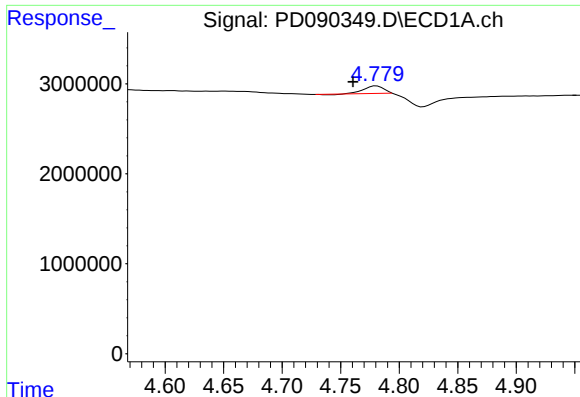

#7 delta-BHC


R.T.: 4.780 min  
Delta R.T.: 0.020 min  
Response: 939463  
Conc: 0.19 ng/ml

Instrument :  
ECD\_D  
ClientSampleId :  
PIBLK551

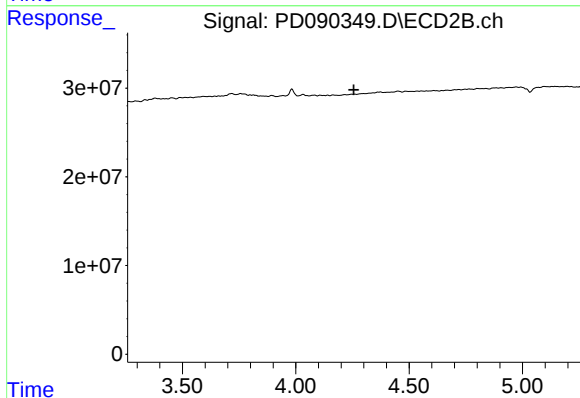


#7 delta-BHC

R.T.: 0.000 min  
Exp R.T. : 4.256 min  
Response: 0  
Conc: N.D.

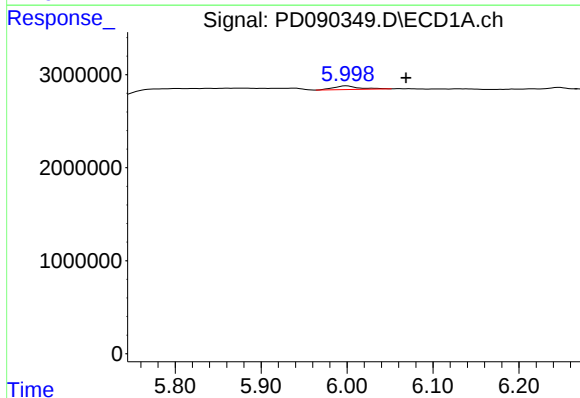


#9 Endosulfan I

R.T.: 5.999 min  
Delta R.T.: -0.070 min  
Response: 821769  
Conc: 0.18 ng/ml

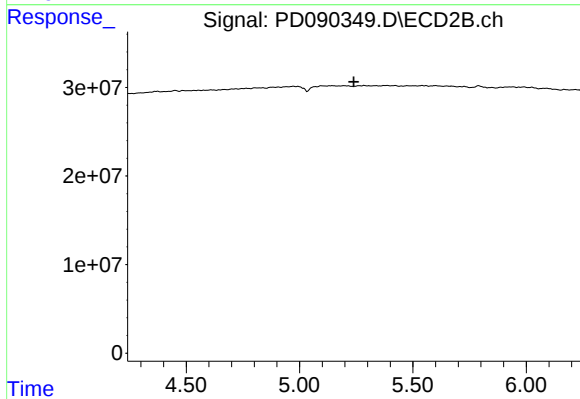

#9 Endosulfan I


R.T.: 0.000 min  
Exp R.T. : 5.240 min  
Response: 0  
Conc: N.D.

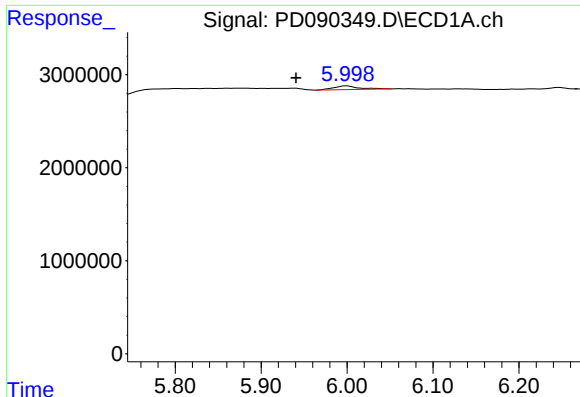

#10 trans-Chlordane


R.T.: 5.999 min  
Delta R.T.: 0.059 min  
Response: 821769  
Conc: 0.18 ng/ml

Instrument :  
ECD\_D  
ClientSampleId :  
PIBLK551

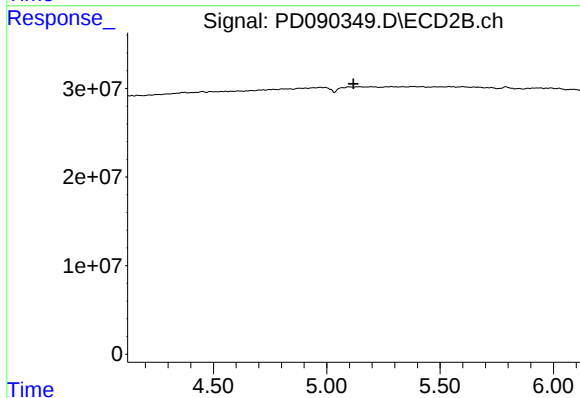


#10 trans-Chlordane

R.T.: 0.000 min  
Exp R.T. : 5.118 min  
Response: 0  
Conc: N.D.

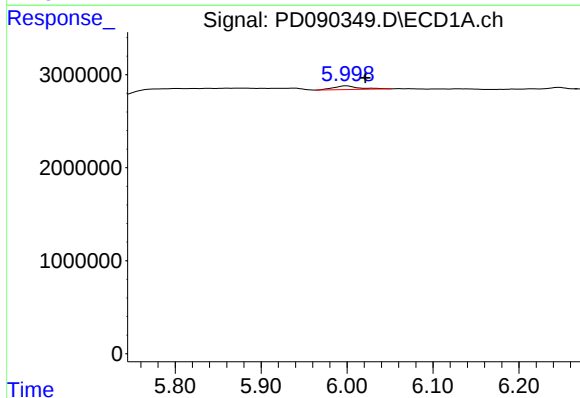


#11 cis-Chlordane

R.T.: 5.999 min  
Delta R.T.: -0.022 min  
Response: 821769  
Conc: 0.17 ng/ml

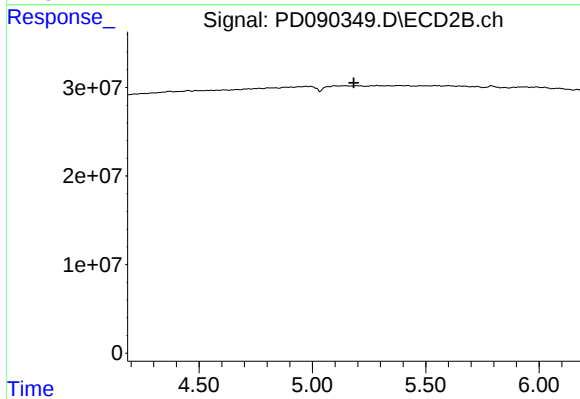

#11 cis-Chlordane


R.T.: 0.000 min  
Exp R.T. : 5.183 min  
Response: 0  
Conc: N.D.

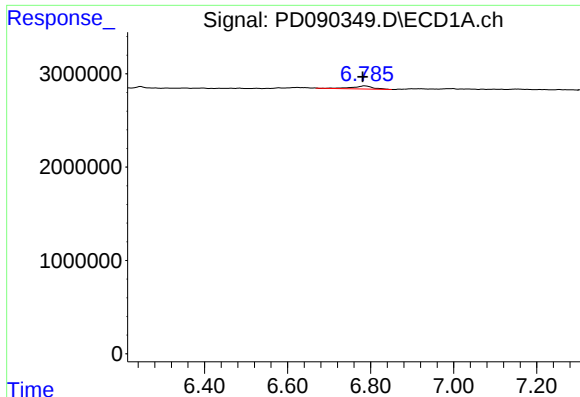

#15 Endosulfan II


R.T.: 6.785 min  
Delta R.T.: 0.004 min  
Response: 1143357  
Conc: 0.30 ng/ml

Instrument :  
ECD\_D  
ClientSampleId :  
PIBLK551

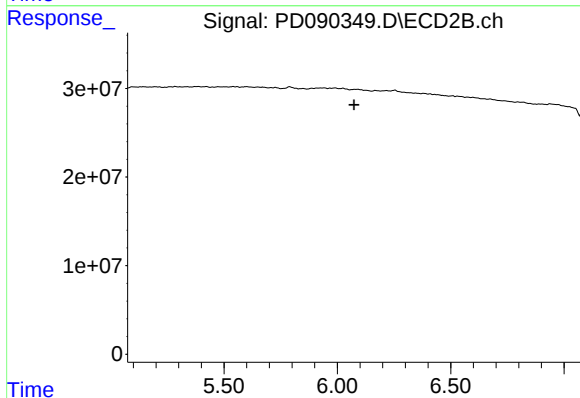


#15 Endosulfan II

R.T.: 0.000 min  
Exp R.T. : 6.073 min  
Response: 0  
Conc: N.D.

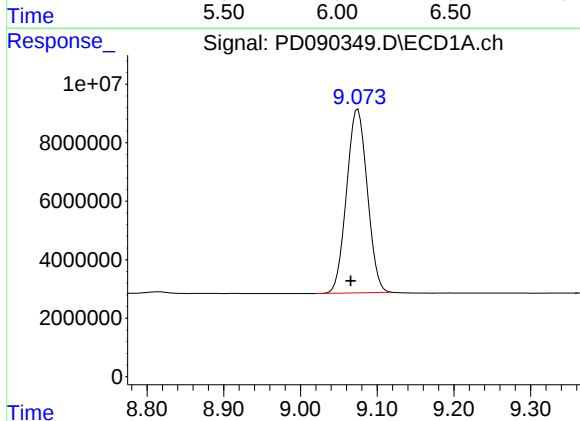

#27 Decachlorobiphenyl

R.T.: 9.075 min  
Delta R.T.: 0.009 min  
Response: 118387550  
Conc: 29.77 ng/ml

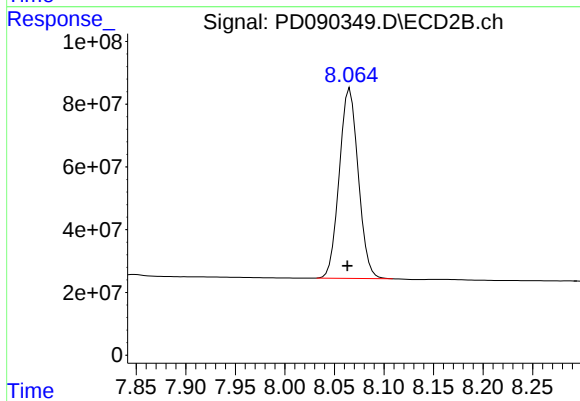

#27 Decachlorobiphenyl

R.T.: 8.066 min  
Delta R.T.: 0.002 min  
Response: 807192941  
Conc: 32.58 ng/ml