

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091925\
 Data File : PD090353.D
 Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
 Acq On : 19 Sep 2025 11:54
 Operator : AR\AJ
 Sample : PB169554BL
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 ECD_D
 ClientSampleId :
 PBLK554

Integration File signal 1: autoint1.e
 Integration File signal 2: autoint2.e
 Quant Time: Sep 22 07:00:52 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091725CLP.M
 Quant Title : GC Extractables
 QLast Update : Thu Sep 18 07:48:10 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 1 µl
 Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
 Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

	Compound	RT#1	RT#2	Resp#1	Resp#2	ng/ml	ng/ml


System Monitoring Compounds							
1)	SA Tetrachlo...	3.546	2.875	49989639	464.1E6	19.177	20.363
27)	SA Decachlor...	9.068	8.063	100.2E6	669.5E6	25.186	27.020
Target Compounds							
3)	MA gamma-BHC...	4.336	0.000	283551	0	<MDL	N.D. #
6)	B beta-BHC	0.000	3.983f	0	10319649	N.D.	0.686
7)	B delta-BHC	4.776	0.000	1442246	0	0.294	N.D. #
9)	A Endosulfan I	6.047	0.000	62357	0	<MDL	N.D. #
11)	B cis-Chlor...	6.016	0.000	817243	0	0.173	N.D. #


(f)=RT Delta > 1/2 Window (#)=Amounts differ by > 25% (m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\ECD_D\Data\PD091925\
Data File : PD090353.D
Signal(s) : Signal #1: ECD1A.ch Signal #2: ECD2B.ch
Acq On : 19 Sep 2025 11:54
Operator : AR\AJ
Sample : PB169554BL
Misc :
ALS Vial : 6 Sample Multiplier: 1

Integration File signal 1: autoint1.e
Integration File signal 2: autoint2.e
Quant Time: Sep 22 07:00:52 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\ECD_D\Method\PD091725CLP.M
Quant Title : GC Extractables
QLast Update : Thu Sep 18 07:48:10 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 1 µl
Signal #1 Phase : ZB-MR1 Signal #2 Phase: ZB-MR2
Signal #1 Info : 30M x 0.32mm x0.5 Signal #2 Info : 30M x 0.32mm x 0.25µm

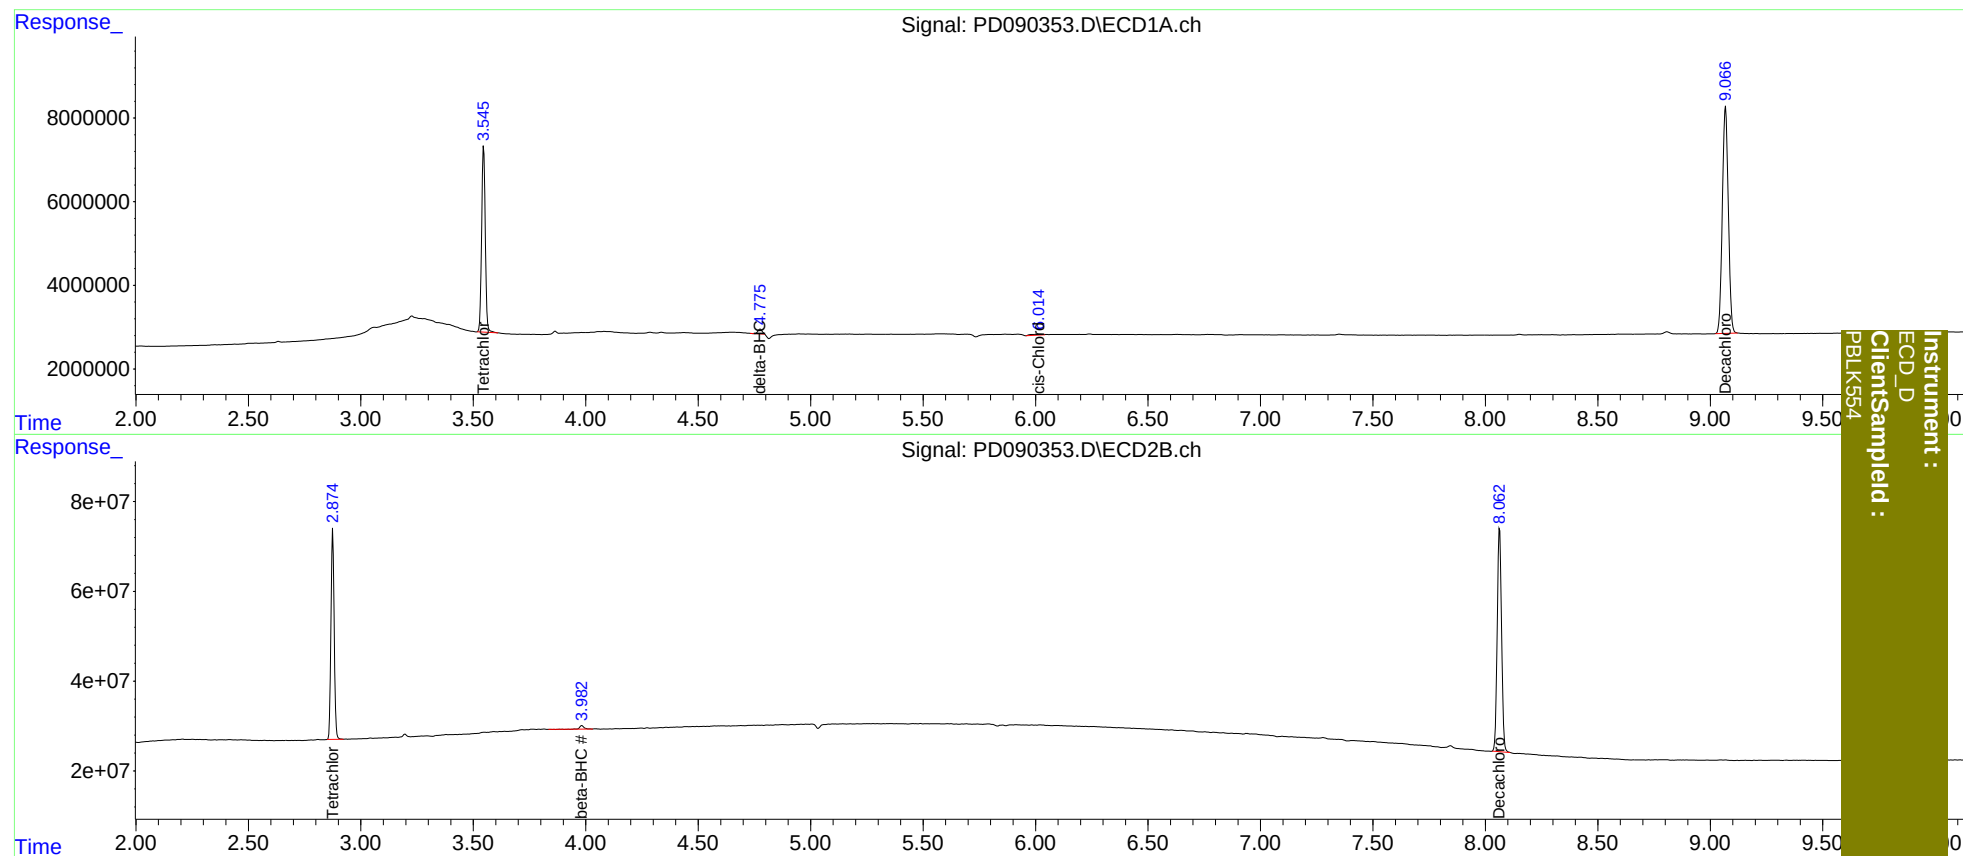


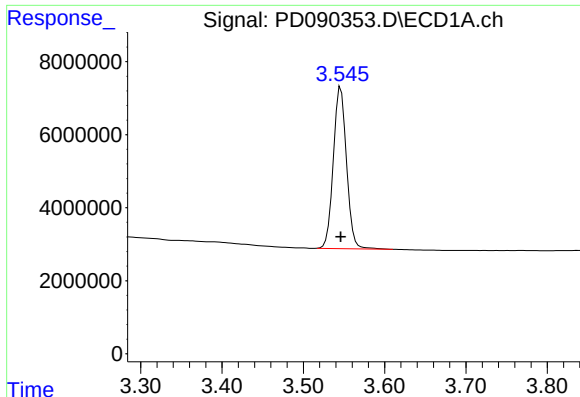

#1 Tetrachloro-m-xylene


R.T.: 3.546 min
Delta R.T.: 0.000 min
Response: 49989639
Conc: 19.18 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK554

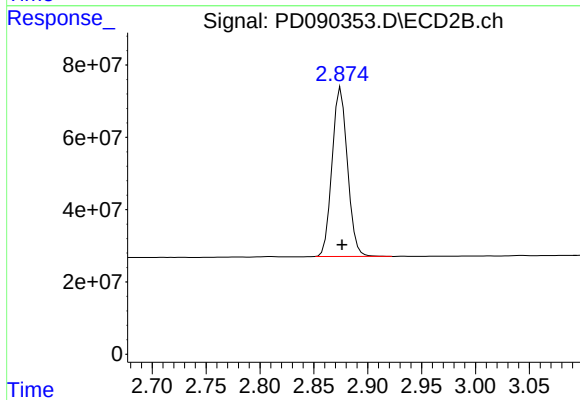


#1 Tetrachloro-m-xylene

R.T.: 2.875 min
Delta R.T.: -0.001 min
Response: 464115294
Conc: 20.36 ng/ml

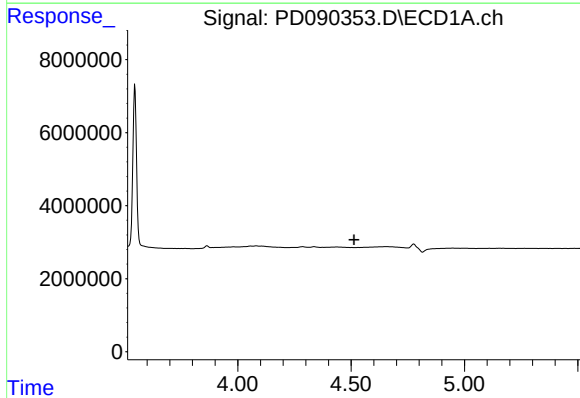


#6 beta-BHC

R.T.: 0.000 min
Exp R.T. : 4.513 min
Response: 0
Conc: N.D.

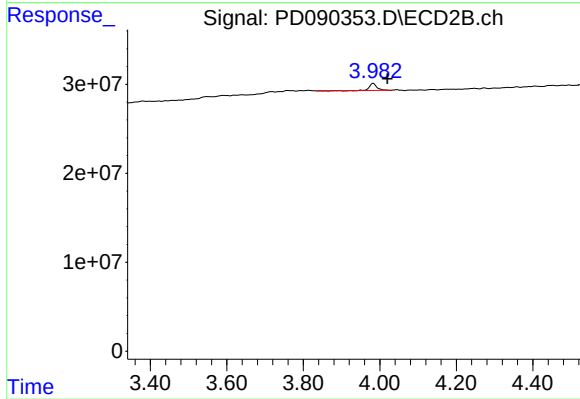

#6 beta-BHC


R.T.: 3.983 min
Delta R.T.: -0.037 min
Response: 10319649
Conc: 0.69 ng/ml

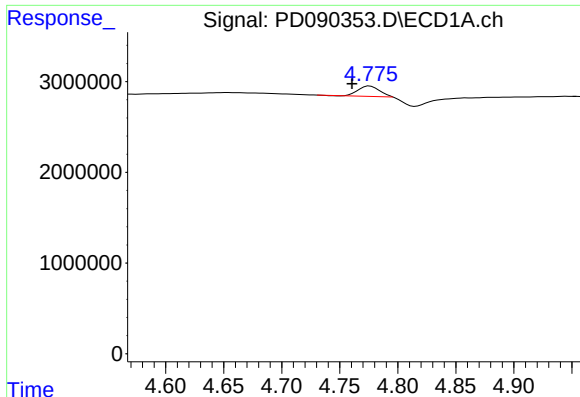

#7 delta-BHC


R.T.: 4.776 min
Delta R.T.: 0.015 min
Response: 1442246
Conc: 0.29 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK554

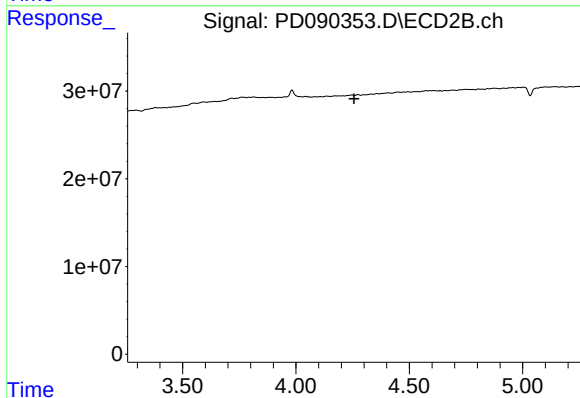


#7 delta-BHC

R.T.: 0.000 min
Exp R.T. : 4.256 min
Response: 0
Conc: N.D.

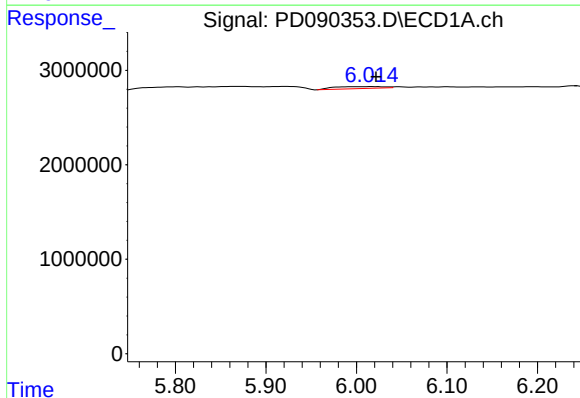


#11 cis-Chlordane

R.T.: 6.016 min
Delta R.T.: -0.005 min
Response: 817243
Conc: 0.17 ng/ml

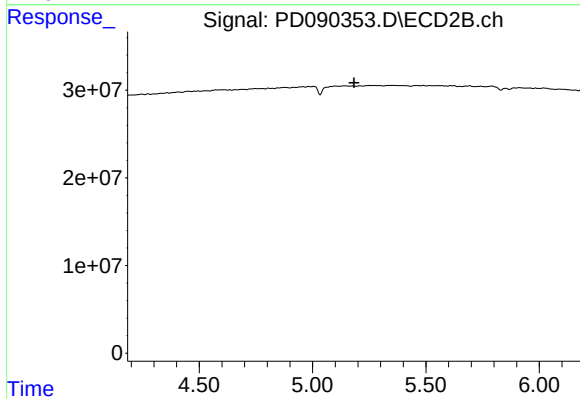

#11 cis-Chlordane


R.T.: 0.000 min
Exp R.T. : 5.183 min
Response: 0
Conc: N.D.

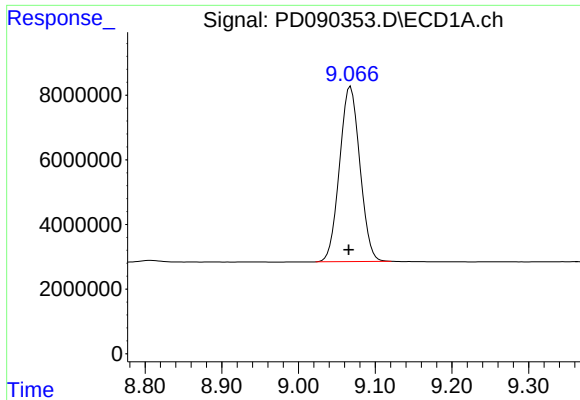

#27 Decachlorobiphenyl

R.T.: 9.068 min
Delta R.T.: 0.002 min
Response: 100169258
Conc: 25.19 ng/ml

Instrument :
ECD_D
ClientSampleId :
PBLK554

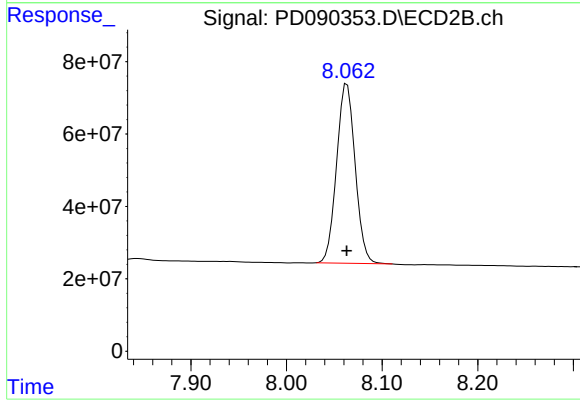

#27 Decachlorobiphenyl

R.T.: 8.063 min
Delta R.T.: 0.000 min
Response: 669525540
Conc: 27.02 ng/ml